

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
 Data File : BP007767.D
 Acq On : 28 Oct 2021 23:32
 Operator : CG/JU
 Sample : M4281-02DL 10X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFY58DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007767.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	15	19	30	rVB	255807	331008	7.65%	1.513%
2	3.811	87	89	97	rBV	10458	15781	0.36%	0.072%
3	4.111	137	140	145	rVB2	10715	16450	0.38%	0.075%
4	6.316	512	515	519	rVB6	3285	4562	0.11%	0.021%
5	6.922	611	618	624	rBV8	9375	20309	0.47%	0.093%
6	7.093	640	647	657	rVB2	20211	41926	0.97%	0.192%
7	7.258	669	675	687	rVB	62000	102750	2.37%	0.470%
8	7.458	703	709	717	rBV	63445	99951	2.31%	0.457%
9	7.928	782	789	800	rBV	828133	1283124	29.65%	5.865%
10	8.640	903	910	915	rBV	50126	83771	1.94%	0.383%
11	8.993	964	970	972	rBV6	3504	6671	0.15%	0.030%
12	9.087	978	986	995	rBV	67959	121530	2.81%	0.556%
13	9.810	1101	1109	1118	rBV2	50800	91681	2.12%	0.419%
14	10.052	1147	1150	1156	rBV8	3294	4518	0.10%	0.021%
15	10.351	1194	1201	1208	rBV	85648	150082	3.47%	0.686%
16	10.516	1221	1229	1236	rBV	31627	58684	1.36%	0.268%
17	10.734	1253	1266	1276	rBV	1110520	1900543	43.91%	8.688%
18	10.863	1278	1288	1294	rBV	75700	135511	3.13%	0.619%
19	13.545	1740	1744	1751	rVB10	3591	7340	0.17%	0.034%
20	13.975	1811	1817	1824	rBV	189704	264717	6.12%	1.210%
21	14.257	1856	1865	1874	rBV	186290	285126	6.59%	1.303%
22	14.563	1908	1917	1932	rBV	1844225	2731337	63.11%	12.485%
23	14.763	1946	1951	1956	rBV6	10288	19885	0.46%	0.091%
24	15.557	2080	2086	2095	rBV	282405	416235	9.62%	1.903%
25	15.675	2101	2106	2118	rVB2	19667	33457	0.77%	0.153%
26	15.798	2123	2127	2134	rVB10	5192	9372	0.22%	0.043%
27	16.363	2218	2223	2227	rBV7	3945	6854	0.16%	0.031%
28	16.439	2234	2236	2242	rBV7	3372	4512	0.10%	0.021%
29	17.104	2343	2349	2353	rBV2	11326	16649	0.38%	0.076%
30	17.322	2378	2386	2396	rBV	2279930	3367502	77.81%	15.394%
31	17.416	2396	2402	2416	rVB2	333959	503605	11.64%	2.302%
32	17.998	2498	2501	2506	rVB5	10821	13354	0.31%	0.061%
33	18.210	2533	2537	2542	rBV4	28551	39893	0.92%	0.182%
34	18.522	2585	2590	2595	rBV9	5889	12693	0.29%	0.058%
35	19.592	2769	2772	2776	rBV4	16398	22682	0.52%	0.104%
36	19.651	2777	2782	2787	rBV	485223	622994	14.39%	2.848%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
Data File : BP007767.D
Acq On : 28 Oct 2021 23:32
Operator : CG/JU
Sample : M4281-02DL 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY58DL

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Title : SVOA CALIBRATION

37	21.410	3075	3081	3091	rBV	3020726	4101272	94.76%	18.748%
38	23.686	3463	3468	3477	rVB2	299638	599792	13.86%	2.742%
39	23.851	3488	3496	3510	rVB2	2087521	4328001	100.00%	19.784%




Sum of corrected areas: 21876124

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
Data File : BP007767.D
Acq On : 28 Oct 2021 23:32
Operator : CG/JU
Sample : M4281-02DL 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY58DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

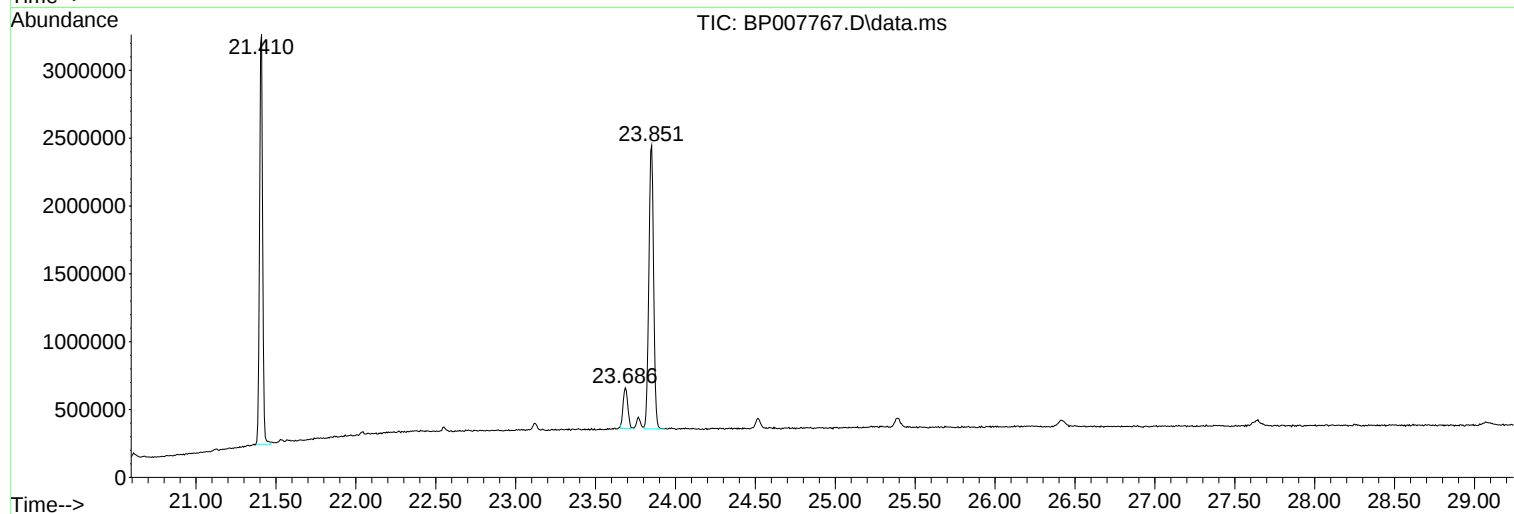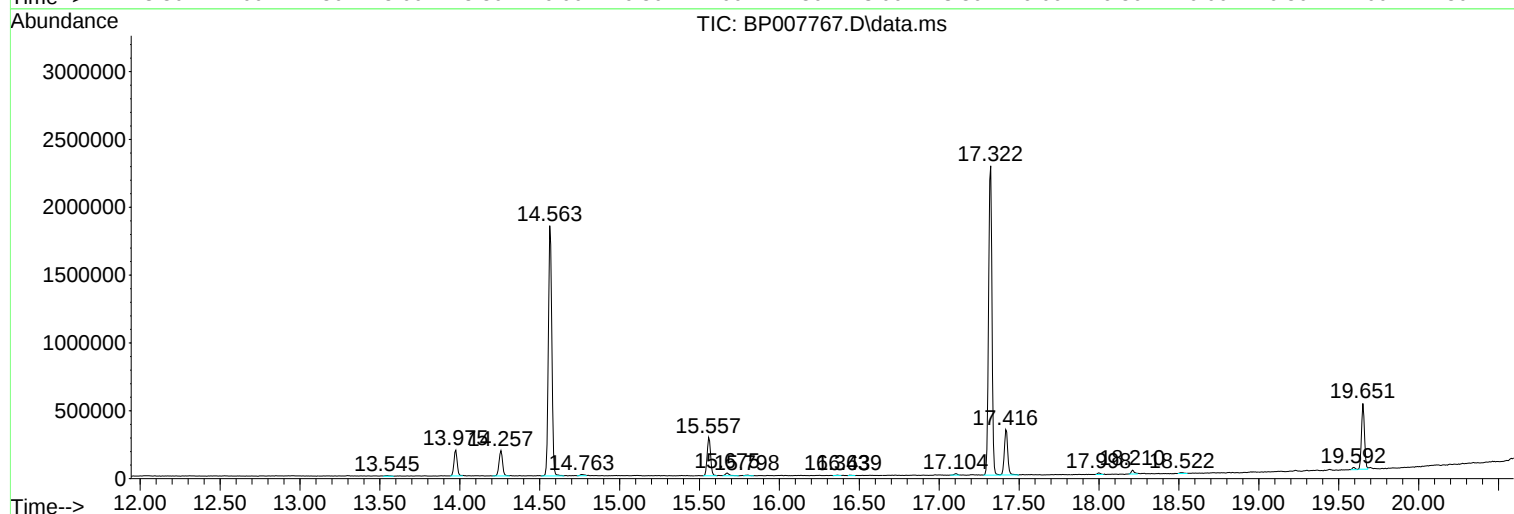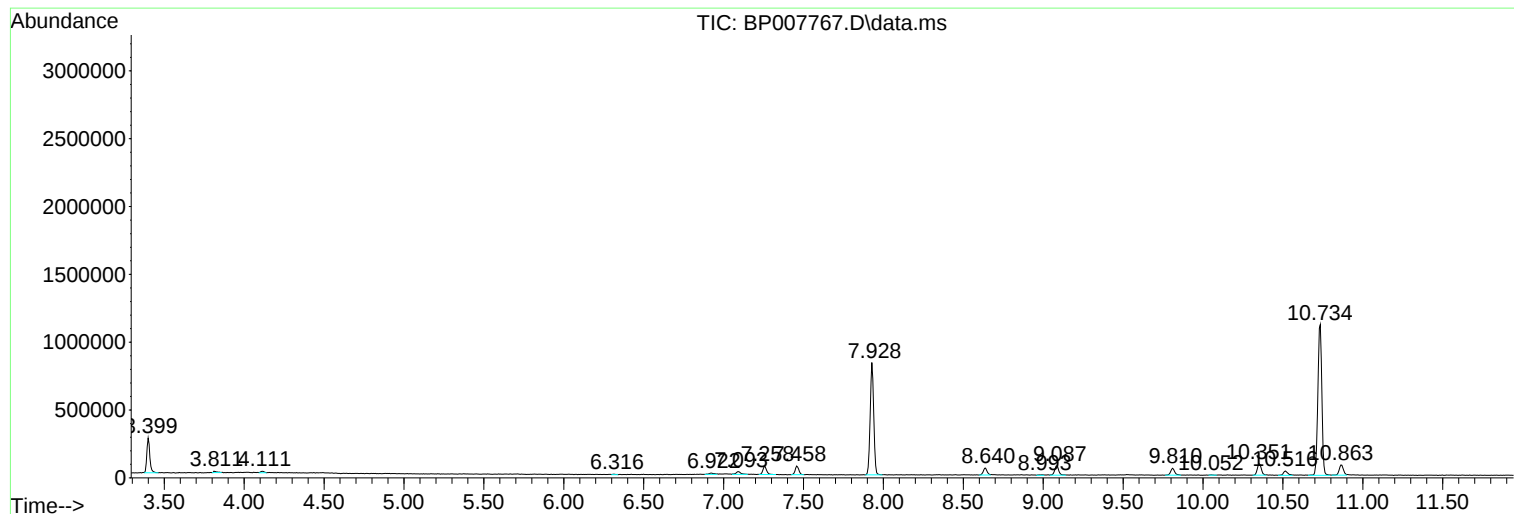

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
Data File : BP007767.D
Acq On : 28 Oct 2021 23:32
Operator : CG/JU
Sample : M4281-02DL 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY58DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
Data File : BP007767.D
Acq On : 28 Oct 2021 23:32
Operator : CG/JU
Sample : M4281-02DL 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY58DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
