

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
 Data File : BP007769.D
 Acq On : 29 Oct 2021 00:40
 Operator : CG/JU
 Sample : M4281-15DL 5X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFY73DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007769.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	4	8	13	rBV2	25780	38317	0.93%	0.160%
2	3.399	15	19	28	rVB	126109	159066	3.84%	0.665%
3	3.799	85	87	95	rBV	25935	38561	0.93%	0.161%
4	4.116	137	141	146	rVB2	12196	15700	0.38%	0.066%
5	4.887	268	272	277	rBV6	8612	14201	0.34%	0.059%
6	5.634	396	399	403	rVB6	4132	4249	0.10%	0.018%
7	6.928	614	619	621	rBV6	4247	5827	0.14%	0.024%
8	7.093	642	647	655	rVB	37509	63774	1.54%	0.266%
9	7.257	668	675	682	rBV	113552	184318	4.45%	0.770%
10	7.457	703	709	717	rBV	122310	200041	4.83%	0.836%
11	7.928	781	789	798	rBV	756461	1188230	28.71%	4.964%
12	8.640	903	910	922	rBV	97391	169720	4.10%	0.709%
13	9.087	979	986	994	rBV	130979	221609	5.36%	0.926%
14	9.216	1001	1008	1013	rBV2	17217	29686	0.72%	0.124%
15	9.539	1061	1063	1074	rVB2	5195	11026	0.27%	0.046%
16	9.810	1102	1109	1118	rBV	104001	175737	4.25%	0.734%
17	10.045	1145	1149	1153	rBV7	2844	4592	0.11%	0.019%
18	10.351	1192	1201	1217	rBV	183052	316633	7.65%	1.323%
19	10.516	1222	1229	1234	rBV2	27987	50180	1.21%	0.210%
20	10.728	1257	1265	1276	rBV	995069	1721828	41.61%	7.194%
21	10.863	1281	1288	1297	rBV	119995	211714	5.12%	0.885%
22	12.322	1528	1536	1543	rBV9	5132	11222	0.27%	0.047%
23	13.975	1811	1817	1823	rBV	358426	494649	11.95%	2.067%
24	14.104	1836	1839	1843	rVB6	2789	4610	0.11%	0.019%
25	14.257	1854	1865	1876	rBV	372207	552990	13.36%	2.310%
26	14.486	1900	1904	1908	rBV7	4316	8640	0.21%	0.036%
27	14.563	1910	1917	1929	rVB	1639037	2449925	59.20%	10.236%
28	14.763	1945	1951	1956	rBV4	24484	44195	1.07%	0.185%
29	15.110	2006	2010	2014	rVB7	3764	6177	0.15%	0.026%
30	15.222	2028	2029	2034	rVB5	4448	4219	0.10%	0.018%
31	15.380	2050	2056	2059	rBV4	7818	11981	0.29%	0.050%
32	15.557	2078	2086	2099	rBV	532618	769606	18.60%	3.215%
33	15.674	2099	2106	2115	rBV2	48485	78779	1.90%	0.329%
34	15.798	2123	2127	2133	rBV5	6844	12073	0.29%	0.050%
35	16.127	2177	2183	2185	rBV6	2339	4904	0.12%	0.020%
36	16.986	2324	2329	2335	rBV8	6128	14399	0.35%	0.060%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
 Data File : BP007769.D
 Acq On : 29 Oct 2021 00:40
 Operator : CG/JU
 Sample : M4281-15DL 5X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFY73DL

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	17.033	2335	2337	2343	rVB7	3183	5136	0.12%	0.021%
38	17.104	2343	2349	2353	rBV2	10453	22044	0.53%	0.092%
39	17.321	2379	2386	2395	rBV	2064896	3020996	73.00%	12.622%
40	17.416	2396	2402	2412	rVV	606639	882780	21.33%	3.688%
41	17.998	2498	2501	2505	rVB6	11656	14955	0.36%	0.062%
42	18.210	2532	2537	2542	rBV6	31838	47944	1.16%	0.200%
43	19.592	2770	2772	2776	rBV3	18223	16302	0.39%	0.068%
44	19.651	2777	2782	2788	rBV	880492	1119280	27.05%	4.676%
45	21.409	3075	3081	3093	rBV	2983592	3936906	95.13%	16.448%
46	23.686	3462	3468	3476	rVB2	614251	1182575	28.58%	4.941%
47	23.768	3479	3482	3488	rVV	153948	254579	6.15%	1.064%
48	23.850	3488	3496	3508	rVB2	2020197	4138345	100.00%	17.290%




Sum of corrected areas: 23935220

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
Data File : BP007769.D
Acq On : 29 Oct 2021 00:40
Operator : CG/JU
Sample : M4281-15DL 5X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY73DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

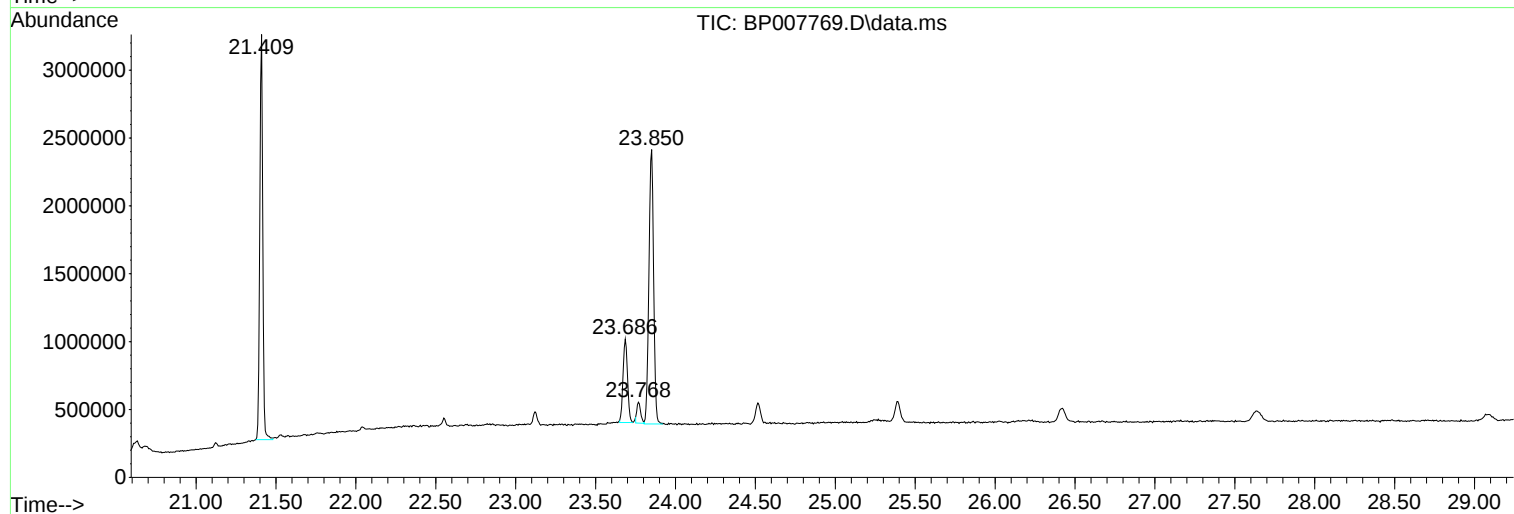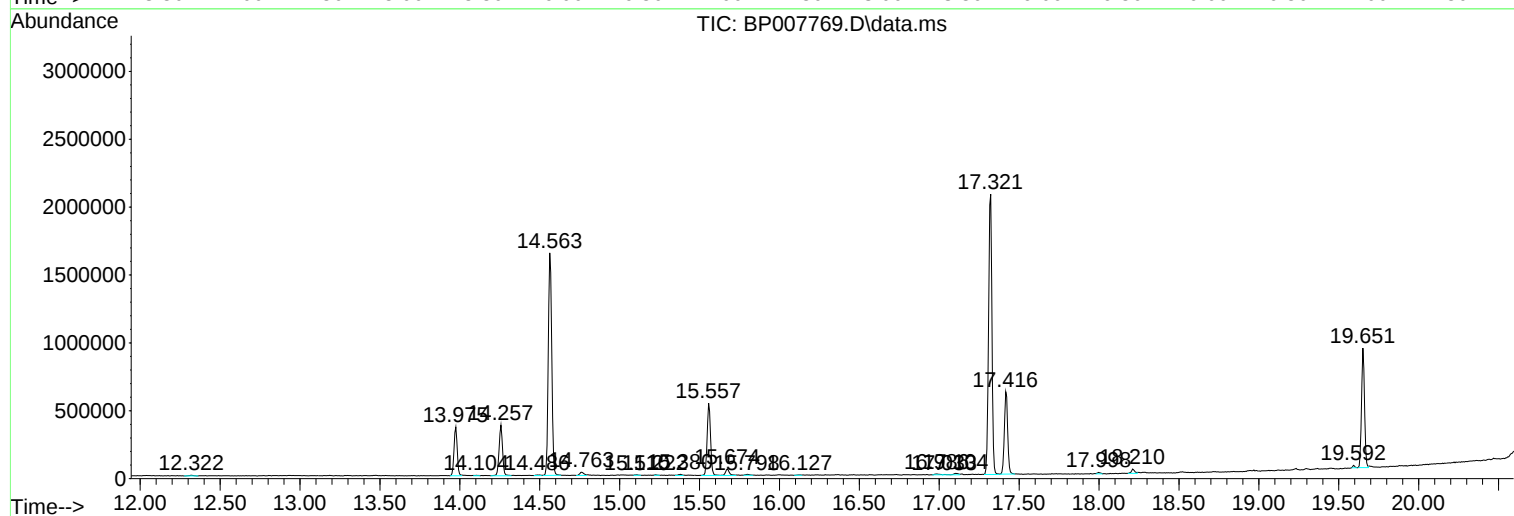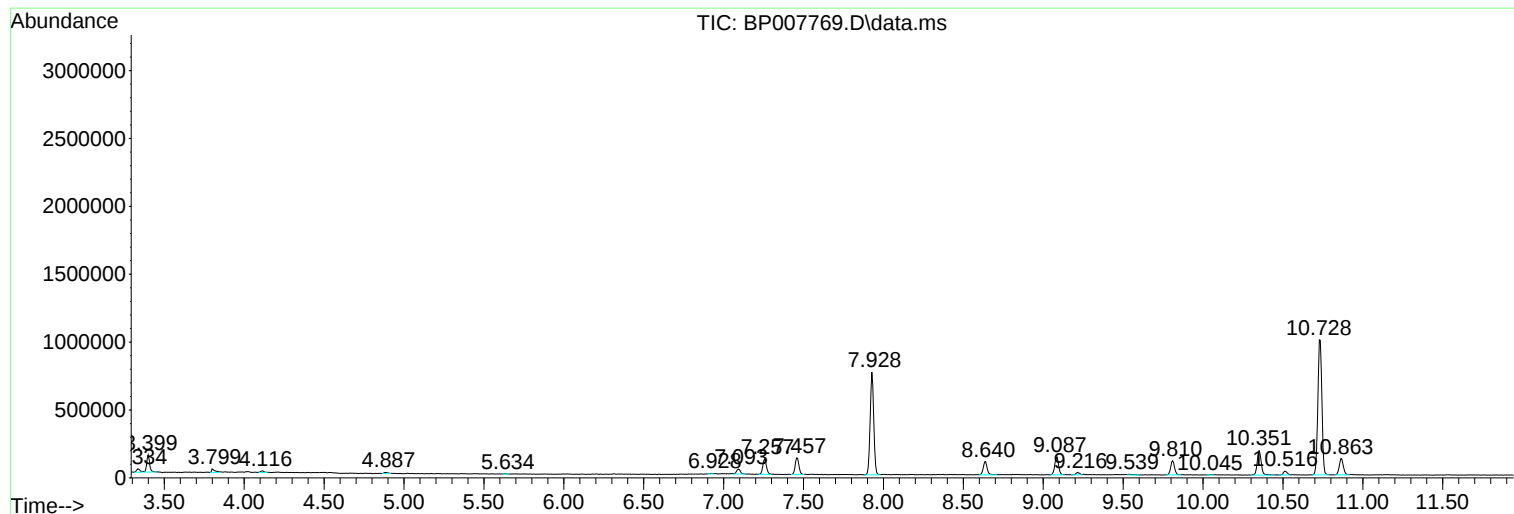

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
Data File : BP007769.D
Acq On : 29 Oct 2021 00:40
Operator : CG/JU
Sample : M4281-15DL 5X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY73DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102821\
Data File : BP007769.D
Acq On : 29 Oct 2021 00:40
Operator : CG/JU
Sample : M4281-15DL 5X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY73DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
