

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102921\
 Data File : BP007782.D
 Acq On : 29 Oct 2021 13:33
 Operator : CG/JU
 Sample : M4282-07DL 2X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFY76DL

Quant Time: Oct 29 14:08:30 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 27 15:37:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.928	152	190710	20.000	ng/u1	0.00
20) Naphthalene-d8	10.734	136	750656	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.569	164	498052	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.322	188	1127310	20.000	ng/u1	0.00
79) Chrysene-d12	21.416	240	1295054	20.000	ng/u1	0.00
88) Perylene-d12	23.863	264	1363496	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.376	96	3794	0.904	ng/uL	0.00
4) Pyridine-d5	3.799	84	41352	3.257	ng/u1	0.02
7) Phenol-d5	7.093	99	72957	5.037	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.258	67	118927	14.788	ng/u1	0.00
11) 2-Chlorophenol-d4	7.464	132	160923	14.284	ng/u1	0.00
15) 4-Methylphenol-d8	8.640	113	117450	10.355	ng/u1	0.00
21) Nitrobenzene-d5	9.087	128	78019	15.251	ng/u1	0.00
24) 2-Nitrophenol-d4	9.811	143	84083	15.049	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.358	165	164834	14.494	ng/u1	0.00
31) 4-Chloroaniline-d4	10.869	131	184039	12.239	ng/u1	0.00
46) Dimethylphthalate-d6	13.981	166	523783	15.526	ng/u1	0.00
49) Acenaphthylene-d8	14.263	160	587290	14.203	ng/u1	0.00
54) 4-Nitrophenol-d4	14.763	143	18597	3.007	ng/u1	0.00
60) Fluorene-d10	15.563	176	456147	16.038	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.681	200	41433	6.871	ng/u1	0.00
73) Anthracene-d10	17.422	188	817064	17.637	ng/u1	0.00
81) Pyrene-d10	19.657	212	1047420	17.372	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.704	264	1102861	16.465	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.405	88	86381	18.404	ng/uL 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102921\
Data File : BP007782.D
Acq On : 29 Oct 2021 13:33
Operator : CG/JU
Sample : M4282-07DL 2X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY76DL

Quant Time: Oct 29 14:08:30 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 27 15:37:43 2021
Response via : Initial Calibration

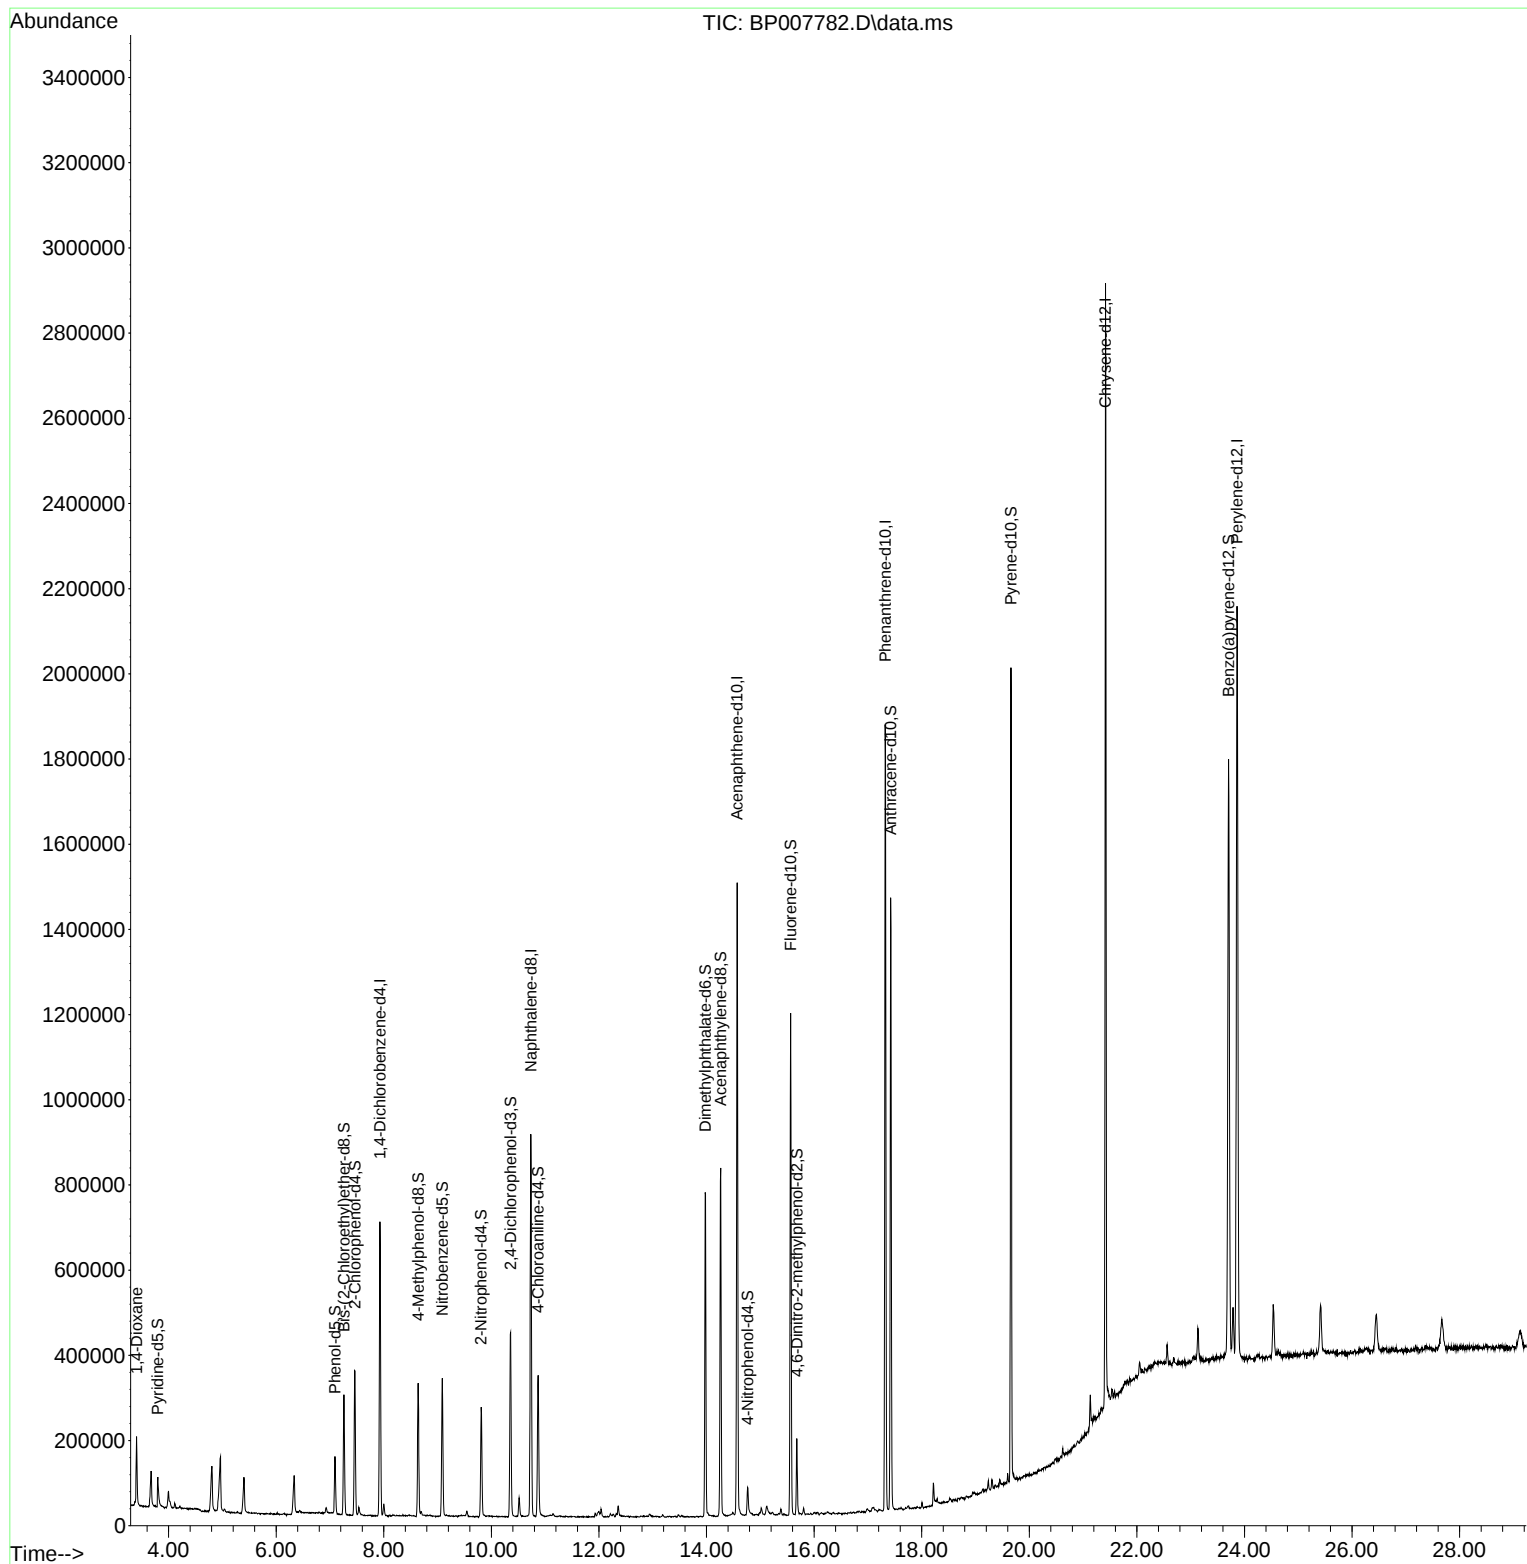

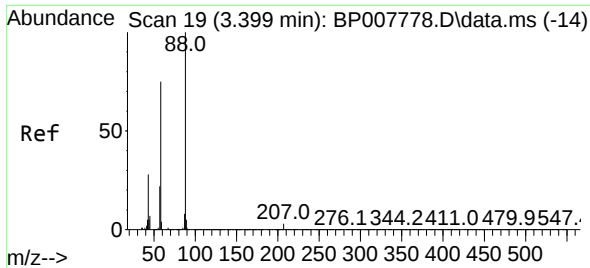

#2
 1,4-Dioxane
 Concen: 18.404 ng/uL
 RT: 3.405 min Scan# 20
 Delta R.T. 0.006 min
 Lab File: BP007782.D
 Acq: 29 Oct 2021 13:33

Instrument :
 BNA_P
 ClientSampleId :
 BFY76DL

Tgt Ion:	88	Resp:	86381
Ion	Ratio	Lower	Upper
88	100		
43	26.2	24.2	36.2
58	68.4	62.5	93.7

