

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102921\
 Data File : BP007779.D
 Acq On : 29 Oct 2021 11:05
 Operator : CG/JU
 Sample : PB140099BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK099

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007779.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	10	13	19	rVB	39240	49206	1.13%	0.123%
2	3.781	81	84	98	rBV	508060	751573	17.23%	1.872%
3	4.111	137	140	146	rVB2	10062	15726	0.36%	0.039%
4	7.093	640	647	659	rVB	586949	909160	20.84%	2.265%
5	7.258	669	675	688	rVB	448137	692750	15.88%	1.726%
6	7.458	702	709	718	rBV	585483	935323	21.44%	2.330%
7	7.928	779	789	800	rBV	623046	972890	22.30%	2.424%
8	8.640	902	910	921	rBV	689833	1116494	25.60%	2.782%
9	9.087	976	986	996	rBV	516168	832897	19.09%	2.075%
10	9.810	1101	1109	1118	rBV	407165	680020	15.59%	1.694%
11	10.351	1191	1201	1211	rBV	658750	1106911	25.38%	2.758%
12	10.734	1259	1266	1276	rVB	782583	1313590	30.11%	3.273%
13	10.869	1281	1289	1302	rBV	627746	1095113	25.11%	2.728%
14	12.004	1477	1482	1485	rBV7	4815	8805	0.20%	0.022%
15	12.322	1531	1536	1542	rVB2	14341	21655	0.50%	0.054%
16	12.957	1639	1644	1650	rBV9	4206	9629	0.22%	0.024%
17	13.540	1737	1743	1747	rBV9	4154	8258	0.19%	0.021%
18	13.981	1811	1818	1824	rBV	1251190	1775723	40.71%	4.424%
19	14.263	1857	1866	1877	rBV	1269106	1907305	43.73%	4.752%
20	14.428	1893	1894	1901	rVB6	3097	4822	0.11%	0.012%
21	14.498	1901	1906	1910	rBV8	5332	10567	0.24%	0.026%
22	14.569	1910	1918	1928	rVV	1221260	1807566	41.44%	4.503%
23	14.763	1941	1951	1963	rBV	585002	894077	20.50%	2.228%
24	15.228	2025	2030	2036	rBV9	7880	12918	0.30%	0.032%
25	15.563	2079	2087	2099	rBV	1822466	2585366	59.27%	6.441%
26	15.681	2100	2107	2117	rBV	387737	551830	12.65%	1.375%
27	15.804	2123	2128	2134	rVB2	23308	36434	0.84%	0.091%
28	16.245	2198	2203	2206	rVB6	3290	5464	0.13%	0.014%
29	16.992	2324	2330	2332	rBV6	7911	12384	0.28%	0.031%
30	17.110	2344	2350	2353	rBV3	6927	12444	0.29%	0.031%
31	17.210	2363	2367	2369	rBV5	5439	6367	0.15%	0.016%
32	17.328	2380	2387	2397	rBV	1549394	2295291	52.62%	5.719%
33	17.422	2397	2403	2417	rVB	2099780	3060222	70.16%	7.624%
34	17.704	2447	2451	2454	rBV6	4659	5838	0.13%	0.015%
35	18.051	2506	2510	2512	rBV4	2739	4598	0.11%	0.011%
36	18.216	2534	2538	2543	rBV8	4446	10171	0.23%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102921\
 Data File : BP007779.D
 Acq On : 29 Oct 2021 11:05
 Operator : CG/JU
 Sample : PB140099BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK099

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	18.722	2622	2624	2629	rBV6	3672	4601	0.11%	0.011%
38	19.233	2708	2711	2718	rVB3	30848	44640	1.02%	0.111%
39	19.304	2720	2723	2728	rVB	27968	37154	0.85%	0.093%
40	19.598	2771	2773	2777	rVB4	13799	13823	0.32%	0.034%
41	19.657	2777	2783	2795	rBV	2856294	3897805	89.36%	9.711%
42	21.416	3077	3082	3095	rBV	2315157	2972488	68.15%	7.406%
43	23.704	3464	3471	3479	rBV	2236910	4361969	100.00%	10.867%
44	23.863	3491	3498	3513	rVB2	1546951	3285904	75.33%	8.187%




Sum of corrected areas: 40137771

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102921\
Data File : BP007779.D
Acq On : 29 Oct 2021 11:05
Operator : CG/JU
Sample : PB140099BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK099

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

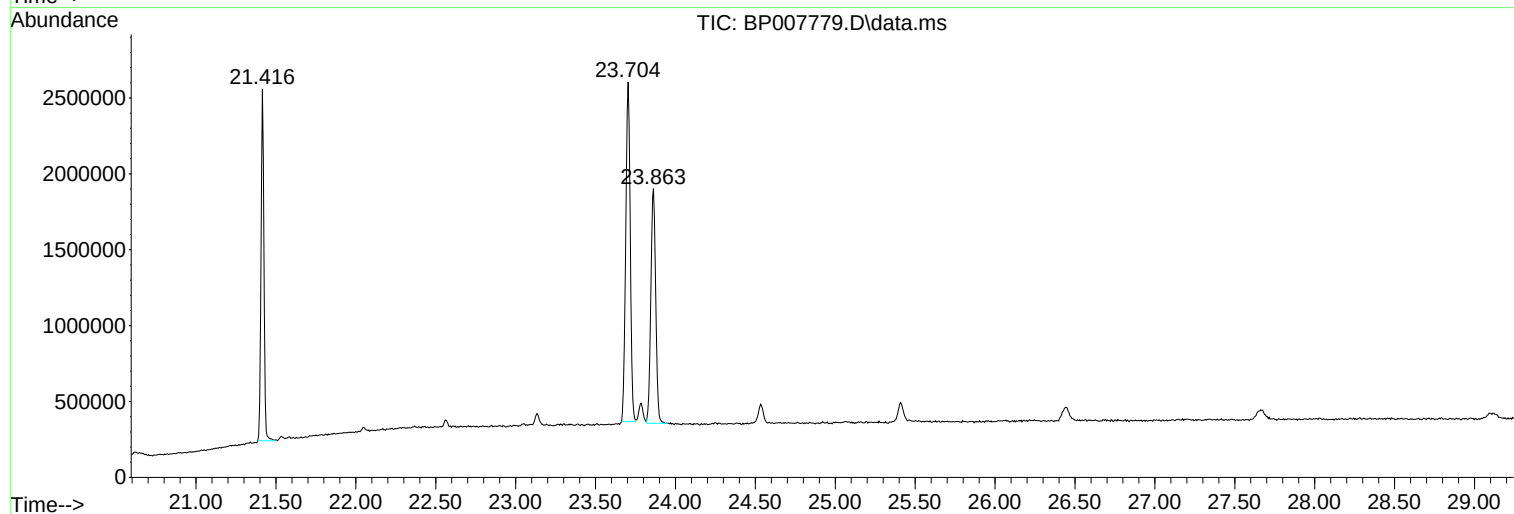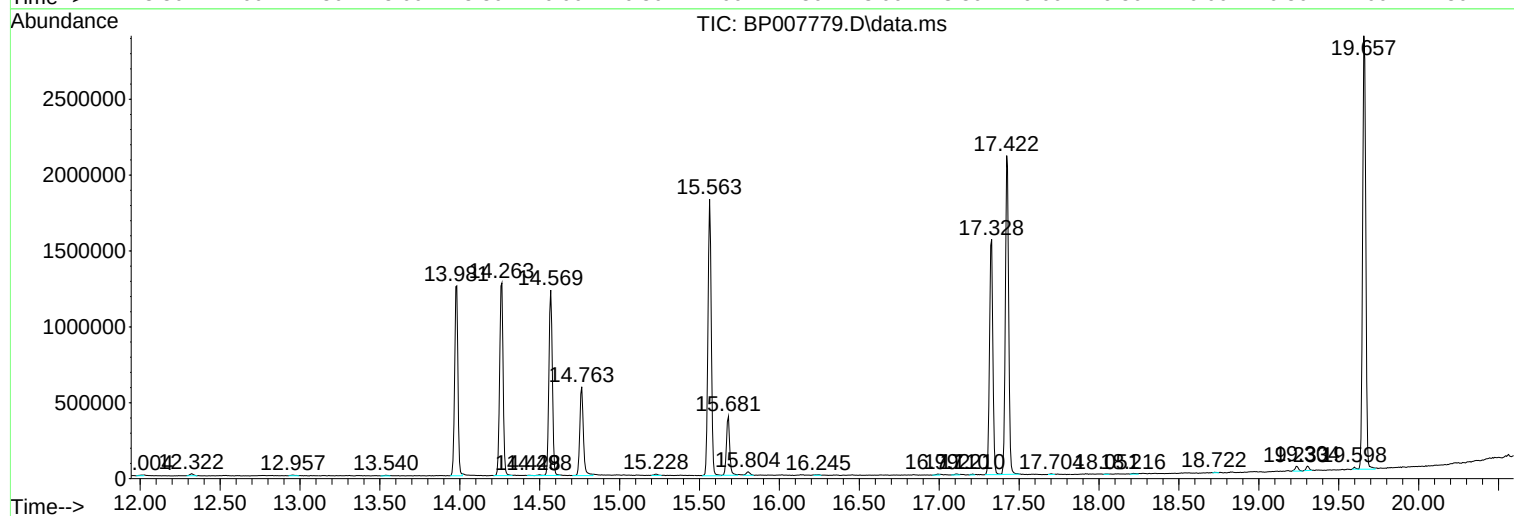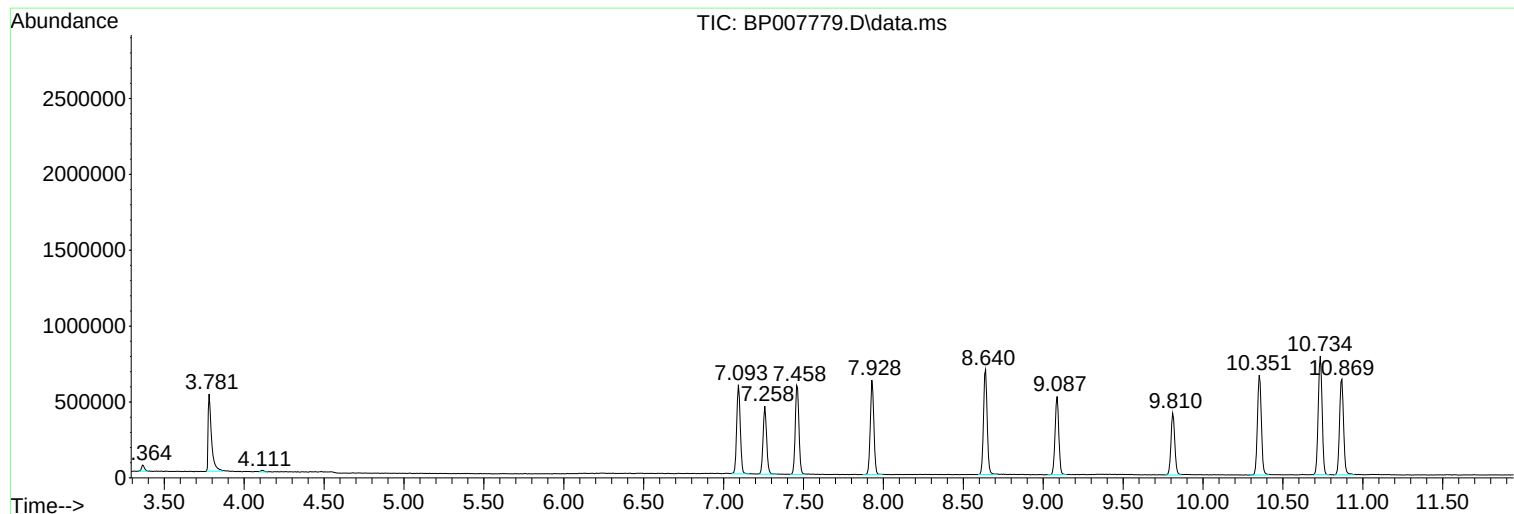

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102921\
Data File : BP007779.D
Acq On : 29 Oct 2021 11:05
Operator : CG/JU
Sample : PB140099BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK099

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102921\
Data File : BP007779.D
Acq On : 29 Oct 2021 11:05
Operator : CG/JU
Sample : PB140099BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK099

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
