

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102921\
 Data File : BP007785.D
 Acq On : 29 Oct 2021 16:28
 Operator : CG/JU
 Sample : M4282-19DL 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFYA0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007785.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	15	19	28	rVB	122367	159408	4.32%	0.805%
2	3.811	88	89	91	rBV	10258	8490	0.23%	0.043%
3	4.105	136	139	145	rVB3	10525	16571	0.45%	0.084%
4	5.858	433	437	439	rBV5	2627	4140	0.11%	0.021%
5	6.322	512	516	519	rVB6	3493	4965	0.13%	0.025%
6	6.369	519	524	528	rBV8	6327	11387	0.31%	0.057%
7	7.099	643	648	653	rVB	28154	43761	1.19%	0.221%
8	7.258	669	675	682	rVB	95237	152839	4.14%	0.772%
9	7.463	702	710	718	rBV	98743	173135	4.69%	0.874%
10	7.928	782	789	798	rBV	695909	1072655	29.05%	5.416%
11	8.640	903	910	917	rBV	75750	133063	3.60%	0.672%
12	9.087	980	986	993	rBV	105722	174438	4.72%	0.881%
13	9.434	1043	1045	1048	rVV4	2818	3847	0.10%	0.019%
14	9.505	1052	1057	1058	rVV5	3411	5285	0.14%	0.027%
15	9.534	1060	1062	1068	rVB7	3212	5576	0.15%	0.028%
16	9.810	1101	1109	1118	rBV2	71730	129334	3.50%	0.653%
17	10.357	1195	1202	1214	rBV	126611	221036	5.99%	1.116%
18	10.516	1225	1229	1231	rBV4	7099	8553	0.23%	0.043%
19	10.734	1259	1266	1274	rBV	894481	1459271	39.52%	7.369%
20	10.869	1282	1289	1298	rBV	92198	163968	4.44%	0.828%
21	11.093	1326	1327	1334	rVB7	4097	6730	0.18%	0.034%
22	11.857	1454	1457	1460	rVB5	2915	4117	0.11%	0.021%
23	11.969	1472	1476	1480	rBV6	3130	5444	0.15%	0.027%
24	12.322	1531	1536	1540	rBV8	3372	5999	0.16%	0.030%
25	12.946	1636	1642	1643	rBV6	6029	10800	0.29%	0.055%
26	13.540	1738	1743	1747	rVB7	2569	4253	0.12%	0.021%
27	13.981	1812	1818	1823	rBV	259784	362425	9.82%	1.830%
28	14.022	1823	1825	1829	rVB5	6286	8029	0.22%	0.041%
29	14.263	1859	1866	1876	rBV	259322	389565	10.55%	1.967%
30	14.487	1898	1904	1908	rBV3	12292	24234	0.66%	0.122%
31	14.569	1910	1918	1930	rVB	1362867	1994441	54.01%	10.071%
32	14.769	1948	1952	1958	rBV4	17971	31331	0.85%	0.158%
33	15.028	1992	1996	2000	rBV3	6532	8977	0.24%	0.045%
34	15.104	2005	2009	2015	rBV4	5521	9476	0.26%	0.048%
35	15.392	2055	2058	2062	rVB5	6164	7210	0.20%	0.036%
36	15.563	2081	2087	2098	rVV	409950	597235	16.17%	3.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102921\
 Data File : BP007785.D
 Acq On : 29 Oct 2021 16:28
 Operator : CG/JU
 Sample : M4282-19DL 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFYA0DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	15.681	2102	2107	2114	rVB2	35596	56784	1.54%	0.287%
38	15.810	2124	2129	2132	rBV5	5280	7879	0.21%	0.040%
39	16.010	2157	2163	2169	rVB5	3634	7881	0.21%	0.040%
40	16.534	2249	2252	2256	rVB6	2701	4362	0.12%	0.022%
41	16.851	2301	2306	2308	rVV6	3910	5924	0.16%	0.030%
42	16.939	2319	2321	2324	rBV4	2810	4129	0.11%	0.021%
43	16.986	2324	2329	2333	rVV2	11035	18523	0.50%	0.094%
44	17.110	2346	2350	2353	rBV3	7828	10874	0.29%	0.055%
45	17.139	2353	2355	2359	rVV4	6724	8137	0.22%	0.041%
46	17.210	2363	2367	2373	rBV9	7250	11546	0.31%	0.058%
47	17.328	2380	2387	2397	rBV	1723335	2497292	67.63%	12.610%
48	17.428	2397	2404	2416	rVB	484441	726230	19.67%	3.667%
49	17.645	2439	2441	2446	rVB5	3248	5478	0.15%	0.028%
50	17.698	2446	2450	2452	rBV5	3559	5188	0.14%	0.026%
51	18.004	2499	2502	2504	rBV4	5925	6768	0.18%	0.034%
52	18.216	2535	2538	2547	rBV9	19303	37252	1.01%	0.188%
53	18.281	2547	2549	2554	rVB6	4572	6002	0.16%	0.030%
54	18.722	2622	2624	2627	rBV4	5054	5047	0.14%	0.025%
55	18.945	2659	2662	2666	rBV3	13415	22120	0.60%	0.112%
56	19.316	2721	2725	2727	rBV2	9330	10180	0.28%	0.051%
57	19.598	2770	2773	2777	rBV5	13193	19301	0.52%	0.097%
58	19.663	2778	2784	2789	rBV	666630	911693	24.69%	4.604%
59	21.416	3077	3082	3089	rBV	2392704	3288763	89.07%	16.607%
60	23.704	3466	3471	3479	rVB2	513233	1012114	27.41%	5.111%
61	23.863	3491	3498	3514	rVB2	1705691	3692530	100.00%	18.645%




Sum of corrected areas: 19803985

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102921\
Data File : BP007785.D
Acq On : 29 Oct 2021 16:28
Operator : CG/JU
Sample : M4282-19DL 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFYA0DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

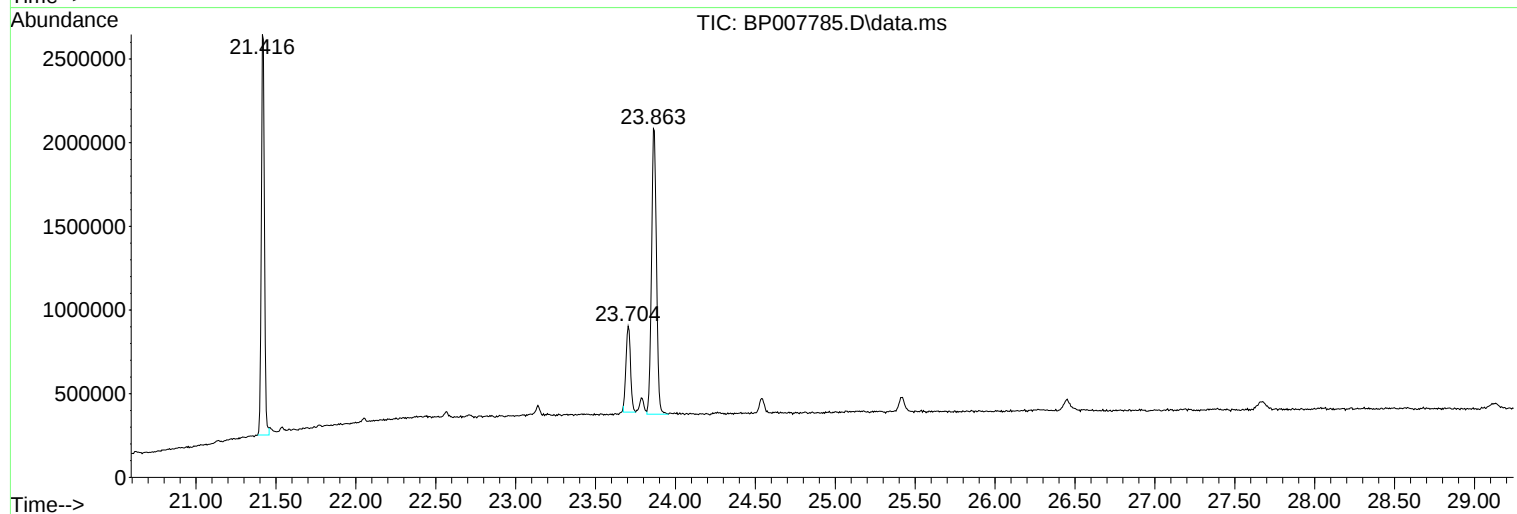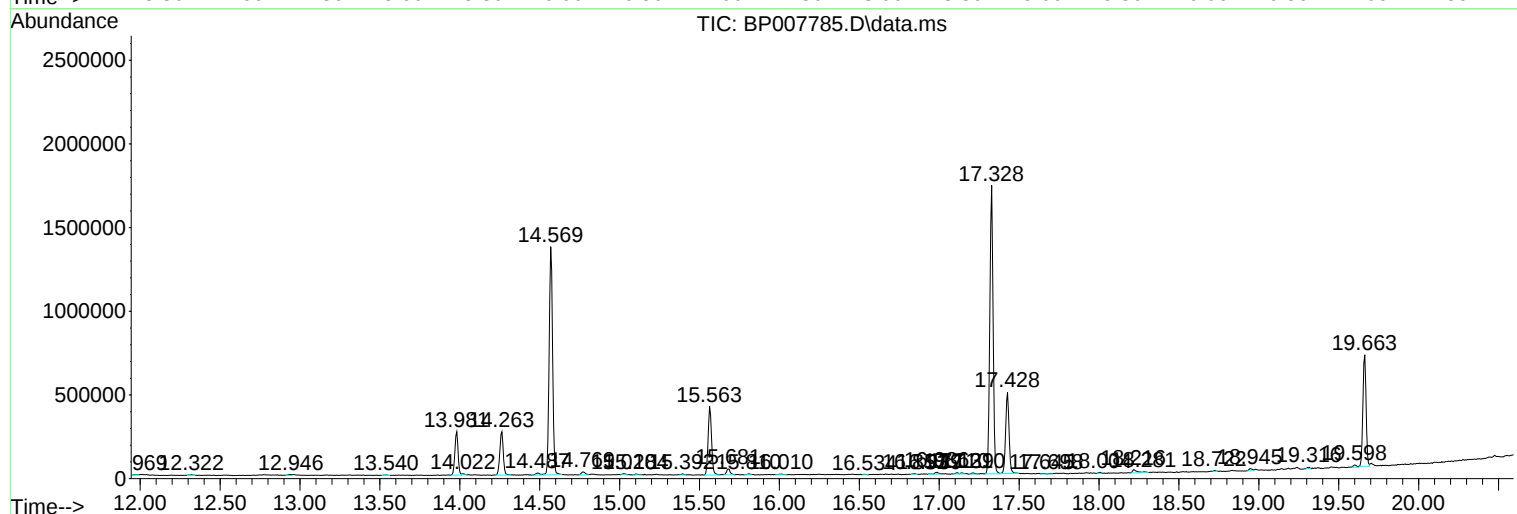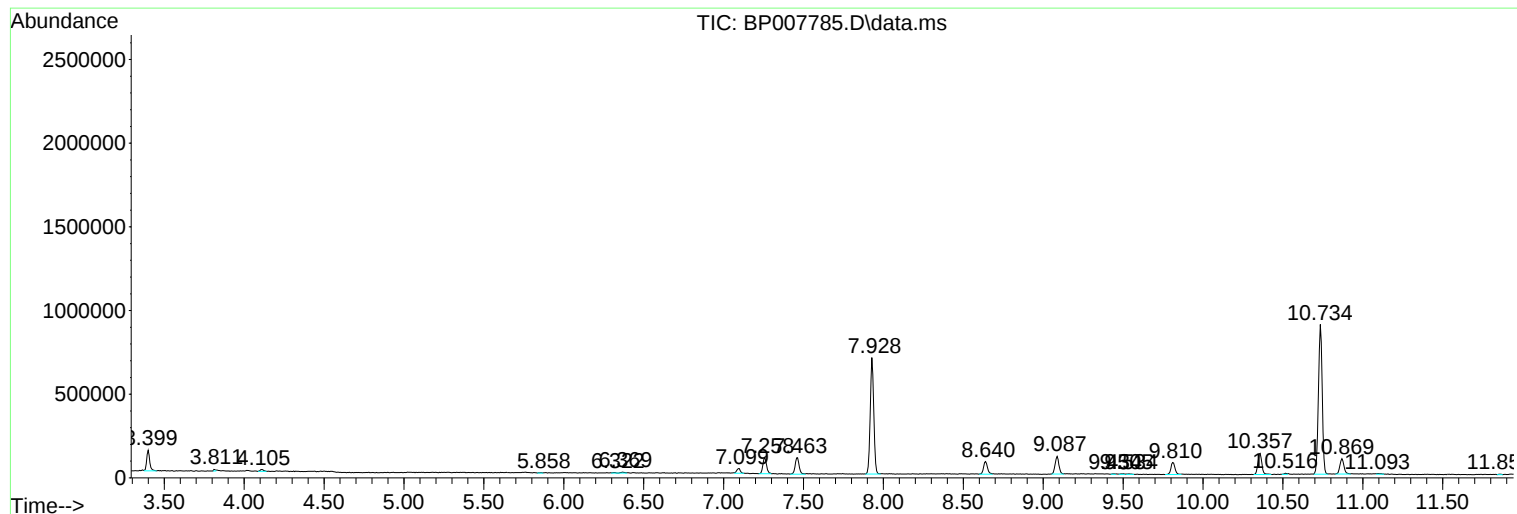

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102921\
Data File : BP007785.D
Acq On : 29 Oct 2021 16:28
Operator : CG/JU
Sample : M4282-19DL 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFYA0DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102921\
Data File : BP007785.D
Acq On : 29 Oct 2021 16:28
Operator : CG/JU
Sample : M4282-19DL 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFYA0DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
