

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102924\
 Data File : BP022721.D
 Acq On : 29 Oct 2024 22:10
 Operator : RC/JU
 Sample : P4492-13
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4ET0

Quant Time: Oct 30 01:06:59 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 29 18:08:42 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.640	152	93384	20.000	ng/ul	0.00
20) Naphthalene-d8	10.393	136	364252	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.263	164	292315	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.069	188	687346	20.000	ng/ul	0.01
79) Chrysene-d12	21.504	240	705465	20.000	ng/ul	0.01
88) Perylene-d12	24.751	264	850119	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.187	96	7004	2.915	ng/uL	0.00
4) Pyridine-d5	3.599	84	94287	14.292	ng/ul	0.00
7) Phenol-d5	6.834	99	137328	17.470	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.987	67	78455	16.981	ng/ul	0.00
11) 2-Chlorophenol-d4	7.187	132	102121	18.309	ng/ul	0.00
15) 4-Methylphenol-d8	8.346	113	118992	18.968	ng/ul	0.00
21) Nitrobenzene-d5	8.781	128	51483	18.382	ng/ul	0.00
24) 2-Nitrophenol-d4	9.493	143	61985	19.116	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.034	165	133642	19.392	ng/ul	0.00
31) 4-Chloroaniline-d4	10.540	131	144573	17.754	ng/ul	0.00
46) Dimethylphthalate-d6	13.675	166	462158	19.899	ng/ul	0.00
49) Acenaphthylene-d8	13.951	160	484890	19.657	ng/ul	0.00
54) 4-Nitrophenol-d4	14.510	143	54206	13.912	ng/ul	0.02
60) Fluorene-d10	15.275	176	416270	20.664	ng/ul	0.01
65) 4,6-Dinitro-2-methylph...	15.440	200	48595	10.750	ng/ul	0.03
73) Anthracene-d10	17.181	188	682832	21.118	ng/ul	0.02
81) Pyrene-d10	19.545	212	849042	22.759	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.527	264	981519	21.619	ng/ul	0.01
Target Compounds						
80) Fluoranthene	19.198	202	55631	1.297	ng/ul	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102924\
Data File : BP022721.D
Acq On : 29 Oct 2024 22:10
Operator : RC/JU
Sample : P4492-13
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4ET0


Quant Time: Oct 30 01:06:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 29 18:08:42 2024
Response via : Initial Calibration

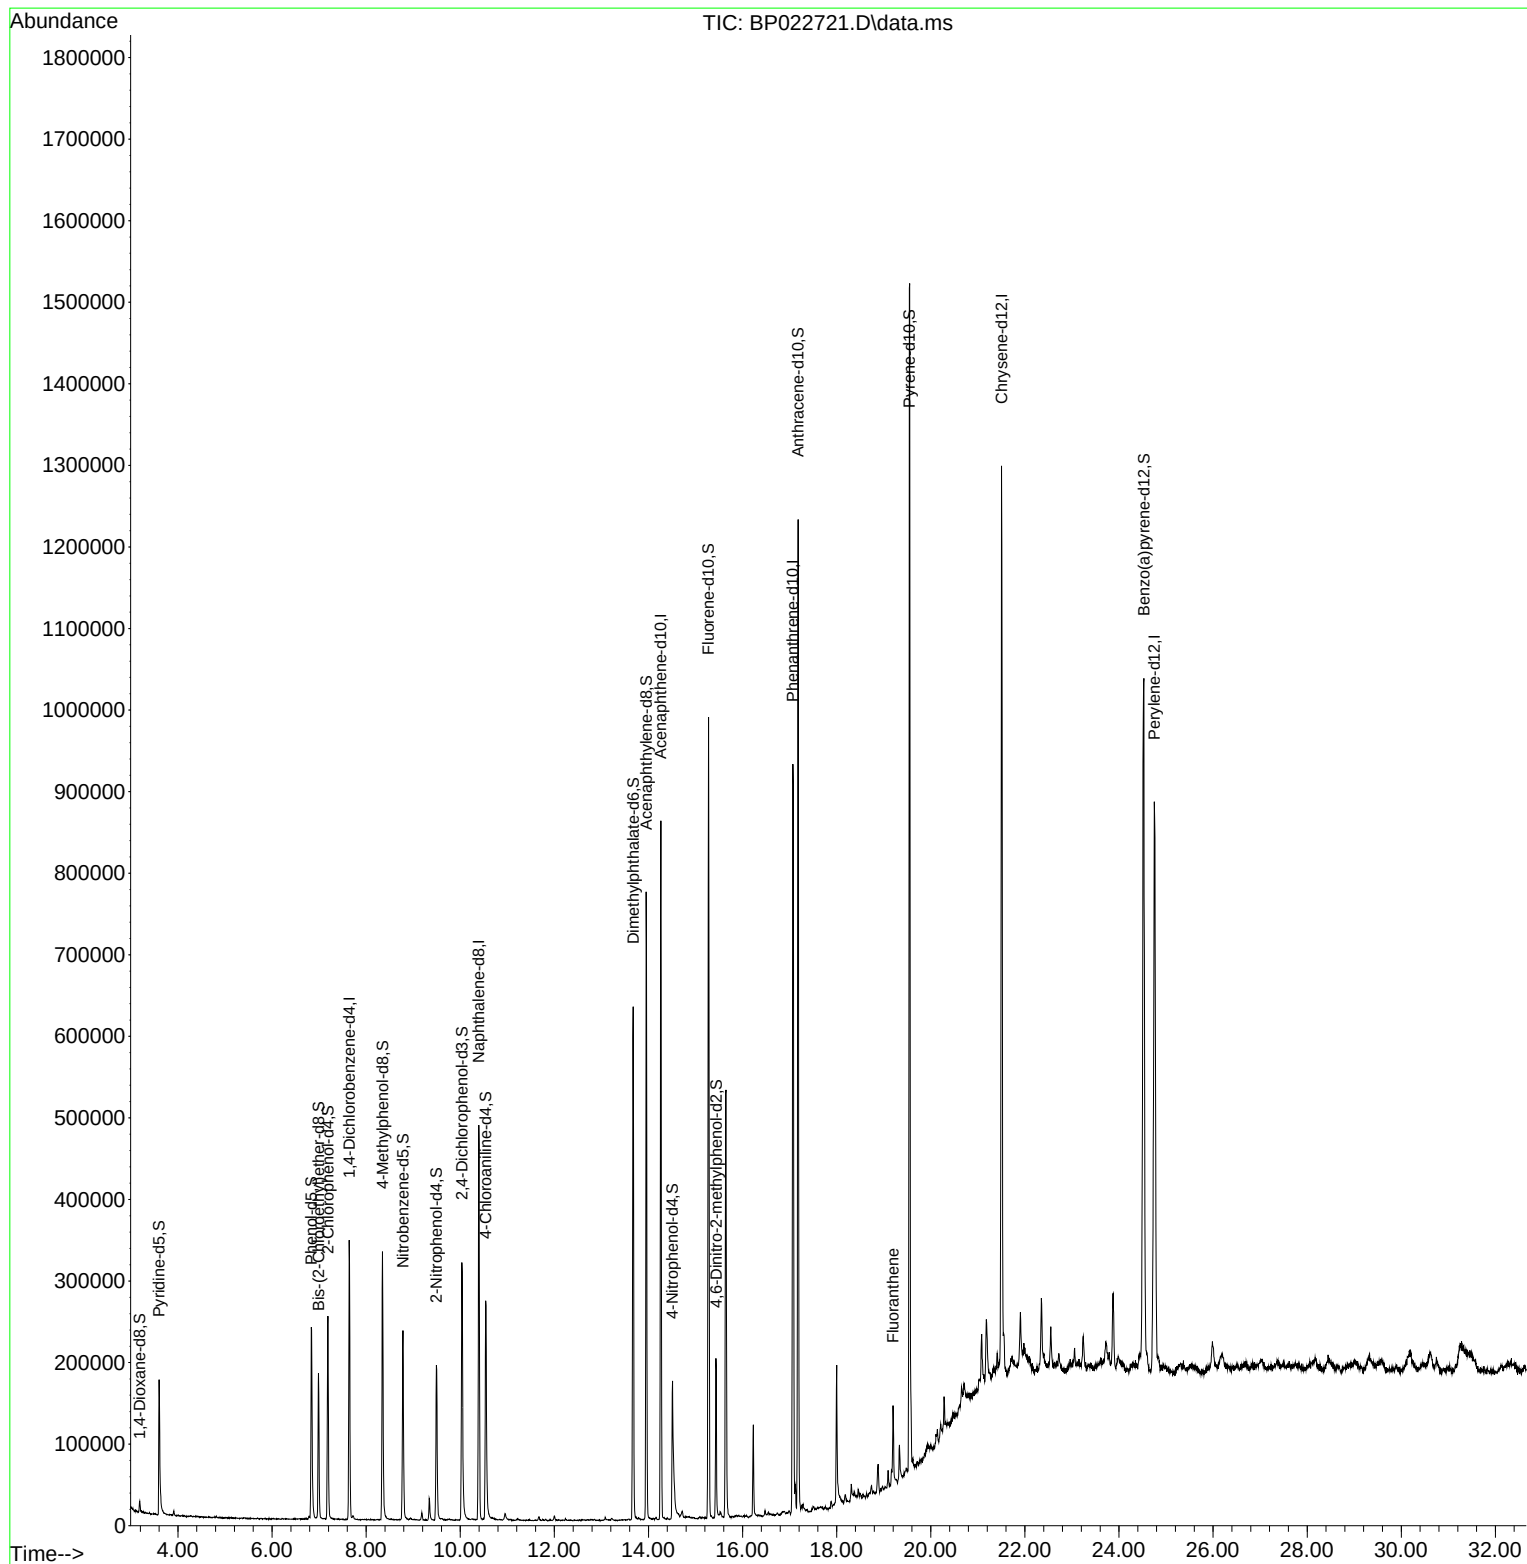

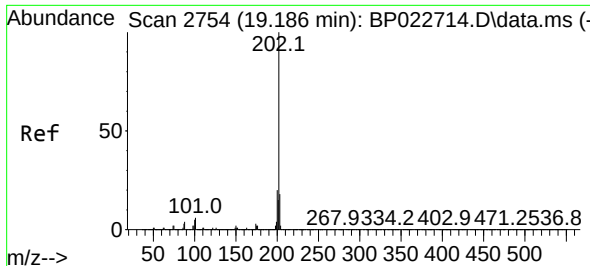

#80
 Fluoranthene
 Concen: 1.297 ng/ul
 RT: 19.198 min Scan# 21
 Delta R.T. 0.012 min
 Lab File: BP022721.D
 Acq: 29 Oct 2024 22:10

Instrument :
 BNA_P
 ClientSampleId :
 A4ET0

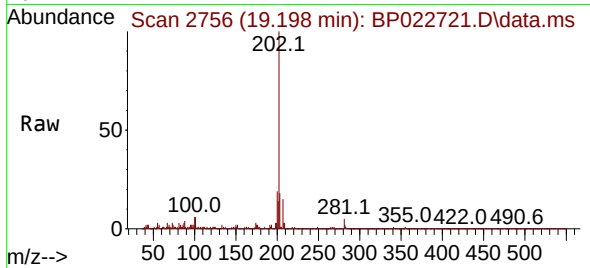

Tgt Ion:202 Resp: 55631
 Ion Ratio Lower Upper
 202 100
 101 6.4 5.8 8.8
 100 6.4 4.5 6.7

