
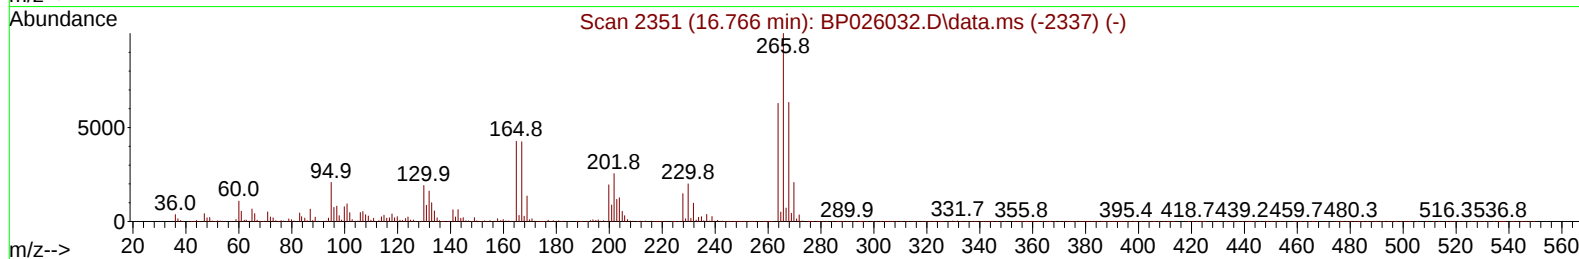
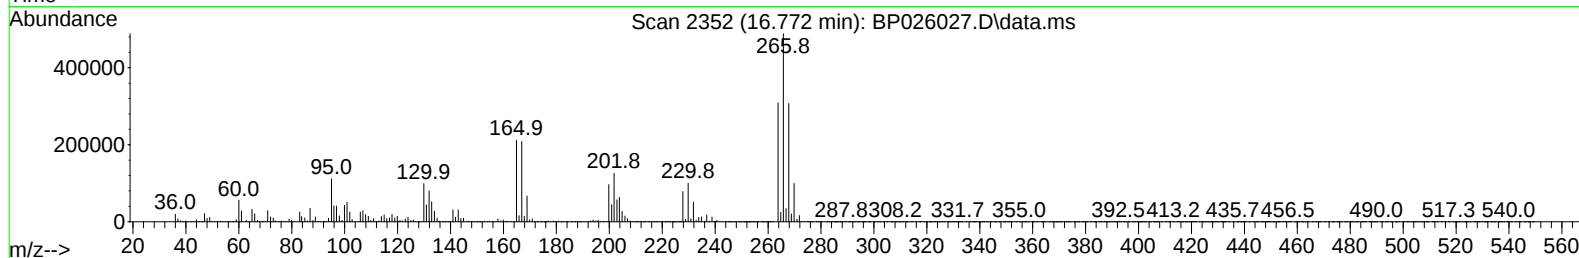


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102925\
Data File : BP026027.D
Acq On : 29 Oct 2025 08:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 29 15:04:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 29 15:02:40 2025
Response via : Initial Calibration

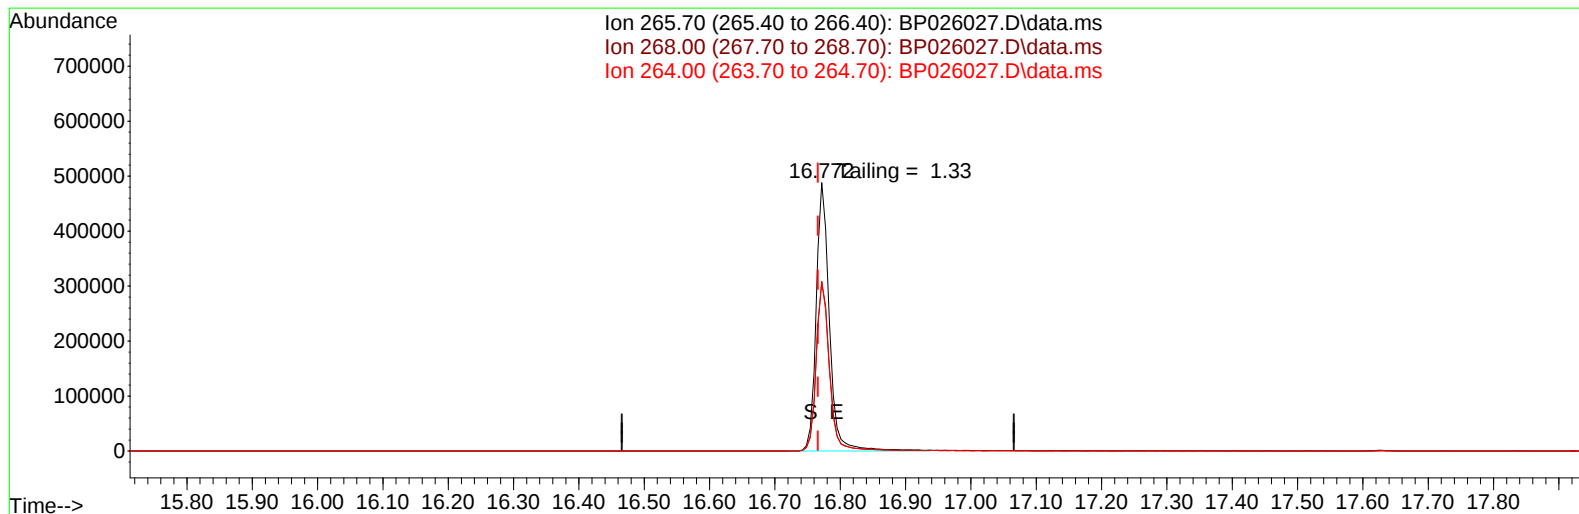

TIC: BP026027.D\data.ms

(70) Pentachlorophenol (C)




16.772min (+ 0.006) 52866.47 ng

response 688723

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	62.93
264.00	62.80	63.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102925\
Data File : BP026027.D
Acq On : 29 Oct 2025 08:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 29 15:04:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 29 15:02:40 2025
Response via : Initial Calibration

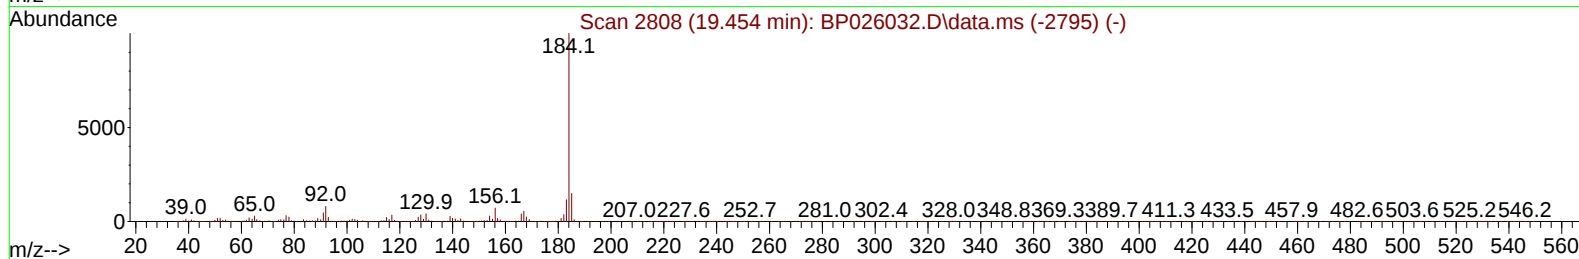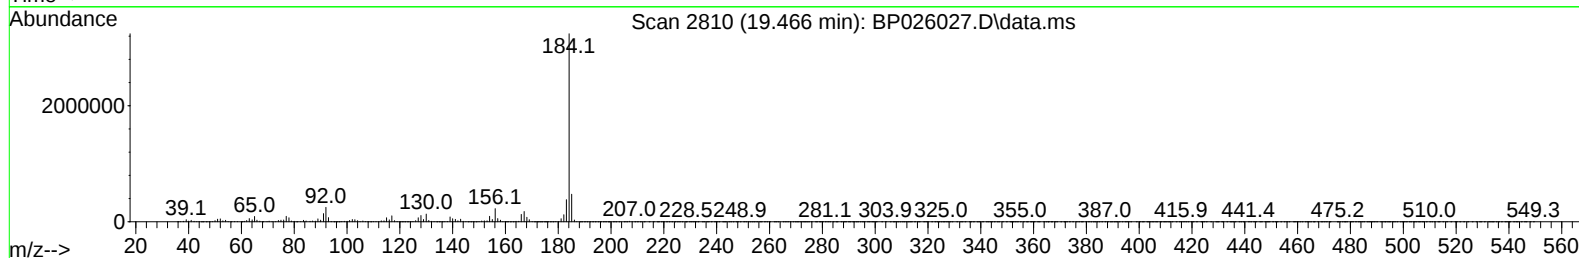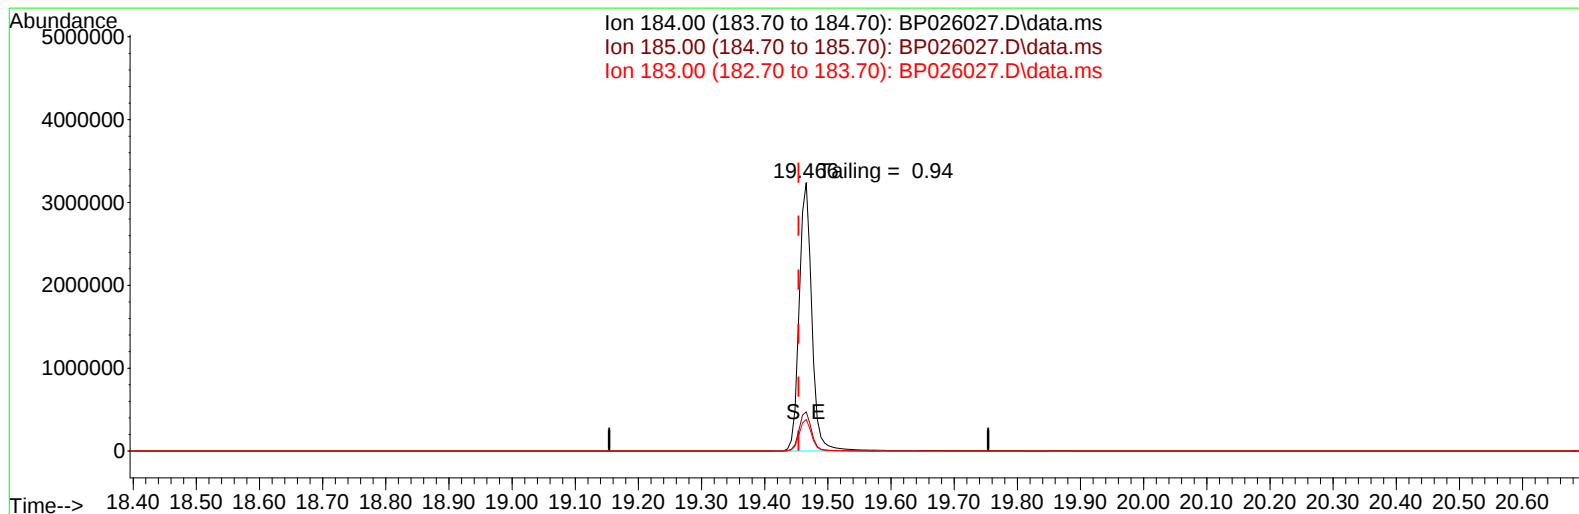

TIC: BP026027.D\data.ms

(77) Benzidine**19.466min (+ 0.012) 16317.24 ng****response 4546390**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.62
183.00	11.50	11.75
0.00	0.00	0.00