

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103123\
 Data File : BP017826.D
 Acq On : 31 Oct 2023 11:24
 Operator : MA/JU
 Sample : PB156548BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK548

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017826.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.276	28	32	43	rVB	32915	66590	2.29%	0.202%
2	3.711	101	106	128	rBV	348171	849251	29.27%	2.576%
3	4.005	154	156	161	rVB3	6807	8357	0.29%	0.025%
4	4.417	222	226	228	rBV5	3137	4507	0.16%	0.014%
5	7.046	666	673	690	rBV	611927	1096012	37.77%	3.324%
6	7.234	699	705	716	rVB	527923	835039	28.78%	2.533%
7	7.411	728	735	751	rVB	684504	1144185	39.43%	3.470%
8	7.887	809	816	826	rBV	535683	864342	29.79%	2.621%
9	8.363	894	897	901	rBV5	2252	3499	0.12%	0.011%
10	8.611	932	939	955	rBV	764351	1289613	44.44%	3.911%
11	8.781	965	968	972	rVB6	2123	3318	0.11%	0.010%
12	9.093	1013	1021	1032	rBV	622847	1045769	36.04%	3.172%
13	9.810	1136	1143	1155	rBV	543454	899313	30.99%	2.728%
14	10.340	1226	1233	1255	rBV	714571	1317104	45.39%	3.995%
15	10.716	1290	1297	1306	rBV	652957	1091047	37.60%	3.309%
16	10.893	1319	1327	1343	rBV	668049	1227220	42.29%	3.722%
17	11.757	1473	1474	1482	rVB8	2511	3556	0.12%	0.011%
18	12.322	1566	1570	1575	rBV3	9780	15731	0.54%	0.048%
19	12.757	1640	1644	1647	rBV6	2388	3872	0.13%	0.012%
20	12.899	1663	1668	1669	rVB4	2179	2948	0.10%	0.009%
21	13.422	1752	1757	1763	rBV3	10072	14627	0.50%	0.044%
22	13.546	1776	1778	1782	rVB5	2816	3122	0.11%	0.009%
23	13.793	1813	1820	1830	rBV5	3210	6684	0.23%	0.020%
24	14.004	1848	1856	1866	rBV	1257254	1737020	59.86%	5.268%
25	14.281	1896	1903	1919	rBV	1428794	2044138	70.44%	6.200%
26	14.587	1946	1955	1963	rBV	902662	1317898	45.42%	3.997%
27	14.834	1991	1997	2015	rBV	274017	611490	21.07%	1.855%
28	15.375	2086	2089	2094	rVB7	3189	4375	0.15%	0.013%
29	15.593	2119	2126	2134	rBV	1795146	2456202	84.64%	7.449%
30	15.740	2145	2151	2163	rBV	473583	709966	24.47%	2.153%
31	15.834	2164	2167	2171	rVB5	9645	14053	0.48%	0.043%
32	16.722	2314	2318	2320	rVB5	2449	2997	0.10%	0.009%
33	17.034	2369	2371	2373	rBV3	2842	3265	0.11%	0.010%
34	17.175	2392	2395	2399	rBV6	2411	3058	0.11%	0.009%
35	17.375	2423	2429	2440	rBV	1052543	1466778	50.55%	4.449%
36	17.481	2440	2447	2462	rVV	1809746	2577087	88.81%	7.816%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103123\
Data File : BP017826.D
Acq On : 31 Oct 2023 11:24
Operator : MA/JU
Sample : PB156548BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK548

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Title : SVOA CALIBRATION

37	19.304	2753	2757	2763	rBV3	22134	28912	1.00%	0.088%
38	19.381	2766	2770	2775	rVB	18593	26694	0.92%	0.081%
39	19.739	2825	2831	2842	rBV	2270155	2901819	100.00%	8.801%
40	21.522	3129	3134	3140	rBV	1031440	1376595	47.44%	4.175%
41	23.910	3533	3540	3551	rBV2	1262469	2544569	87.69%	7.718%
42	24.080	3563	3569	3580	rVB	650523	1348783	46.48%	4.091%




Sum of corrected areas: 32971405

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103123\
Data File : BP017826.D
Acq On : 31 Oct 2023 11:24
Operator : MA/JU
Sample : PB156548BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK548

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

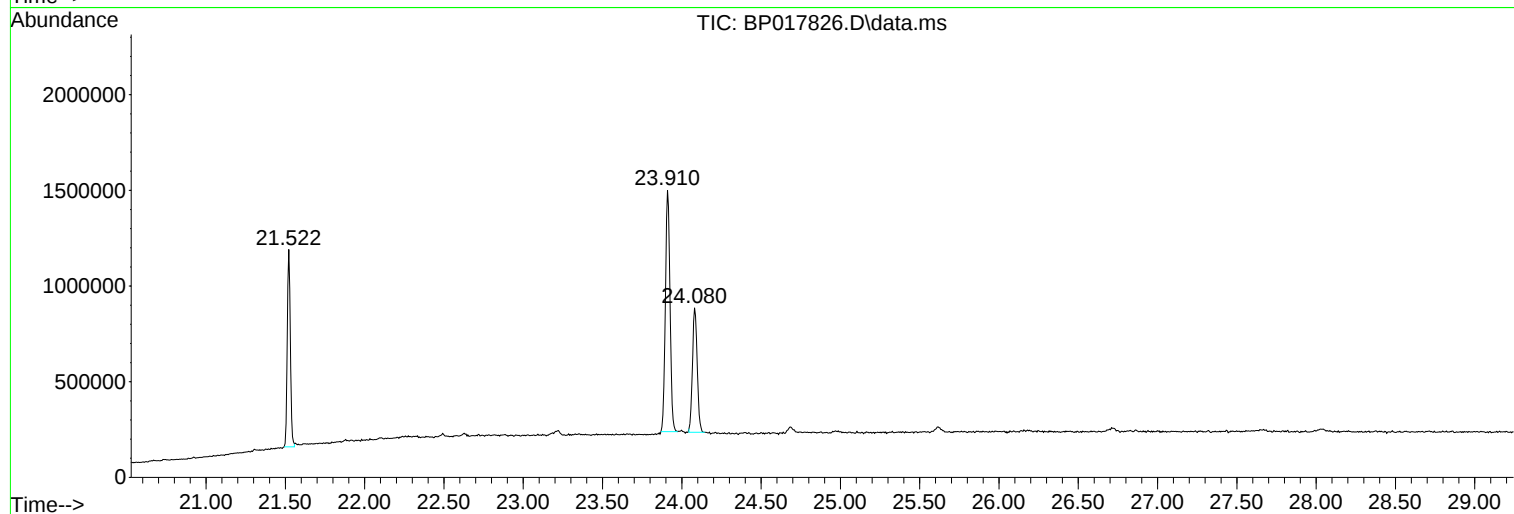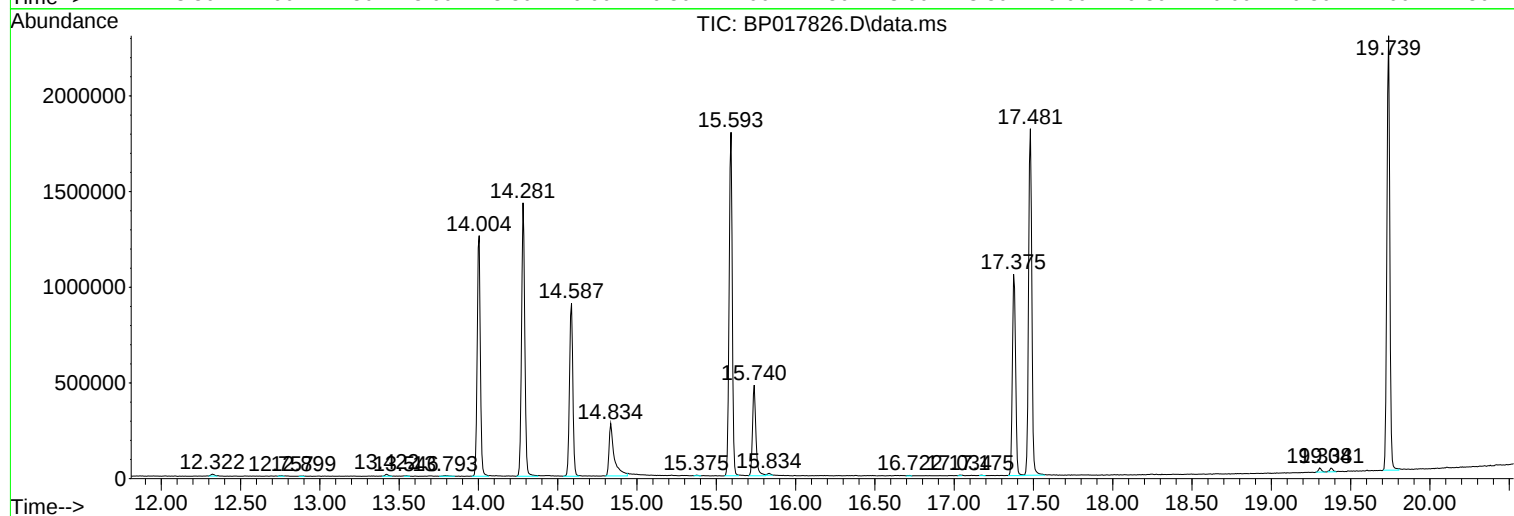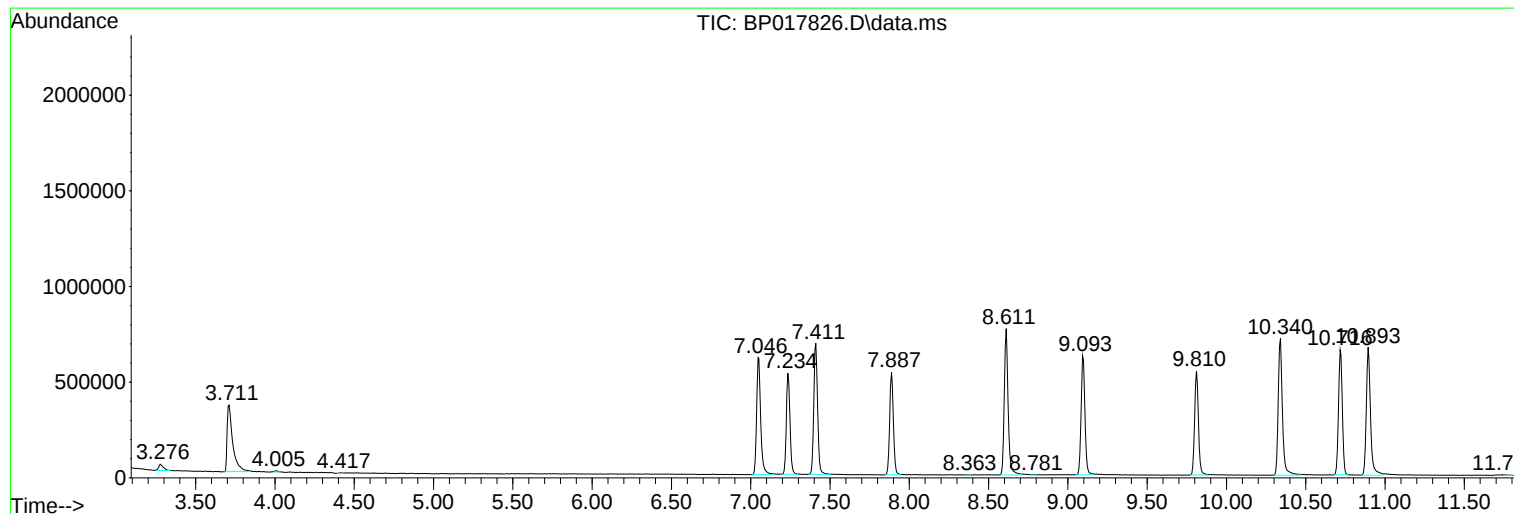

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103123\
Data File : BP017826.D
Acq On : 31 Oct 2023 11:24
Operator : MA/JU
Sample : PB156548BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK548

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103123\
Data File : BP017826.D
Acq On : 31 Oct 2023 11:24
Operator : MA/JU
Sample : PB156548BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK548

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------