

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103123\
 Data File : BP017835.D
 Acq On : 31 Oct 2023 17:35
 Operator : MA/JU
 Sample : PB156551BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK551

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017835.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	28	33	42	rVB	36307	75356	2.30%	0.199%
2	3.711	102	106	129	rBV	403790	984828	30.00%	2.601%
3	4.411	221	225	226	rBV4	3095	4310	0.13%	0.011%
4	7.052	667	674	690	rBV	753400	1260201	38.39%	3.328%
5	7.240	697	706	720	rBV	608149	971003	29.58%	2.564%
6	7.410	728	735	752	rBV	793353	1324095	40.33%	3.497%
7	7.893	807	817	831	rBV	595976	994720	30.30%	2.627%
8	8.610	932	939	955	rBV	875535	1482862	45.17%	3.916%
9	9.099	1015	1022	1039	rBV	732688	1210307	36.87%	3.196%
10	9.816	1135	1144	1162	rBV	609150	1053961	32.10%	2.783%
11	10.340	1226	1233	1251	rBV	852613	1506990	45.90%	3.980%
12	10.722	1291	1298	1306	rBV	757580	1250856	38.10%	3.303%
13	10.899	1320	1328	1342	rBV	773890	1386888	42.25%	3.663%
14	11.746	1471	1472	1478	rVB6	2445	3689	0.11%	0.010%
15	12.210	1548	1551	1554	rBV5	2704	3607	0.11%	0.010%
16	12.328	1564	1571	1578	rBV2	11717	25102	0.76%	0.066%
17	13.422	1748	1757	1763	rBV2	14049	22899	0.70%	0.060%
18	13.687	1796	1802	1807	rBV10	3544	9380	0.29%	0.025%
19	13.792	1814	1820	1827	rVB9	5493	10951	0.33%	0.029%
20	14.004	1848	1856	1867	rBV	1446258	1974871	60.16%	5.215%
21	14.192	1880	1888	1890	rBV9	2593	4773	0.15%	0.013%
22	14.287	1897	1904	1914	rBV	1639650	2324667	70.81%	6.139%
23	14.434	1925	1929	1933	rVB7	3551	5534	0.17%	0.015%
24	14.587	1948	1955	1966	rBV	999324	1497405	45.61%	3.954%
25	14.834	1992	1997	2023	rBV	344960	783803	23.88%	2.070%
26	15.216	2060	2062	2068	rVV7	2691	3457	0.11%	0.009%
27	15.375	2086	2089	2093	rBV5	5483	7540	0.23%	0.020%
28	15.592	2114	2126	2134	rBV	2013341	2811030	85.63%	7.424%
29	15.739	2145	2151	2162	rBV	548231	797954	24.31%	2.107%
30	15.834	2165	2167	2173	rVB6	12413	18264	0.56%	0.048%
31	16.057	2202	2205	2210	rBV7	2136	3310	0.10%	0.009%
32	16.645	2302	2305	2310	rVB6	3435	4515	0.14%	0.012%
33	17.045	2367	2373	2377	rVB9	4315	7997	0.24%	0.021%
34	17.169	2391	2394	2398	rBV6	3193	4838	0.15%	0.013%
35	17.381	2423	2430	2441	rBV	1212834	1662774	50.65%	4.391%
36	17.481	2441	2447	2464	rVB	2049609	2918846	88.91%	7.708%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103123\
Data File : BP017835.D
Acq On : 31 Oct 2023 17:35
Operator : MA/JU
Sample : PB156551BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK551

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Title : SVOA CALIBRATION

37	17.704	2481	2485	2487	rBV5	2279	3674	0.11%	0.010%
38	18.239	2574	2576	2580	rVB5	4721	4784	0.15%	0.013%
39	18.657	2643	2647	2650	rVB5	2813	3914	0.12%	0.010%
40	19.310	2754	2758	2763	rBV2	24655	33588	1.02%	0.089%
41	19.386	2767	2771	2774	rBV	22352	28526	0.87%	0.075%
42	19.745	2826	2832	2839	rBV	2476916	3282941	100.00%	8.670%
43	21.527	3130	3135	3146	rBV	1193435	1581016	48.16%	4.175%
44	23.921	3534	3542	3551	rBV2	1458773	2983419	90.88%	7.879%
45	24.092	3564	3571	3580	rVB	720876	1530995	46.63%	4.043%




Sum of corrected areas: 37866440

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103123\
Data File : BP017835.D
Acq On : 31 Oct 2023 17:35
Operator : MA/JU
Sample : PB156551BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK551

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

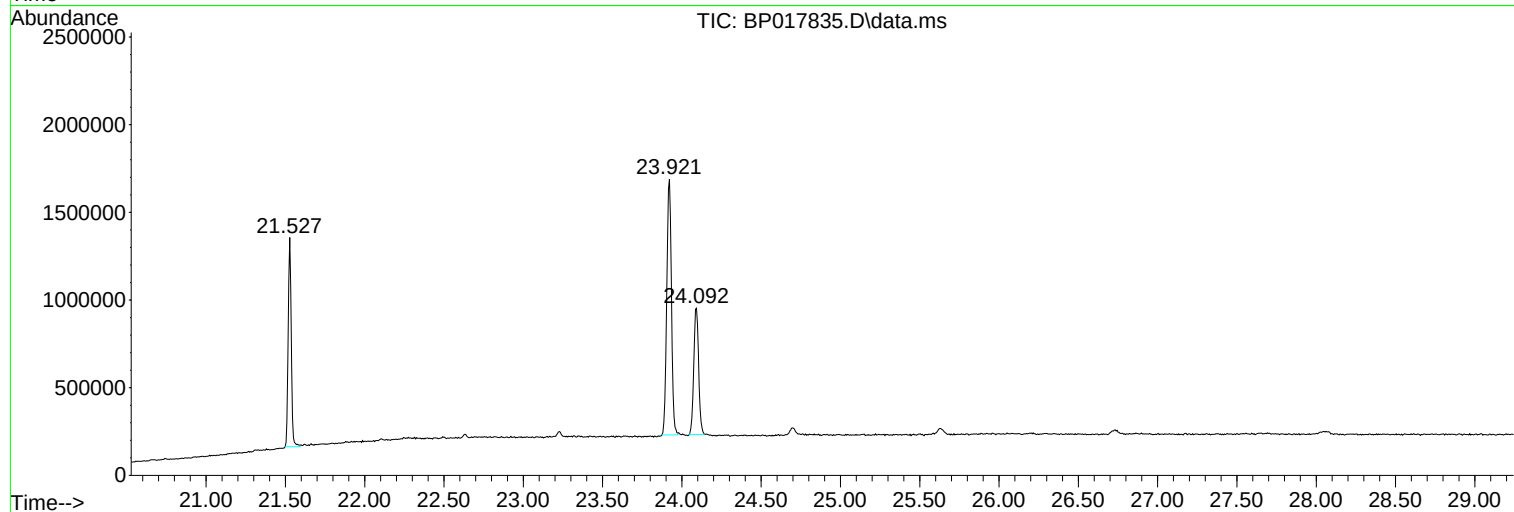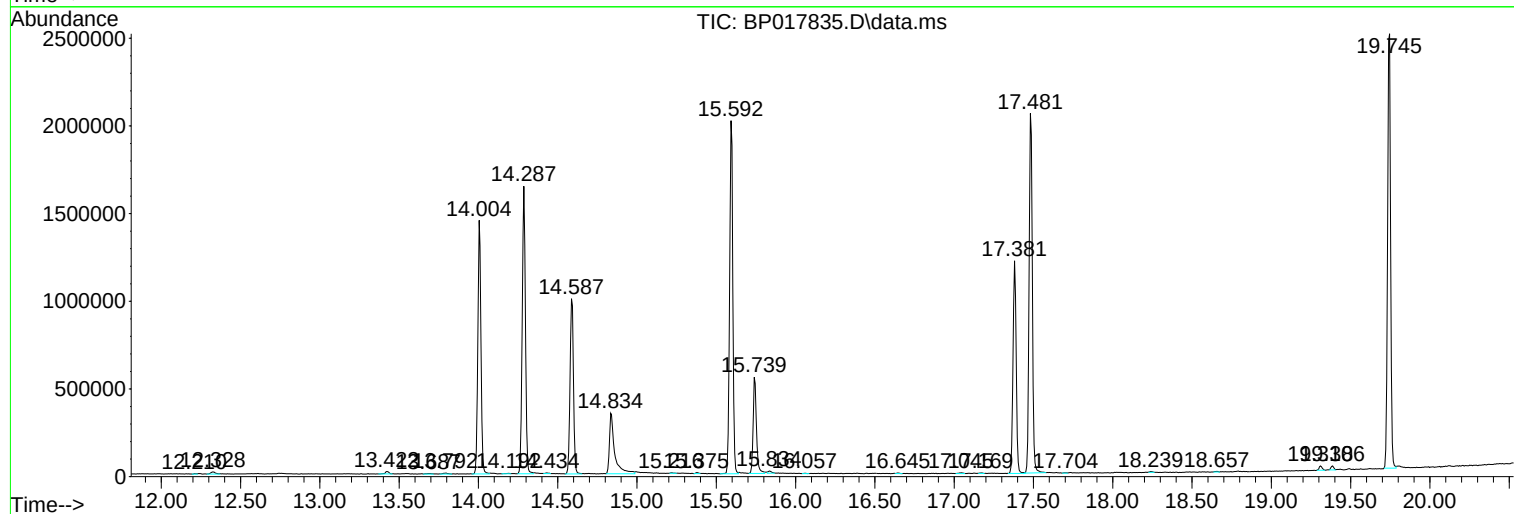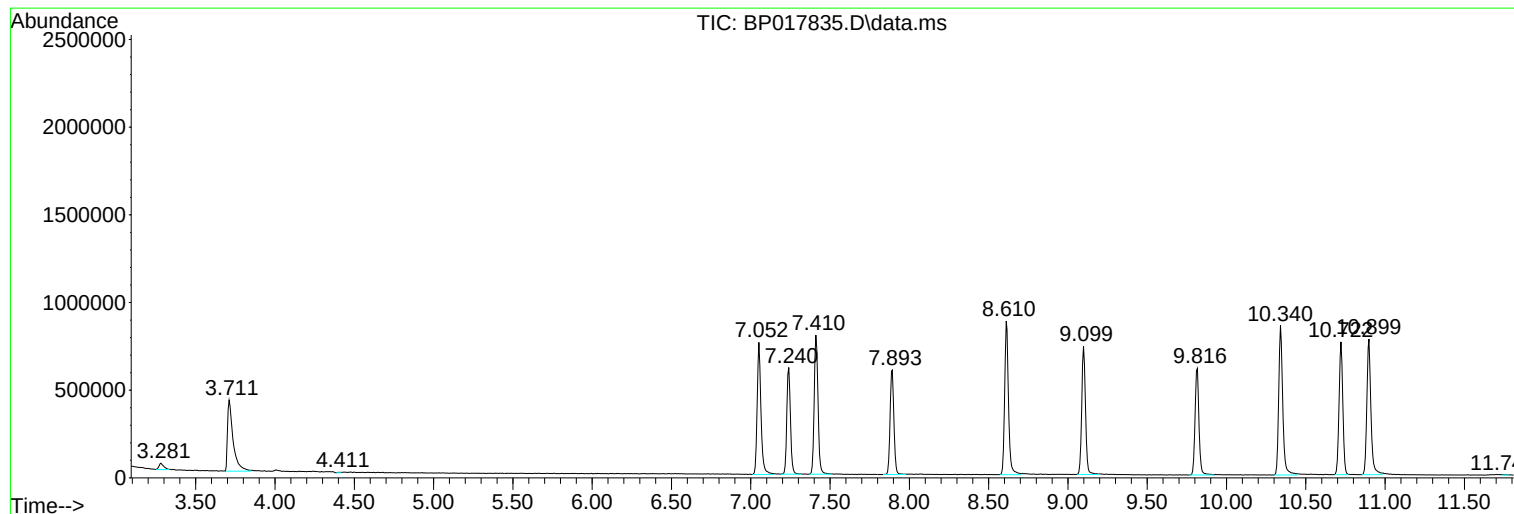

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103123\
Data File : BP017835.D
Acq On : 31 Oct 2023 17:35
Operator : MA/JU
Sample : PB156551BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK551

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103123\
Data File : BP017835.D
Acq On : 31 Oct 2023 17:35
Operator : MA/JU
Sample : PB156551BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK551

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------