

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103123\
 Data File : BP017836.D
 Acq On : 31 Oct 2023 18:09
 Operator : MA/JU
 Sample : 05139-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017836.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.317	37	39	40	rBV2	3717	2681	0.18%	0.034%
2	3.840	126	128	130	rBV3	2854	2959	0.20%	0.038%
3	3.999	151	155	161	rBV3	11341	21062	1.42%	0.268%
4	4.399	219	223	228	rBV3	4134	8142	0.55%	0.104%
5	4.540	245	247	248	rVB2	2742	1524	0.10%	0.019%
6	4.716	275	277	282	rVB6	2271	3140	0.21%	0.040%
7	4.946	315	316	318	rBV2	2358	1502	0.10%	0.019%
8	5.775	455	457	460	rVB3	2527	1966	0.13%	0.025%
9	6.034	498	501	503	rBV4	1607	1555	0.10%	0.020%
10	6.081	505	509	510	rBV4	1679	2073	0.14%	0.026%
11	6.146	518	520	523	rVB3	2567	1912	0.13%	0.024%
12	6.305	544	547	548	rBV3	1780	1775	0.12%	0.023%
13	6.428	567	568	571	rBV3	1673	1559	0.10%	0.020%
14	6.499	577	580	582	rVB4	1524	1548	0.10%	0.020%
15	6.763	624	625	629	rBV5	2156	2788	0.19%	0.036%
16	6.928	650	653	659	rVV7	2114	3388	0.23%	0.043%
17	7.063	674	676	682	rVB7	1445	2081	0.14%	0.027%
18	7.416	733	736	738	rBV4	1839	2125	0.14%	0.027%
19	7.669	776	779	780	rBV3	1479	1544	0.10%	0.020%
20	7.881	804	815	833	rBV	540041	941505	63.30%	11.991%
21	8.234	874	875	879	rBV4	1506	1639	0.11%	0.021%
22	8.281	881	883	885	rVB3	1819	1622	0.11%	0.021%
23	8.546	924	928	929	rVB4	1827	1948	0.13%	0.025%
24	8.557	929	930	933	rBV3	1878	2070	0.14%	0.026%
25	8.652	944	946	949	rBV4	1933	1678	0.11%	0.021%
26	8.863	980	982	985	rVB3	1490	1693	0.11%	0.022%
27	9.252	1045	1048	1050	rVV4	1873	2099	0.14%	0.027%
28	9.275	1050	1052	1056	rVB5	2140	2506	0.17%	0.032%
29	9.369	1064	1068	1072	rVB6	1258	2194	0.15%	0.028%
30	9.999	1174	1175	1178	rBV3	2021	1681	0.11%	0.021%
31	10.710	1289	1296	1317	rBV	661522	1170279	78.69%	14.905%
32	10.846	1317	1319	1325	rVB7	2047	3806	0.26%	0.048%
33	11.034	1349	1351	1354	rBV4	1975	1892	0.13%	0.024%
34	11.257	1386	1389	1392	rBV5	1296	1737	0.12%	0.022%
35	11.540	1432	1437	1440	rBV7	1470	2158	0.15%	0.027%
36	11.763	1473	1475	1477	rVV2	2055	2066	0.14%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103123\
 Data File : BP017836.D
 Acq On : 31 Oct 2023 18:09
 Operator : MA/JU
 Sample : 05139-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Title : SVOA CALIBRATION

37	11.810	1480	1483	1485	rBV4	1435	1536	0.10%	0.020%
38	11.963	1507	1509	1514	rVB6	2151	2394	0.16%	0.030%
39	12.010	1514	1517	1520	rBV5	1667	1651	0.11%	0.021%
40	12.381	1577	1580	1582	rVV4	1515	1683	0.11%	0.021%

41	13.251	1724	1728	1731	rBV6	1374	2146	0.14%	0.027%
42	13.287	1732	1734	1739	rVB6	1840	1561	0.10%	0.020%
43	13.334	1739	1742	1746	rBV6	1419	1669	0.11%	0.021%
44	13.422	1751	1757	1760	rBV8	3219	5659	0.38%	0.072%
45	13.545	1774	1778	1781	rVB5	1386	1916	0.13%	0.024%

46	13.581	1781	1784	1786	rBV4	2084	1694	0.11%	0.022%
47	13.881	1832	1835	1838	rBV5	1674	1653	0.11%	0.021%
48	13.922	1838	1842	1844	rVB5	1216	1708	0.11%	0.022%
49	13.981	1851	1852	1855	rVB3	1879	1731	0.12%	0.022%
50	14.192	1882	1888	1890	rBV6	1534	2358	0.16%	0.030%

51	14.310	1904	1908	1912	rBV7	1856	3037	0.20%	0.039%
52	14.575	1946	1953	1966	rBV	905797	1371159	92.19%	17.464%
53	14.698	1972	1974	1977	rVB3	1677	1599	0.11%	0.020%
54	14.887	2002	2006	2007	rBV4	1707	1889	0.13%	0.024%
55	15.210	2058	2061	2064	rVB5	2213	2125	0.14%	0.027%

56	15.239	2064	2066	2069	rBV4	1381	1508	0.10%	0.019%
57	15.369	2083	2088	2091	rBV7	1527	2349	0.16%	0.030%
58	15.422	2093	2097	2099	rBV4	1592	1912	0.13%	0.024%
59	15.463	2102	2104	2108	rVB5	1695	2191	0.15%	0.028%
60	15.598	2125	2127	2129	rBV3	1946	1950	0.13%	0.025%

61	15.734	2144	2150	2151	rBV6	1287	1772	0.12%	0.023%
62	15.786	2157	2159	2161	rBV3	1681	1607	0.11%	0.020%
63	16.045	2201	2203	2206	rBV3	1047	1522	0.10%	0.019%
64	16.363	2252	2257	2259	rBV6	1476	1682	0.11%	0.021%
65	16.445	2269	2271	2274	rBV4	1654	1758	0.12%	0.022%

66	16.516	2281	2283	2285	rBV2	1751	1524	0.10%	0.019%
67	16.592	2294	2296	2299	rBV4	1619	1899	0.13%	0.024%
68	16.639	2299	2304	2307	rVV7	1742	2933	0.20%	0.037%
69	16.757	2322	2324	2326	rBV2	1278	1625	0.11%	0.021%
70	16.910	2348	2350	2355	rVB6	1078	1681	0.11%	0.021%

71	17.098	2381	2382	2385	rBV3	1721	1613	0.11%	0.021%
72	17.139	2387	2389	2391	rBV3	1459	1535	0.10%	0.020%
73	17.269	2408	2411	2415	rVB6	1999	3167	0.21%	0.040%
74	17.369	2422	2428	2443	rBV	985834	1487294	100.00%	18.943%
75	17.598	2464	2467	2468	rVB2	2150	1714	0.12%	0.022%

76	17.739	2489	2491	2495	rVB5	1974	2502	0.17%	0.032%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103123\
Data File : BP017836.D
Acq On : 31 Oct 2023 18:09
Operator : MA/JU
Sample : 05139-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC-BLANK

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Title : SVOA CALIBRATION

77	17.845	2507	2509	2512	rBV4	2167	2273	0.15%	0.029%
78	18.051	2542	2544	2546	rVB2	1708	1548	0.10%	0.020%
79	18.163	2560	2563	2565	rBV4	1798	2337	0.16%	0.030%
80	18.192	2565	2568	2570	rBV4	1757	2115	0.14%	0.027%
81	19.086	2718	2720	2723	rVB4	2838	2451	0.16%	0.031%
82	21.516	3128	3133	3141	rBV	1048266	1377040	92.59%	17.539%
83	24.074	3561	3568	3579	rVB	629677	1320959	88.82%	16.824%




Sum of corrected areas: 7851526

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103123\
Data File : BP017836.D
Acq On : 31 Oct 2023 18:09
Operator : MA/JU
Sample : 05139-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

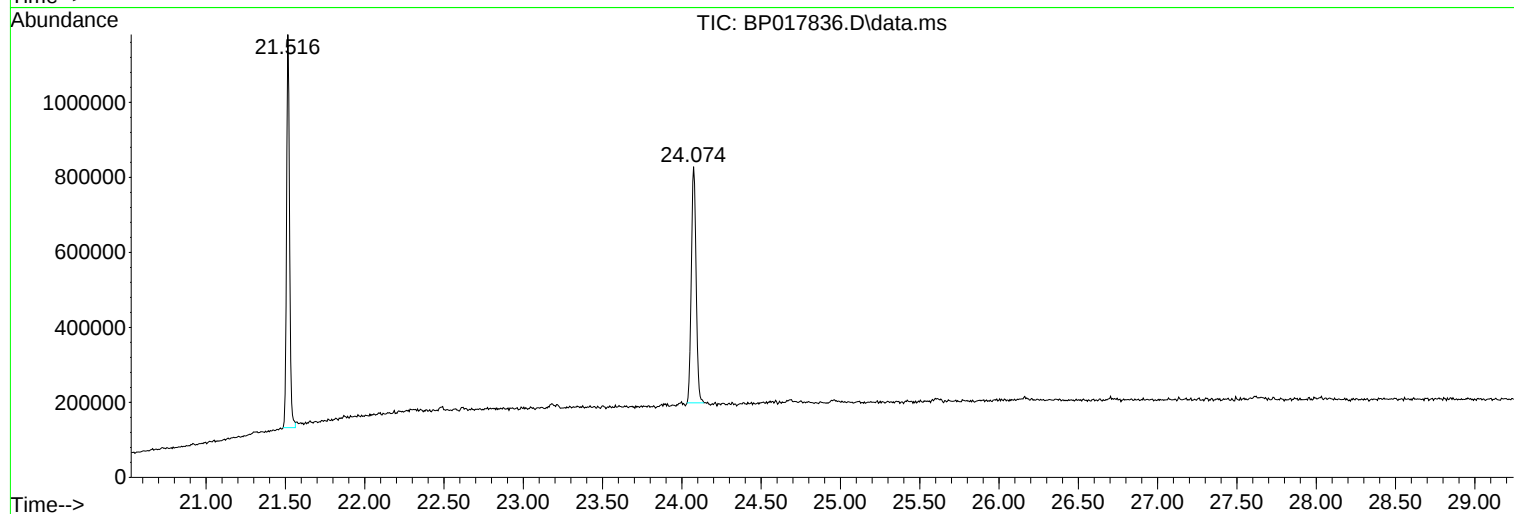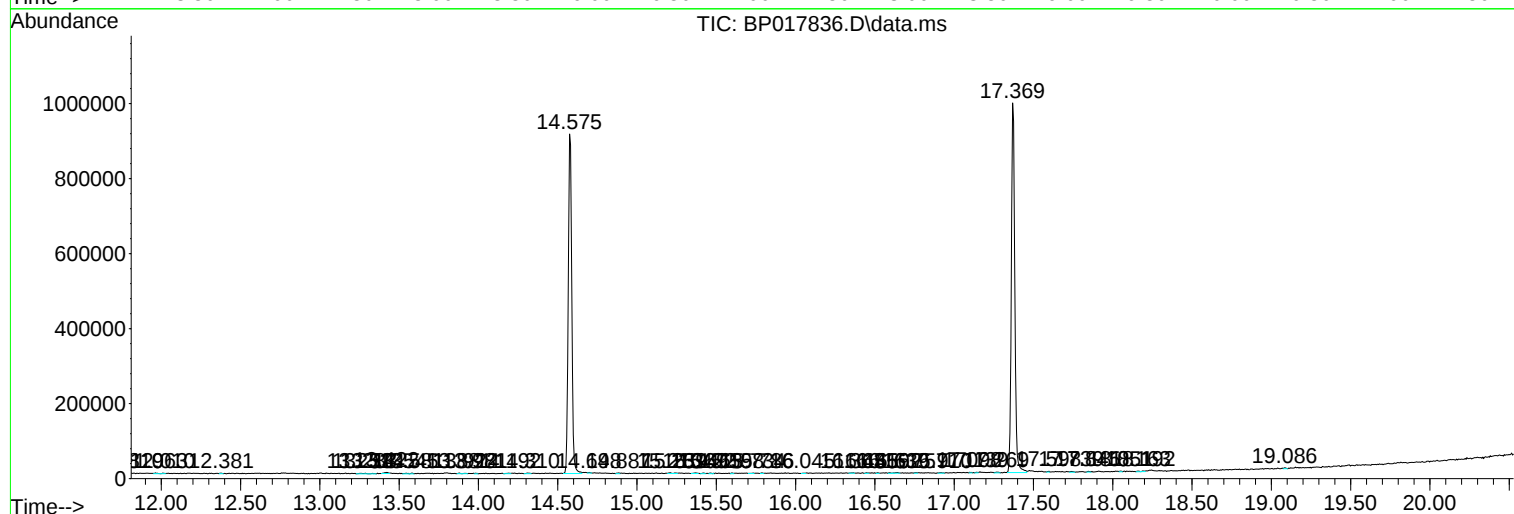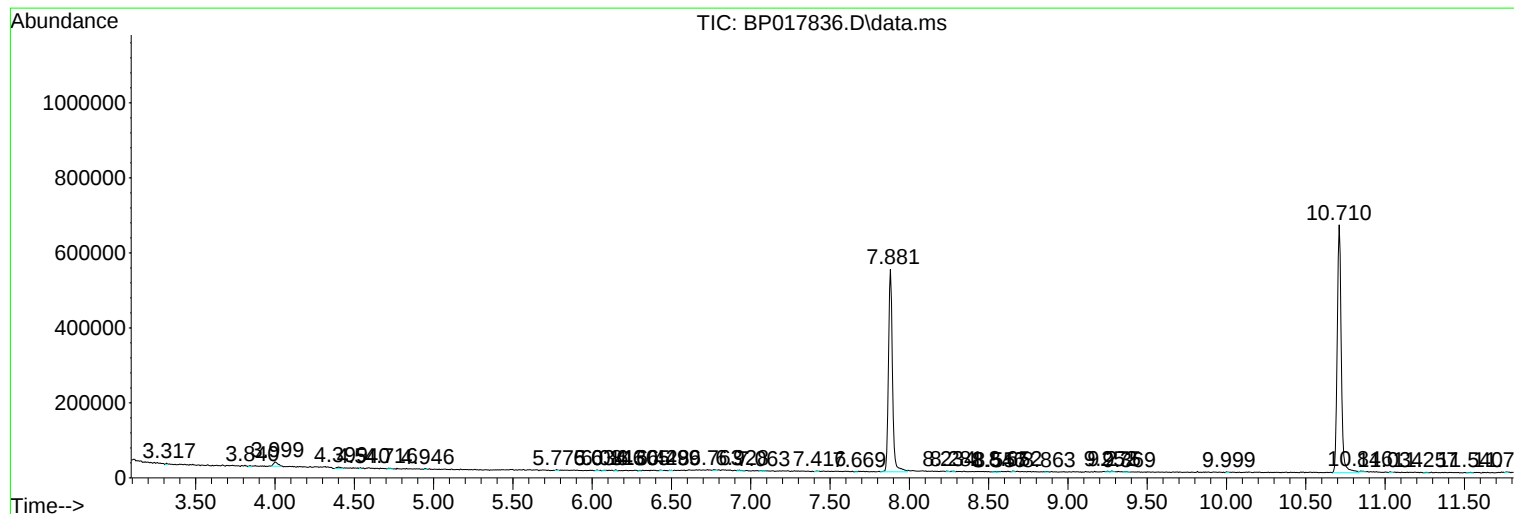

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103123\
Data File : BP017836.D
Acq On : 31 Oct 2023 18:09
Operator : MA/JU
Sample : 05139-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103123\
Data File : BP017836.D
Acq On : 31 Oct 2023 18:09
Operator : MA/JU
Sample : 05139-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------