




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
Data File : BP017866.D
Acq On : 02 Nov 2023 00:33
Operator : MA/JU
Sample : 04944-07
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A49F4

Manual IntegrationsAPPROVED

Quant Time: Nov 02 02:18:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 19 01:32:15 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/03/2023
Supervised By :mohammad ahmed 11/04/2023

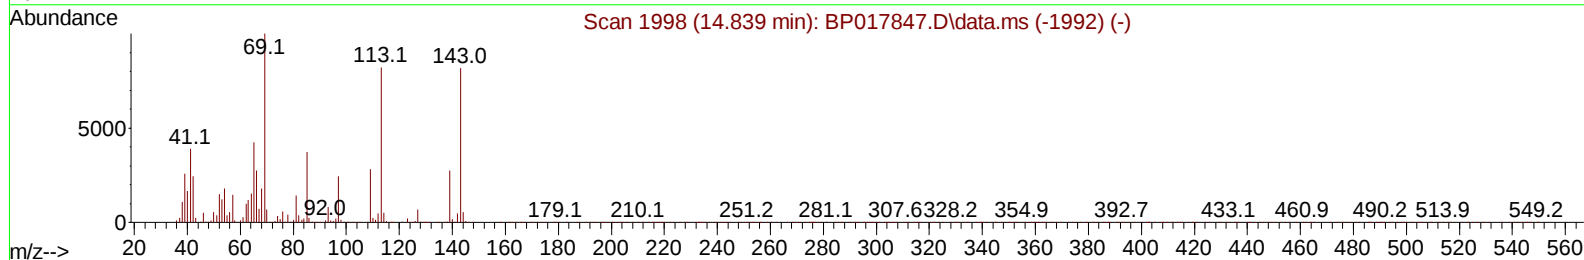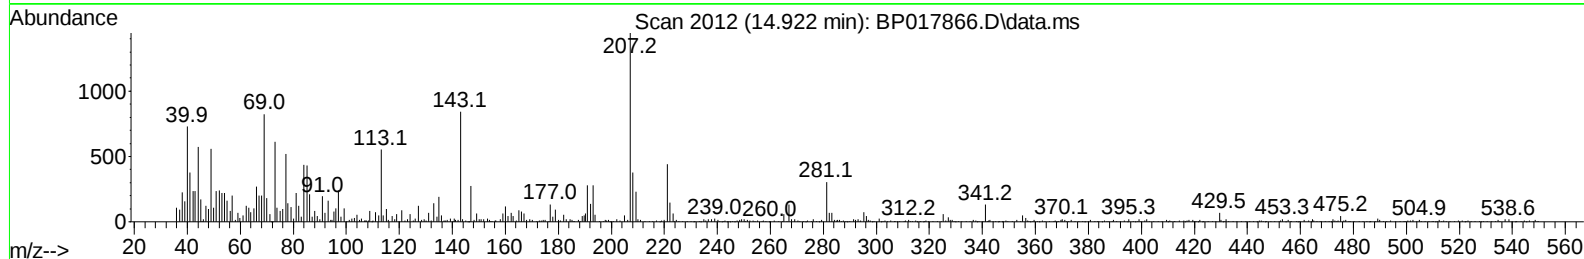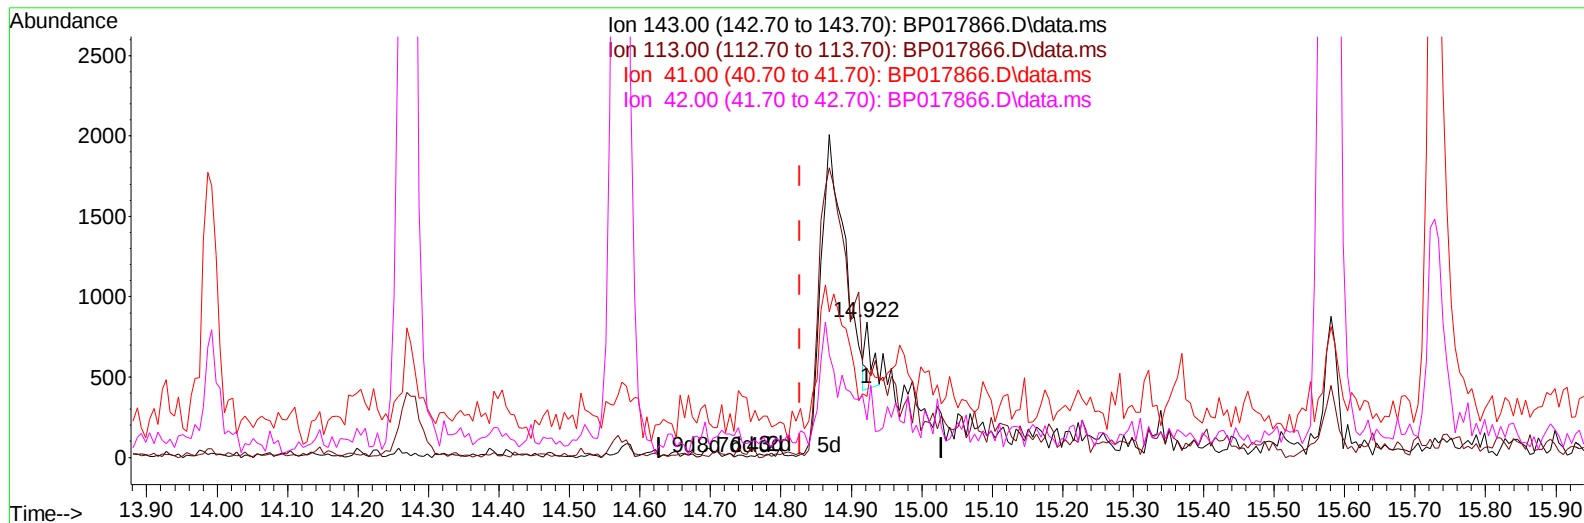

TIC: BP017866.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.922min (+ 0.094) 0.08 ng/u1

response 264

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	81.70	65.40
41.00	39.20	44.91
42.00	25.60	27.73

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
 Data File : BP017866.D
 Acq On : 02 Nov 2023 00:33
 Operator : MA/JU
 Sample : 04944-07
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A49F4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/03/2023
 Supervised By :mohammad ahmed 11/04/2023

Quant Time: Nov 02 02:19:59 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 19 01:32:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.875	152	132065	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.704	136	485247	20.000	ng/ul	-0.02
38) Acenaphthene-d10	14.575	164	272603	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.369	188	554739	20.000	ng/ul	0.00
79) Chrysene-d12	21.510	240	483955	20.000	ng/ul	0.00
88) Perylene-d12	24.063	264	514349	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	12548	3.535	ng/uL	0.02
4) Pyridine-d5	3.711	84	80647	8.677	ng/ul	0.02
7) Phenol-d5	7.046	99	48283	4.393	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	172406	25.402	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.399	132	159049	17.744	ng/ul	-0.01
15) 4-Methylphenol-d8	8.605	113	92304	10.695	ng/ul	0.00
21) Nitrobenzene-d5	9.087	128	100899	25.661	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.799	143	106108	24.424	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.328	165	177216	20.795	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.881	131	268026	24.032	ng/ul	-0.01
46) Dimethylphthalate-d6	13.992	166	618769	27.039	ng/ul	-0.01
49) Acenaphthylene-d8	14.269	160	667707	26.163	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.869	143	8145m	2.498	ng/ul	0.04
60) Fluorene-d10	15.581	176	515107	26.040	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.728	200	67870	18.574	ng/ul	0.00
73) Anthracene-d10	17.469	188	771517	27.215	ng/ul	0.00
81) Pyrene-d10	19.727	212	892795	29.425	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.892	264	772094	26.951	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
Data File : BP017866.D
Acq On : 02 Nov 2023 00:33
Operator : MA/JU
Sample : 04944-07
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A49F4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/03/2023
Supervised By :mohammad ahmed 11/04/2023

Quant Time: Nov 02 02:19:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 19 01:32:15 2023
Response via : Initial Calibration

