

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
 Data File : BP017848.D
 Acq On : 01 Nov 2023 10:31
 Operator : MA/JU
 Sample : PB156550BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK550

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017848.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	29	33	44	rVB2	16405	41316	2.31%	0.183%
2	3.711	103	106	121	rBV	160970	417568	23.32%	1.852%
3	4.869	301	303	305	rBV2	2387	1982	0.11%	0.009%
4	5.105	341	343	347	rBV5	1675	1865	0.10%	0.008%
5	6.487	572	578	579	rBV6	2698	3746	0.21%	0.017%
6	6.952	655	657	660	rVB4	2638	2582	0.14%	0.011%
7	7.046	667	673	688	rVV	290867	530948	29.65%	2.354%
8	7.234	699	705	715	rBV	252183	419245	23.41%	1.859%
9	7.328	719	721	727	rVB6	4148	6400	0.36%	0.028%
10	7.405	727	734	752	rBV	330352	577273	32.24%	2.560%
11	7.881	808	815	826	rBV	536191	891031	49.76%	3.951%
12	8.193	865	868	870	rBV4	1699	1977	0.11%	0.009%
13	8.316	885	889	890	rBV4	1997	2411	0.13%	0.011%
14	8.352	890	895	900	rVV9	3984	7790	0.44%	0.035%
15	8.605	932	938	953	rBV	339446	634145	35.42%	2.812%
16	8.746	960	962	970	rVB7	5238	9666	0.54%	0.043%
17	8.822	973	975	980	rBV6	1572	2398	0.13%	0.011%
18	8.946	991	996	1001	rVV8	5191	8262	0.46%	0.037%
19	9.093	1013	1021	1036	rBV	298964	522697	29.19%	2.318%
20	9.652	1110	1116	1119	rBV6	3618	5858	0.33%	0.026%
21	9.810	1136	1143	1154	rBV	232569	420457	23.48%	1.864%
22	9.887	1154	1156	1162	rVV6	5943	12291	0.69%	0.054%
23	10.157	1196	1202	1206	rBV6	2820	4796	0.27%	0.021%
24	10.340	1226	1233	1250	rBV	318470	623748	34.83%	2.766%
25	10.540	1263	1267	1270	rVB6	1597	2577	0.14%	0.011%
26	10.716	1287	1297	1313	rBV	687673	1148456	64.14%	5.092%
27	10.893	1319	1327	1340	rBV	291975	573405	32.02%	2.543%
28	10.981	1340	1342	1351	rVB9	10010	18575	1.04%	0.082%
29	12.322	1564	1570	1577	rBV4	11037	20801	1.16%	0.092%
30	12.404	1577	1584	1587	rBV9	5442	9649	0.54%	0.043%
31	12.498	1596	1600	1601	rBV4	2023	2446	0.14%	0.011%
32	12.616	1613	1620	1627	rBV5	7587	17360	0.97%	0.077%
33	12.693	1629	1633	1637	rBV7	1339	1801	0.10%	0.008%
34	12.757	1639	1644	1651	rVB8	5168	10124	0.57%	0.045%
35	13.028	1686	1690	1696	rBV9	2586	5515	0.31%	0.024%
36	13.416	1751	1756	1761	rBV4	10633	19157	1.07%	0.085%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
 Data File : BP017848.D
 Acq On : 01 Nov 2023 10:31
 Operator : MA/JU
 Sample : PB156550BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK550

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Title : SVOA CALIBRATION

37	13.469	1761	1765	1773	rVB4	5225	10013	0.56%	0.044%
38	13.793	1816	1820	1823	rBV6	2301	2974	0.17%	0.013%
39	13.998	1849	1855	1871	rBV	599379	863142	48.20%	3.827%
40	14.104	1871	1873	1876	rVB4	2026	1920	0.11%	0.009%
41	14.228	1887	1894	1896	rBV7	2414	4547	0.25%	0.020%
42	14.281	1896	1903	1917	rVV	643044	972164	54.29%	4.311%
43	14.522	1940	1944	1947	rBV6	1377	2125	0.12%	0.009%
44	14.581	1947	1954	1962	rVV	921492	1331552	74.36%	5.904%
45	14.645	1962	1965	1971	rVB3	9634	15700	0.88%	0.070%
46	14.851	1991	2000	2021	rBV3	63689	261628	14.61%	1.160%
47	15.004	2021	2026	2035	rVB5	10645	27917	1.56%	0.124%
48	15.222	2059	2063	2069	rVB9	6104	9253	0.52%	0.041%
49	15.375	2085	2089	2091	rBV4	3300	4536	0.25%	0.020%
50	15.410	2092	2095	2101	rVB3	8444	12121	0.68%	0.054%
51	15.587	2119	2125	2132	rBV	1000102	1428992	79.81%	6.336%
52	15.639	2132	2134	2142	rVB2	20567	30758	1.72%	0.136%
53	15.739	2144	2151	2161	rBV	165036	286852	16.02%	1.272%
54	15.828	2164	2166	2171	rVV6	7613	13990	0.78%	0.062%
55	15.875	2171	2174	2179	rVB3	8105	13165	0.74%	0.058%
56	16.245	2234	2237	2239	rBV4	1751	2152	0.12%	0.010%
57	16.486	2273	2278	2279	rBV5	2452	4150	0.23%	0.018%
58	16.545	2285	2288	2294	rVB6	5436	8229	0.46%	0.036%
59	16.622	2298	2301	2309	rVB8	9251	16607	0.93%	0.074%
60	16.910	2347	2350	2352	rBV3	1511	1945	0.11%	0.009%
61	17.022	2366	2369	2370	rBV2	3075	3824	0.21%	0.017%
62	17.169	2391	2394	2397	rVB5	2742	3944	0.22%	0.017%
63	17.198	2397	2399	2403	rVB4	2338	1974	0.11%	0.009%
64	17.375	2423	2429	2435	rBV	1285227	1725531	96.37%	7.651%
65	17.475	2440	2446	2464	rVB2	1004372	1502932	83.94%	6.664%
66	17.681	2478	2481	2482	rBV3	1572	1918	0.11%	0.009%
67	17.969	2528	2530	2532	rVB3	2735	1918	0.11%	0.009%
68	18.045	2539	2543	2544	rBV4	2459	1881	0.11%	0.008%
69	18.316	2586	2589	2594	rBV2	7667	13213	0.74%	0.059%
70	19.310	2753	2758	2762	rBV5	13353	20879	1.17%	0.093%
71	19.380	2766	2770	2773	rBV	20269	29810	1.66%	0.132%
72	19.733	2825	2830	2840	rBV	1248555	1744204	97.41%	7.734%
73	21.522	3129	3134	3144	rBV	1324791	1785406	99.71%	7.917%
74	23.910	3534	3540	3555	rVB	818223	1617860	90.35%	7.174%
75	24.080	3562	3569	3582	rVB	856497	1790581	100.00%	7.940%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
Data File : BP017848.D
Acq On : 01 Nov 2023 10:31
Operator : MA/JU
Sample : PB156550BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK550

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Title : SVOA CALIBRATION


Sum of corrected areas: 22552625

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
Data File : BP017848.D
Acq On : 01 Nov 2023 10:31
Operator : MA/JU
Sample : PB156550BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK550

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

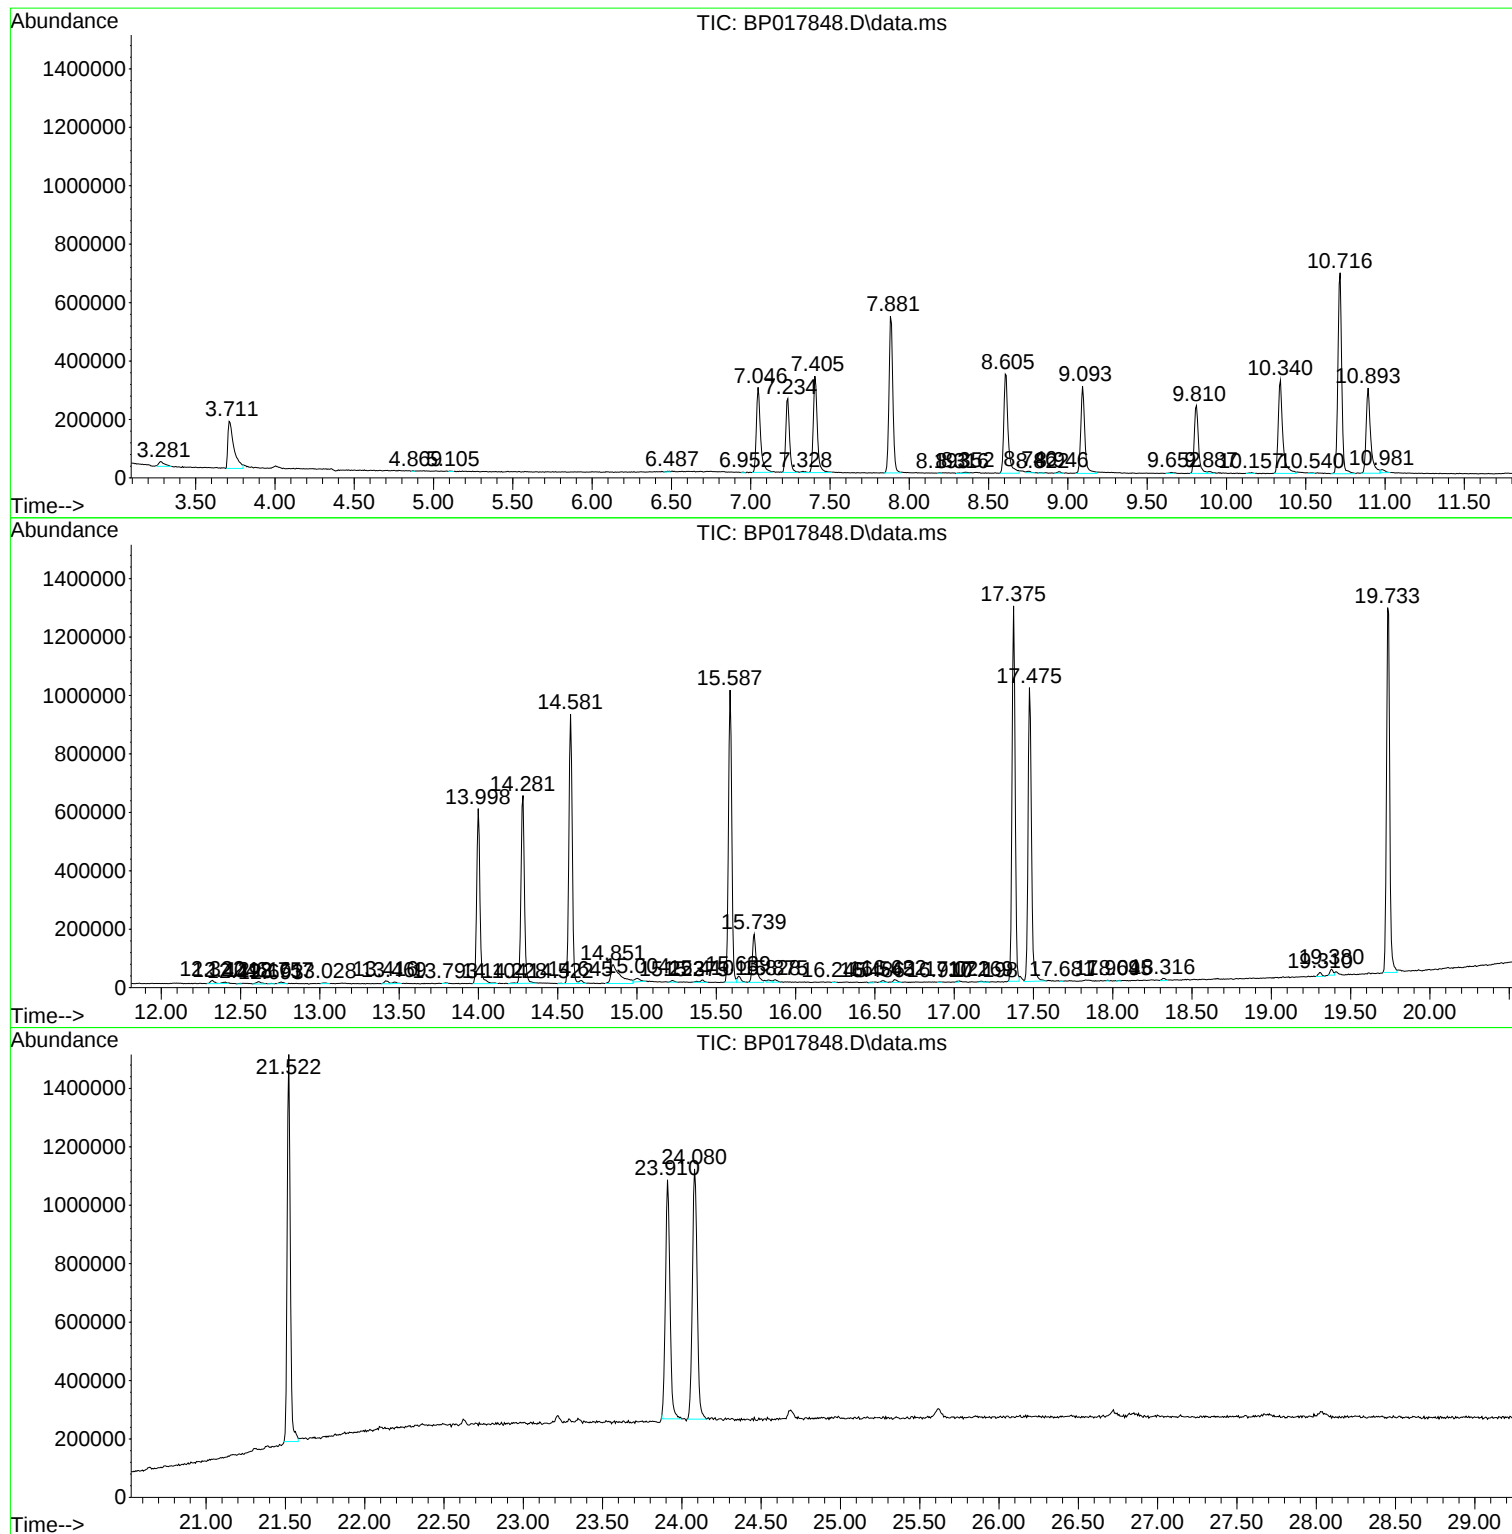

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
Data File : BP017848.D
Acq On : 01 Nov 2023 10:31
Operator : MA/JU
Sample : PB156550BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK550

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
Data File : BP017848.D
Acq On : 01 Nov 2023 10:31
Operator : MA/JU
Sample : PB156550BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK550

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc