

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
 Data File : BP017857.D
 Acq On : 01 Nov 2023 19:29
 Operator : MA/JU
 Sample : PB156542BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK542

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017857.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	27	32	41	rVB	26088	55232	2.04%	0.166%
2	3.705	101	105	132	rBV	295717	744364	27.48%	2.239%
3	3.999	150	155	163	rVB2	18323	37339	1.38%	0.112%
4	5.440	399	400	404	rBV4	3020	2833	0.10%	0.009%
5	5.858	469	471	474	rBV3	2257	2730	0.10%	0.008%
6	5.899	476	478	482	rVB5	2311	2894	0.11%	0.009%
7	7.040	666	672	688	rBV	574542	1022570	37.76%	3.076%
8	7.228	696	704	716	rBV	477772	780379	28.81%	2.347%
9	7.399	727	733	749	rBV	650599	1091336	40.29%	3.282%
10	7.875	807	814	828	rBV	622389	1026250	37.89%	3.087%
11	8.063	842	846	848	rVB4	2481	2777	0.10%	0.008%
12	8.504	918	921	923	rBV4	2715	3451	0.13%	0.010%
13	8.604	931	938	951	rBV	694455	1222668	45.14%	3.677%
14	9.087	1012	1020	1034	rBV	601421	995249	36.75%	2.993%
15	9.798	1134	1141	1153	rBV	510406	879733	32.48%	2.646%
16	10.328	1224	1231	1250	rBV	664306	1258840	46.48%	3.786%
17	10.510	1260	1262	1268	rVB7	1885	2867	0.11%	0.009%
18	10.710	1287	1296	1307	rVB	790701	1304347	48.16%	3.923%
19	10.887	1315	1326	1344	rBV	596257	1145333	42.29%	3.445%
20	12.316	1563	1569	1578	rVV3	8215	19612	0.72%	0.059%
21	13.151	1706	1711	1714	rBV7	1950	2867	0.11%	0.009%
22	13.410	1750	1755	1764	rBV10	8433	15223	0.56%	0.046%
23	13.992	1848	1854	1865	rBV	1190254	1640783	60.58%	4.935%
24	14.275	1894	1902	1915	rBV	1292054	1914383	70.68%	5.758%
25	14.575	1945	1953	1965	rBV	1074471	1558498	57.54%	4.688%
26	14.775	1984	1987	1990	rBV5	2204	3186	0.12%	0.010%
27	14.834	1990	1997	2021	rBV	238346	615991	22.74%	1.853%
28	15.581	2117	2124	2136	rBV	1596195	2301129	84.96%	6.921%
29	15.728	2143	2149	2161	rBV	446004	664533	24.54%	1.999%
30	15.822	2162	2165	2173	rVB9	9144	16477	0.61%	0.050%
31	16.633	2296	2303	2305	rBV8	2540	4025	0.15%	0.012%
32	17.033	2368	2371	2376	rVB7	3167	5087	0.19%	0.015%
33	17.157	2387	2392	2396	rBV7	3603	6681	0.25%	0.020%
34	17.369	2422	2428	2437	rBV	1290508	1767471	65.26%	5.316%
35	17.469	2439	2445	2461	rVB	1786338	2451630	90.52%	7.374%
36	17.822	2503	2505	2510	rVB6	2325	2766	0.10%	0.008%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
 Data File : BP017857.D
 Acq On : 01 Nov 2023 19:29
 Operator : MA/JU
 Sample : PB156542BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK542

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Title : SVOA CALIBRATION

37	18.010	2533	2537	2541	rBV7	3567	5245	0.19%	0.016%
38	18.116	2552	2555	2559	rBV6	2577	3262	0.12%	0.010%
39	18.222	2571	2573	2575	rBV3	3438	3516	0.13%	0.011%
40	18.780	2665	2668	2670	rBV4	2531	3841	0.14%	0.012%
41	19.304	2753	2757	2763	rVB4	18816	26414	0.98%	0.079%
42	19.374	2766	2769	2774	rVB	17899	23459	0.87%	0.071%
43	19.610	2806	2809	2813	rBV5	5257	8051	0.30%	0.024%
44	19.733	2824	2830	2839	rBV	2198608	2708394	100.00%	8.146%
45	21.516	3128	3133	3142	rBV	1267721	1713678	63.27%	5.154%
46	23.904	3532	3539	3549	rBV2	1216467	2450831	90.49%	7.371%
47	24.074	3561	3568	3584	rVB	791558	1729301	63.85%	5.201%




Sum of corrected areas: 33247526

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
Data File : BP017857.D
Acq On : 01 Nov 2023 19:29
Operator : MA/JU
Sample : PB156542BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK542

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

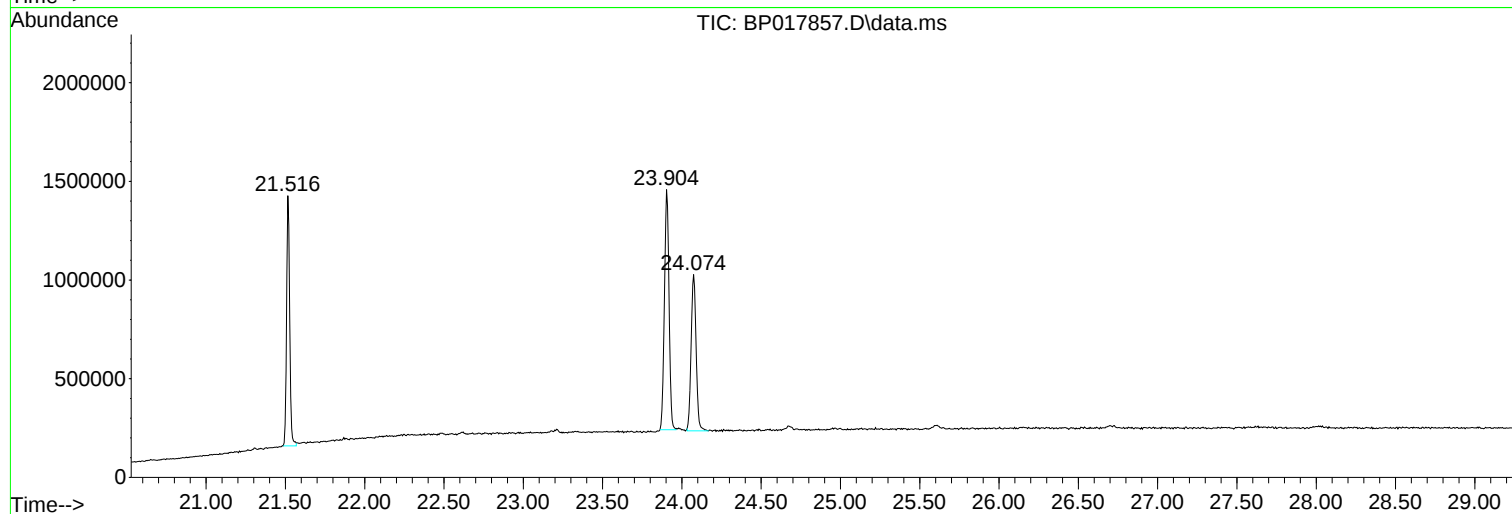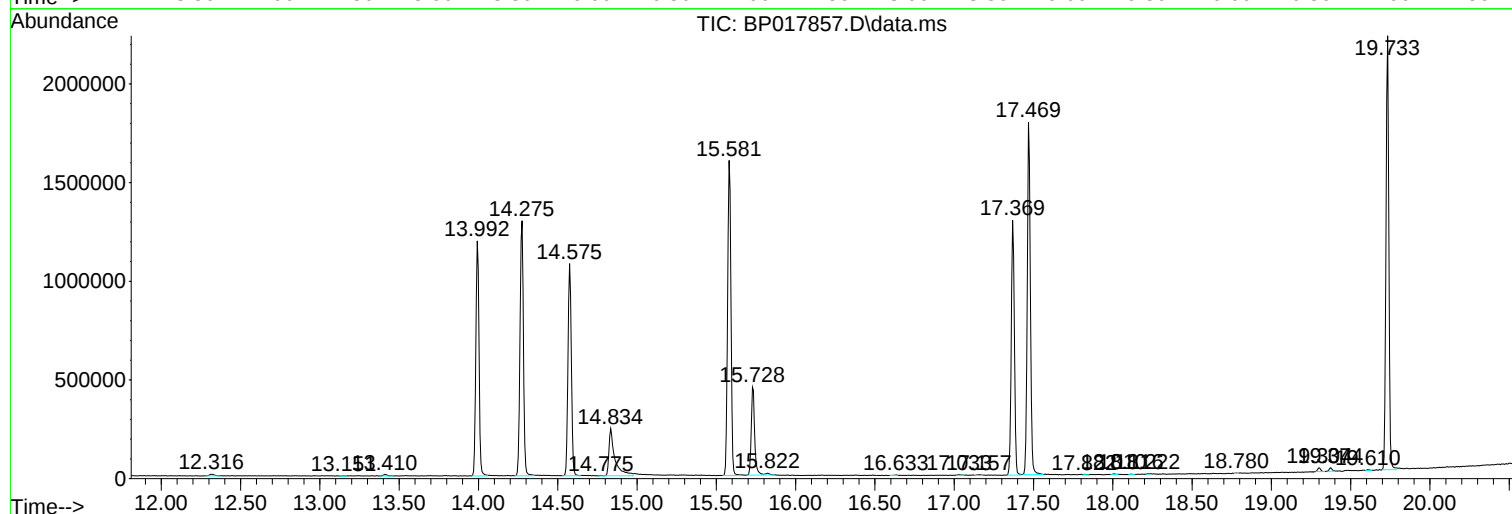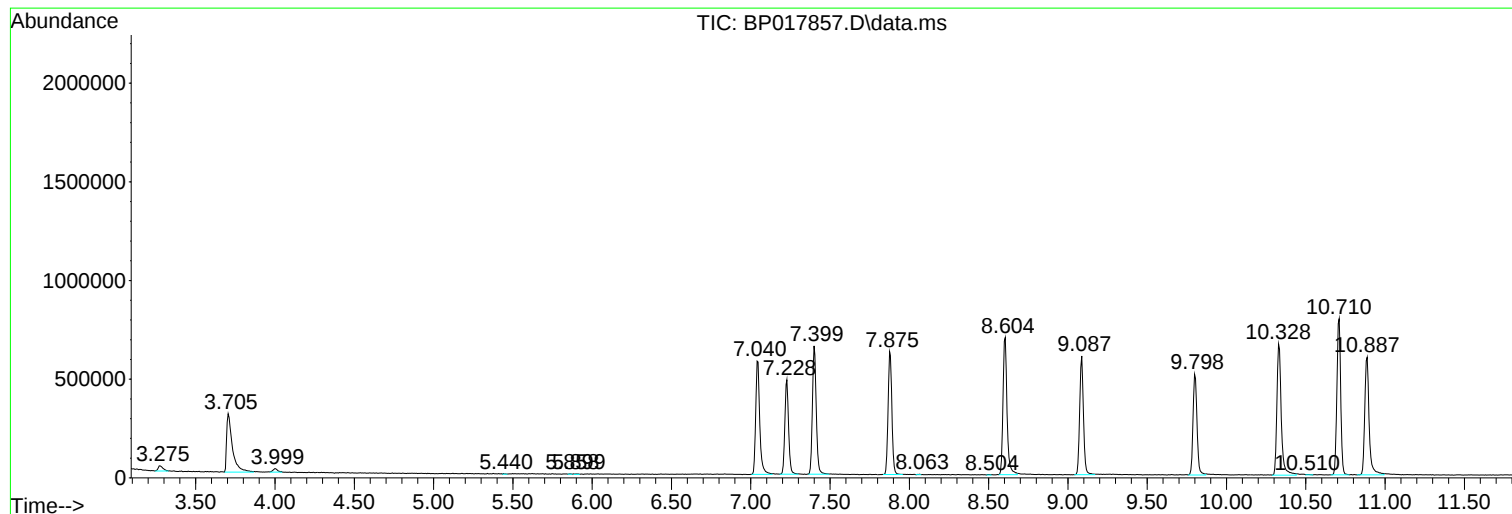

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
Data File : BP017857.D
Acq On : 01 Nov 2023 19:29
Operator : MA/JU
Sample : PB156542BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK542

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
Data File : BP017857.D
Acq On : 01 Nov 2023 19:29
Operator : MA/JU
Sample : PB156542BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK542

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------