

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
 Data File : BP017858.D
 Acq On : 01 Nov 2023 20:03
 Operator : MA/JU
 Sample : PB156543BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK543

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017858.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.276	27	32	41	rVB	26883	55971	2.03%	0.178%
2	3.705	101	105	127	rBV	303286	740696	26.85%	2.353%
3	4.005	151	156	165	rVB2	17822	39486	1.43%	0.125%
4	5.128	345	347	350	rVB4	2388	2895	0.10%	0.009%
5	5.799	456	461	462	rBV5	2134	2885	0.10%	0.009%
6	7.040	666	672	687	rBV	594771	1047317	37.97%	3.327%
7	7.228	698	704	715	rVB	487112	792121	28.72%	2.516%
8	7.399	726	733	747	rBV	658939	1114568	40.41%	3.541%
9	7.875	807	814	824	rBV	461201	775115	28.10%	2.462%
10	8.605	929	938	953	rBV	716474	1259010	45.64%	3.999%
11	9.087	1012	1020	1034	rBV	605096	1023670	37.11%	3.252%
12	9.410	1070	1075	1077	rVB6	2273	2898	0.11%	0.009%
13	9.799	1131	1141	1152	rBV	532595	903942	32.77%	2.871%
14	10.328	1224	1231	1253	rBV	689745	1289527	46.75%	4.096%
15	10.710	1289	1296	1305	rBV	586784	973001	35.27%	3.091%
16	10.887	1318	1326	1344	rBV	601677	1170871	42.45%	3.719%
17	11.587	1443	1445	1452	rVB8	1722	3070	0.11%	0.010%
18	12.316	1564	1569	1578	rBV4	10072	21190	0.77%	0.067%
19	13.416	1751	1756	1759	rBV5	7843	12278	0.45%	0.039%
20	13.993	1848	1854	1865	rBV	1211161	1679837	60.90%	5.336%
21	14.275	1892	1902	1915	rBV	1379695	1971668	71.48%	6.263%
22	14.575	1944	1953	1962	rBV	811155	1161453	42.11%	3.690%
23	14.640	1962	1964	1969	rVB5	2793	3824	0.14%	0.012%
24	14.834	1991	1997	2019	rBV	255412	621027	22.51%	1.973%
25	15.581	2117	2124	2133	rBV	1728322	2352845	85.30%	7.474%
26	15.728	2143	2149	2161	rBV	474000	710660	25.76%	2.258%
27	15.822	2161	2165	2174	rVB9	10420	21044	0.76%	0.067%
28	17.028	2368	2370	2374	rBV4	2857	3647	0.13%	0.012%
29	17.157	2390	2392	2396	rBV4	2862	4032	0.15%	0.013%
30	17.369	2421	2428	2438	rBV	935313	1303245	47.25%	4.140%
31	17.469	2438	2445	2463	rVV	1778017	2507220	90.90%	7.965%
32	17.922	2520	2522	2525	rBV4	1904	2762	0.10%	0.009%
33	18.010	2533	2537	2538	rBV4	3922	4076	0.15%	0.013%
34	18.239	2569	2576	2579	rBV8	4494	10913	0.40%	0.035%
35	19.298	2752	2756	2763	rBV5	19473	29799	1.08%	0.095%
36	19.375	2765	2769	2773	rVB2	14767	20827	0.76%	0.066%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
Data File : BP017858.D
Acq On : 01 Nov 2023 20:03
Operator : MA/JU
Sample : PB156543BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK543

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Title : SVOA CALIBRATION

37	19.733	2824	2830	2840	rBV	2145777	2758334	100.00%	8.762%
38	21.516	3128	3133	3145	rBV	944402	1291672	46.83%	4.103%
39	23.904	3531	3539	3553	rVB2	1198777	2540601	92.11%	8.071%
40	24.074	3561	3568	3578	rVB	594185	1249791	45.31%	3.970%




Sum of corrected areas: 31479788

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
Data File : BP017858.D
Acq On : 01 Nov 2023 20:03
Operator : MA/JU
Sample : PB156543BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK543

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

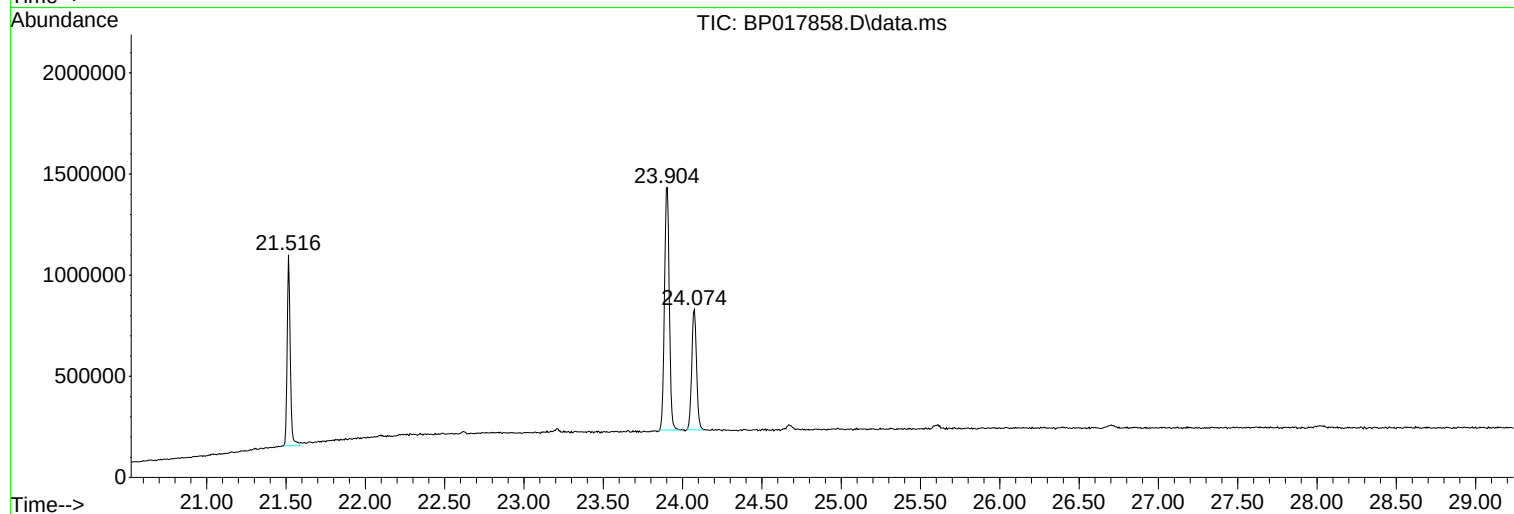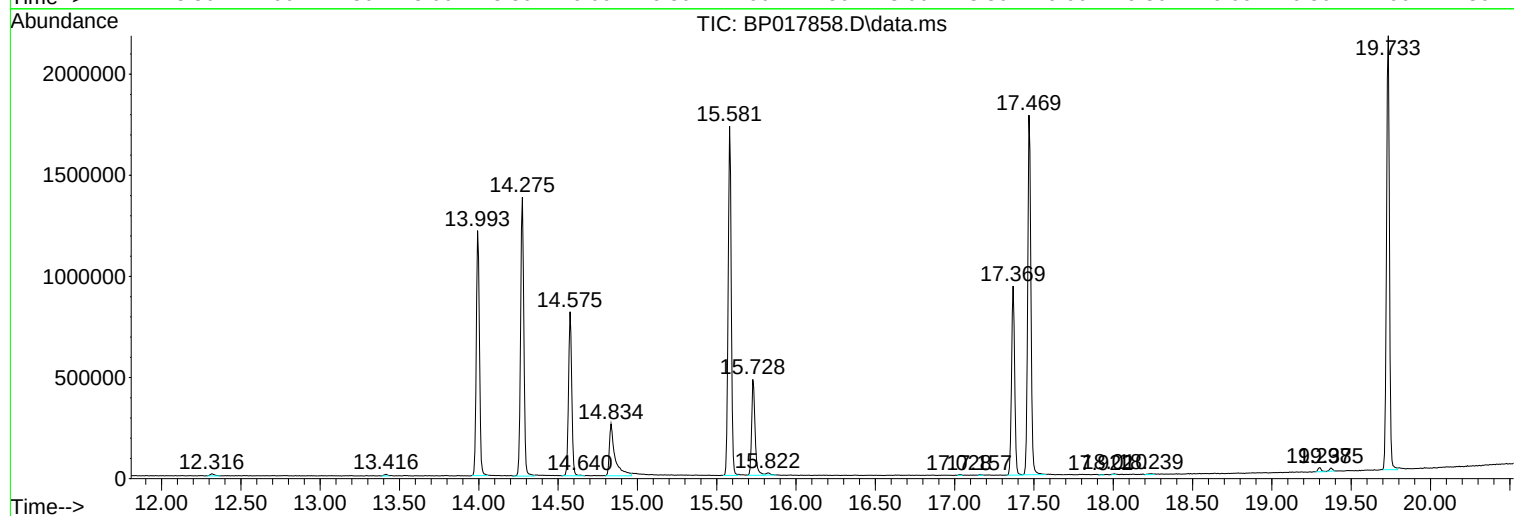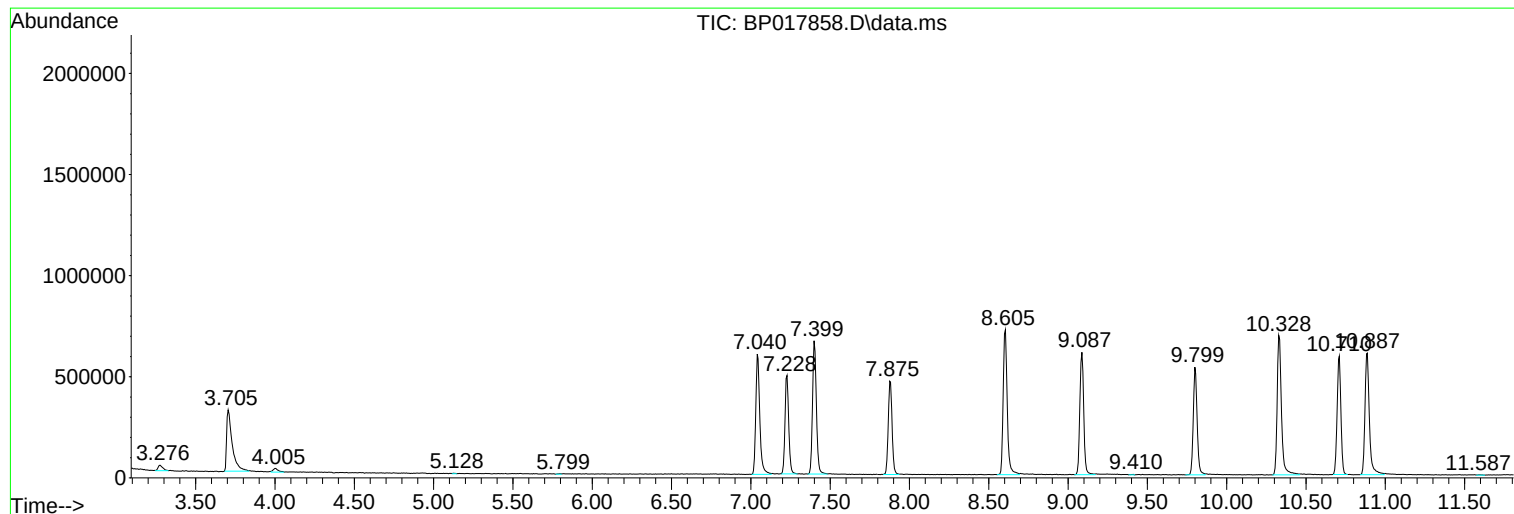

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
Data File : BP017858.D
Acq On : 01 Nov 2023 20:03
Operator : MA/JU
Sample : PB156543BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK543

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
Data File : BP017858.D
Acq On : 01 Nov 2023 20:03
Operator : MA/JU
Sample : PB156543BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK543

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------