

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
 Data File : BP017874.D
 Acq On : 02 Nov 2023 05:37
 Operator : MA/JU
 Sample : PB156564BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK564

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017874.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	27	32	40	rBV	37790	75645	2.04%	0.177%
2	3.705	101	105	128	rBV	428441	1105453	29.75%	2.593%
3	4.405	220	224	225	rBV3	4987	6955	0.19%	0.016%
4	7.040	665	672	691	rBV	798531	1372131	36.93%	3.218%
5	7.222	697	703	718	rVB	667387	1084743	29.20%	2.544%
6	7.399	726	733	745	rBV	913749	1512044	40.70%	3.546%
7	7.875	807	814	826	rBV	659546	1068221	28.75%	2.505%
8	8.599	929	937	955	rBV	987859	1696063	45.65%	3.978%
9	9.081	1009	1019	1031	rBV	824729	1379631	37.13%	3.236%
10	9.799	1132	1141	1154	rBV	704032	1192754	32.10%	2.798%
11	10.328	1223	1231	1252	rBV	939556	1712499	46.09%	4.017%
12	10.704	1287	1295	1307	rBV	850703	1357338	36.53%	3.184%
13	10.881	1318	1325	1343	rBV	901065	1612487	43.40%	3.782%
14	12.310	1563	1568	1579	rVB2	12861	25152	0.68%	0.059%
15	13.410	1748	1755	1762	rBV5	12066	22345	0.60%	0.052%
16	13.528	1770	1775	1782	rVB10	3017	7492	0.20%	0.018%
17	13.992	1846	1854	1867	rBV	1625409	2270895	61.12%	5.326%
18	14.269	1894	1901	1917	rBV	1864693	2726522	73.39%	6.395%
19	14.575	1946	1953	1964	rVB	1085082	1611387	43.37%	3.779%
20	14.828	1989	1996	2020	rBV	389493	888468	23.91%	2.084%
21	15.581	2117	2124	2134	rBV	2255391	3199652	86.12%	7.505%
22	15.728	2143	2149	2161	rBV	646381	911350	24.53%	2.138%
23	15.816	2161	2164	2170	rVB5	11238	18279	0.49%	0.043%
24	17.028	2366	2370	2374	rVB7	3380	5003	0.13%	0.012%
25	17.157	2388	2392	2397	rVB7	3954	7392	0.20%	0.017%
26	17.363	2421	2427	2438	rBV	1317371	1796393	48.35%	4.213%
27	17.469	2438	2445	2457	rBV2	2260320	3300690	88.84%	7.742%
28	17.680	2476	2481	2483	rBV6	2771	4135	0.11%	0.010%
29	18.227	2571	2574	2577	rVB5	4480	4760	0.13%	0.011%
30	18.498	2618	2620	2624	rVB5	2856	4054	0.11%	0.010%
31	18.780	2663	2668	2671	rBV7	3384	6618	0.18%	0.016%
32	18.880	2682	2685	2687	rBV4	3149	4162	0.11%	0.010%
33	19.298	2751	2756	2761	rBV2	29139	40368	1.09%	0.095%
34	19.369	2764	2768	2773	rVB2	20051	30108	0.81%	0.071%
35	19.604	2805	2808	2812	rBV4	12384	15553	0.42%	0.036%
36	19.727	2823	2829	2840	rBV	2843553	3715239	100.00%	8.714%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
Data File : BP017874.D
Acq On : 02 Nov 2023 05:37
Operator : MA/JU
Sample : PB156564BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK564

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Title : SVOA CALIBRATION

37	20.639	2981	2984	2987	rBV4	20925	21059	0.57%	0.049%
38	21.510	3127	3132	3143	rBV2	1260408	1737065	46.76%	4.074%
39	23.898	3530	3538	3549	rVB2	1610500	3386439	91.15%	7.943%
40	24.068	3560	3567	3578	rVB	808193	1699348	45.74%	3.986%




Sum of corrected areas: 42635892

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
Data File : BP017874.D
Acq On : 02 Nov 2023 05:37
Operator : MA/JU
Sample : PB156564BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK564

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

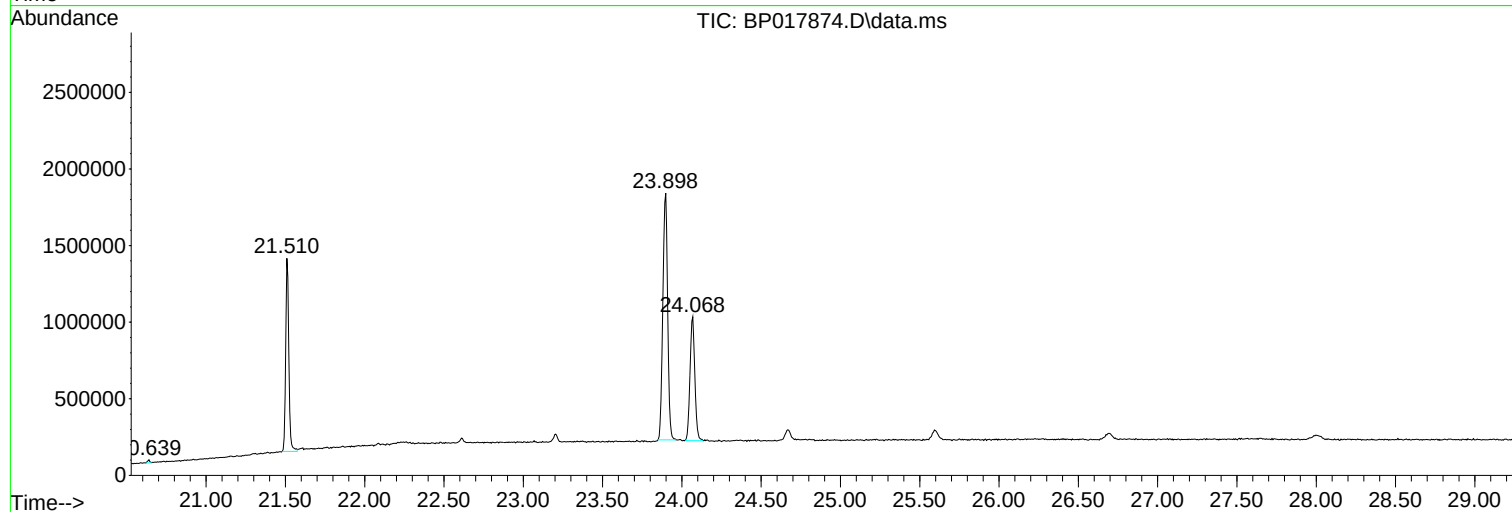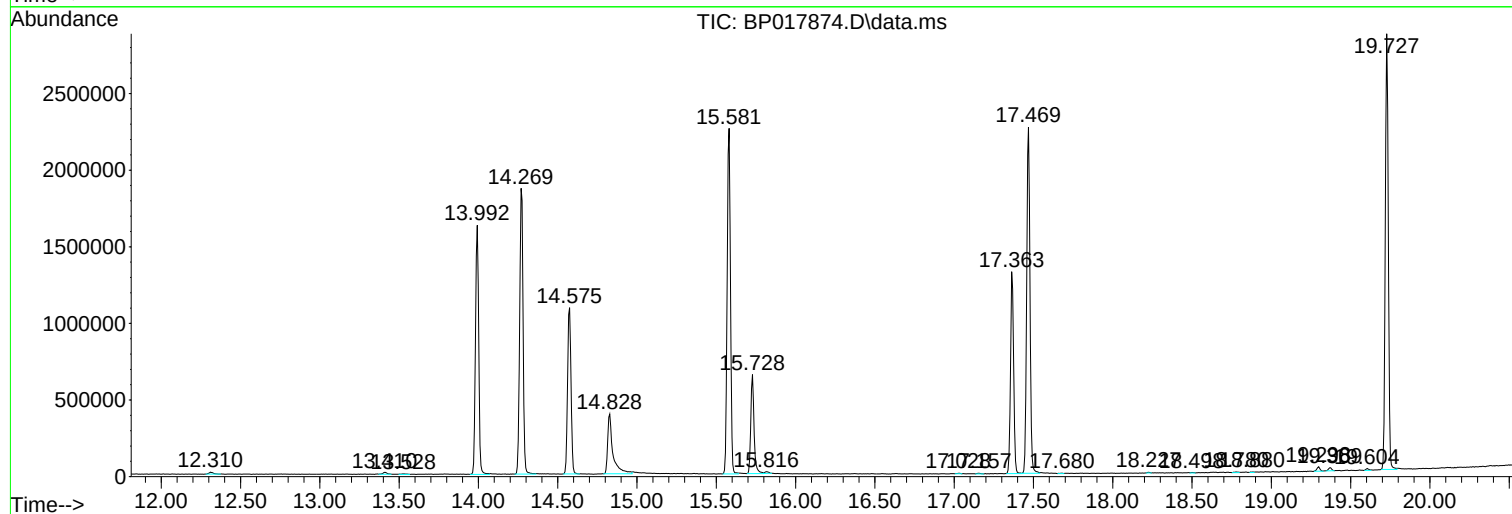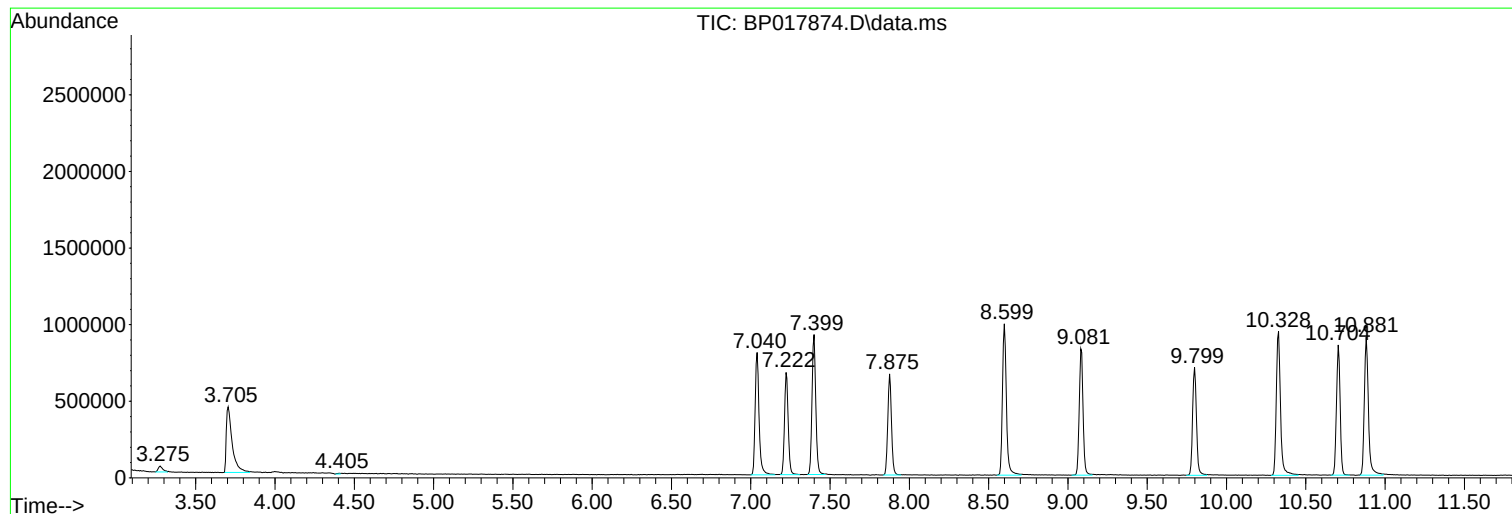

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
Data File : BP017874.D
Acq On : 02 Nov 2023 05:37
Operator : MA/JU
Sample : PB156564BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK564

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
Data File : BP017874.D
Acq On : 02 Nov 2023 05:37
Operator : MA/JU
Sample : PB156564BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK564

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc