

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
 Data File : BP017883.D
 Acq On : 02 Nov 2023 13:17
 Operator : MA/JU
 Sample : PB156594BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK594

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017883.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	28	31	46	rVB	37328	92270	2.76%	0.247%
2	3.699	100	104	127	rVB	337751	794058	23.79%	2.123%
3	3.993	151	154	161	rVB	16646	30466	0.91%	0.081%
4	5.487	406	408	412	rVB5	3592	3857	0.12%	0.010%
5	7.040	665	672	684	rBV	688447	1193422	35.76%	3.190%
6	7.222	697	703	714	rBV	549634	882869	26.45%	2.360%
7	7.399	726	733	745	rBV	771265	1287770	38.58%	3.442%
8	7.875	808	814	823	rVV	564788	902424	27.04%	2.412%
9	8.599	929	937	952	rBV	858274	1464527	43.88%	3.915%
10	9.081	1012	1019	1032	rBV	690726	1175633	35.23%	3.142%
11	9.499	1087	1090	1094	rVB5	2854	5061	0.15%	0.014%
12	9.799	1134	1141	1154	rBV	634249	1051131	31.49%	2.810%
13	10.328	1222	1231	1251	rBV	836052	1528187	45.79%	4.085%
14	10.704	1287	1295	1304	rBV	696566	1173617	35.16%	3.137%
15	10.881	1317	1325	1351	rBV	747633	1397167	41.86%	3.735%
16	11.040	1351	1352	1358	rVB6	4666	6127	0.18%	0.016%
17	11.751	1471	1473	1478	rBV6	2446	4076	0.12%	0.011%
18	12.310	1561	1568	1573	rBV4	11796	26257	0.79%	0.070%
19	12.528	1601	1605	1606	rBV4	3247	4031	0.12%	0.011%
20	12.604	1613	1618	1620	rBV6	2709	3483	0.10%	0.009%
21	13.404	1746	1754	1761	rBV4	13632	25106	0.75%	0.067%
22	13.528	1772	1775	1779	rBV5	3178	4621	0.14%	0.012%
23	13.781	1817	1818	1825	rVB7	2170	3580	0.11%	0.010%
24	13.992	1846	1854	1863	rBV	1446782	2004032	60.05%	5.357%
25	14.269	1892	1901	1917	rBV	1571123	2403346	72.01%	6.424%
26	14.575	1946	1953	1965	rBV	980168	1434363	42.98%	3.834%
27	14.828	1990	1996	2020	rBV	320289	806268	24.16%	2.155%
28	15.581	2117	2124	2134	rBV	2046106	2816226	84.38%	7.528%
29	15.728	2143	2149	2160	rBV	586036	831317	24.91%	2.222%
30	15.822	2161	2165	2172	rVV7	12128	24681	0.74%	0.066%
31	16.369	2255	2258	2264	rVB7	4218	6770	0.20%	0.018%
32	17.033	2367	2371	2373	rVB5	2604	3474	0.10%	0.009%
33	17.157	2387	2392	2394	rBV5	4435	4713	0.14%	0.013%
34	17.304	2414	2417	2421	rVB6	2168	3349	0.10%	0.009%
35	17.369	2421	2428	2438	rBV	1121192	1595463	47.80%	4.265%
36	17.469	2438	2445	2460	rVV	2180518	3007812	90.12%	8.040%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
 Data File : BP017883.D
 Acq On : 02 Nov 2023 13:17
 Operator : MA/JU
 Sample : PB156594BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK594

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Title : SVOA CALIBRATION

37	17.816	2500	2504	2507	rVB6	3313	3896	0.12%	0.010%
38	18.004	2532	2536	2538	rBV5	4103	5501	0.16%	0.015%
39	18.228	2567	2574	2575	rBV7	6845	10998	0.33%	0.029%
40	18.428	2607	2608	2611	rBV3	3037	3366	0.10%	0.009%
41	19.298	2752	2756	2760	rBV3	26566	37561	1.13%	0.100%
42	19.369	2764	2768	2775	rVB2	22401	34520	1.03%	0.092%
43	19.733	2823	2830	2838	rBV	2433335	3337495	100.00%	8.921%
44	21.516	3128	3133	3143	rBV	1154645	1539937	46.14%	4.116%
45	23.898	3531	3538	3549	rVB2	1425373	2980111	89.29%	7.966%
46	24.068	3561	3567	3576	rVB	679606	1456326	43.64%	3.893%




Sum of corrected areas: 37411265

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
Data File : BP017883.D
Acq On : 02 Nov 2023 13:17
Operator : MA/JU
Sample : PB156594BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK594

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

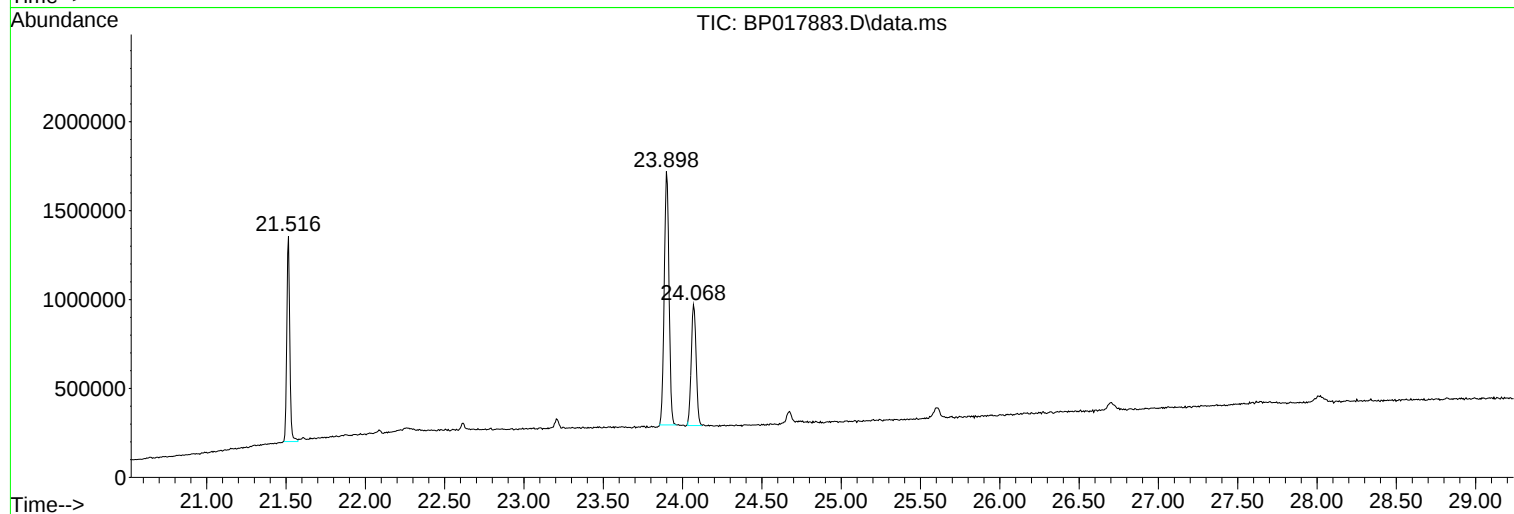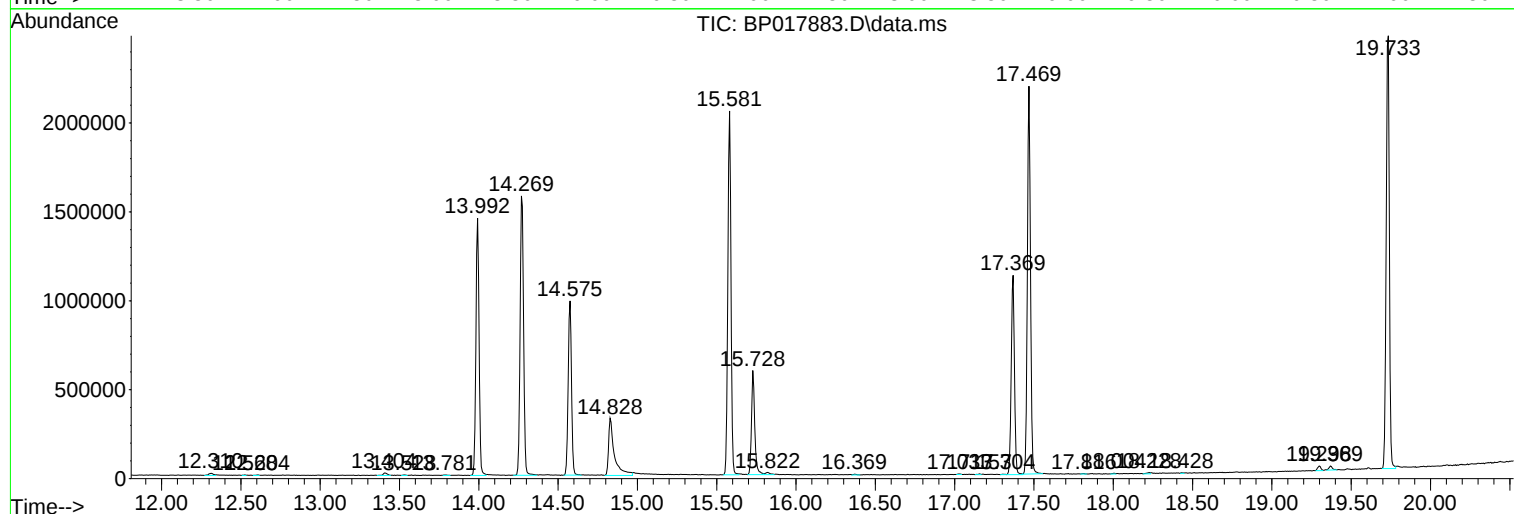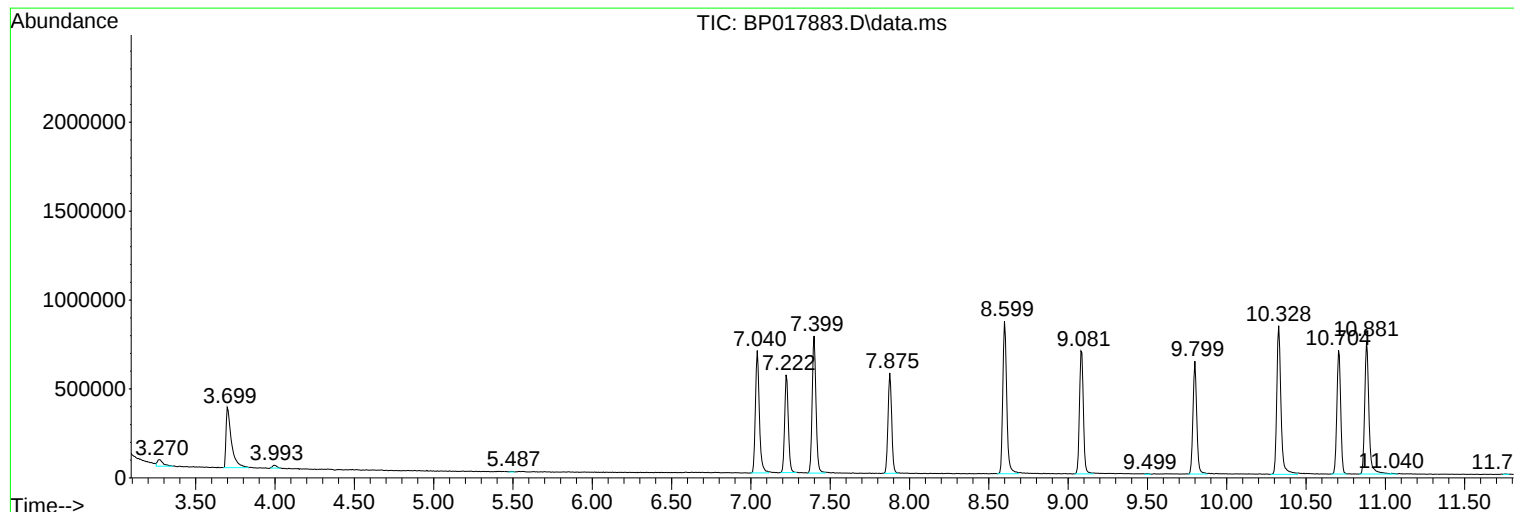

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
Data File : BP017883.D
Acq On : 02 Nov 2023 13:17
Operator : MA/JU
Sample : PB156594BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK594

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
Data File : BP017883.D
Acq On : 02 Nov 2023 13:17
Operator : MA/JU
Sample : PB156594BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK594

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------