

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
 Data File : BP017884.D
 Acq On : 02 Nov 2023 13:51
 Operator : MA/JU
 Sample : PB156595BL
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK595

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017884.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	44	rVB	38964	86719	2.61%	0.227%
2	3.699	99	104	122	rBV	339469	790995	23.77%	2.069%
3	3.993	151	154	165	rVB3	20390	42549	1.28%	0.111%
4	7.040	665	672	691	rBV	664954	1187127	35.68%	3.105%
5	7.222	697	703	717	rVB	560496	887397	26.67%	2.321%
6	7.399	726	733	745	rBV	760903	1263401	37.97%	3.304%
7	7.875	807	814	823	rBV	639214	1022730	30.74%	2.675%
8	8.599	930	937	954	rBV	862073	1448773	43.54%	3.789%
9	9.081	1011	1019	1030	rBV	690065	1172368	35.24%	3.066%
10	9.799	1133	1141	1155	rBV	623235	1056245	31.75%	2.762%
11	10.328	1224	1231	1247	rBV	823571	1500042	45.08%	3.923%
12	10.705	1288	1295	1306	rBV	801514	1328535	39.93%	3.474%
13	10.881	1318	1325	1341	rBV	740034	1345937	40.45%	3.520%
14	12.316	1560	1569	1575	rBV2	11133	22569	0.68%	0.059%
15	13.410	1750	1755	1763	rBV5	10249	17998	0.54%	0.047%
16	13.528	1772	1775	1783	rBV10	4092	8076	0.24%	0.021%
17	13.993	1846	1854	1869	rBV	1452338	2003213	60.21%	5.239%
18	14.269	1893	1901	1915	rBV	1588746	2403719	72.25%	6.286%
19	14.575	1941	1953	1964	rBV	1136241	1641344	49.33%	4.293%
20	14.828	1990	1996	2015	rBV	302421	752417	22.61%	1.968%
21	15.581	2116	2124	2135	rBV	2029731	2840424	85.37%	7.428%
22	15.728	2143	2149	2161	rBV	531730	797926	23.98%	2.087%
23	15.816	2161	2164	2171	rVB3	10480	19310	0.58%	0.051%
24	17.034	2367	2371	2376	rBV7	4459	7398	0.22%	0.019%
25	17.151	2390	2391	2397	rVB6	3333	4062	0.12%	0.011%
26	17.369	2421	2428	2436	rBV	1317664	1809631	54.39%	4.733%
27	17.469	2439	2445	2463	rVB	2180305	3030009	91.07%	7.924%
28	17.804	2498	2502	2503	rBV4	3566	4557	0.14%	0.012%
29	18.222	2570	2573	2575	rBV4	2964	4729	0.14%	0.012%
30	19.298	2752	2756	2761	rVB	25561	32238	0.97%	0.084%
31	19.369	2765	2768	2773	rVB	19819	25912	0.78%	0.068%
32	19.728	2824	2829	2838	rBV	2593579	3327168	100.00%	8.701%
33	21.516	3128	3133	3144	rBV	1247087	1725279	51.85%	4.512%
34	23.904	3531	3539	3551	rVB	1426641	3000480	90.18%	7.847%
35	24.069	3561	3567	3576	rVB	787307	1626118	48.87%	4.253%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
Data File : BP017884.D
Acq On : 02 Nov 2023 13:51
Operator : MA/JU
Sample : PB156595BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK595

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 38237395

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
Data File : BP017884.D
Acq On : 02 Nov 2023 13:51
Operator : MA/JU
Sample : PB156595BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK595

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

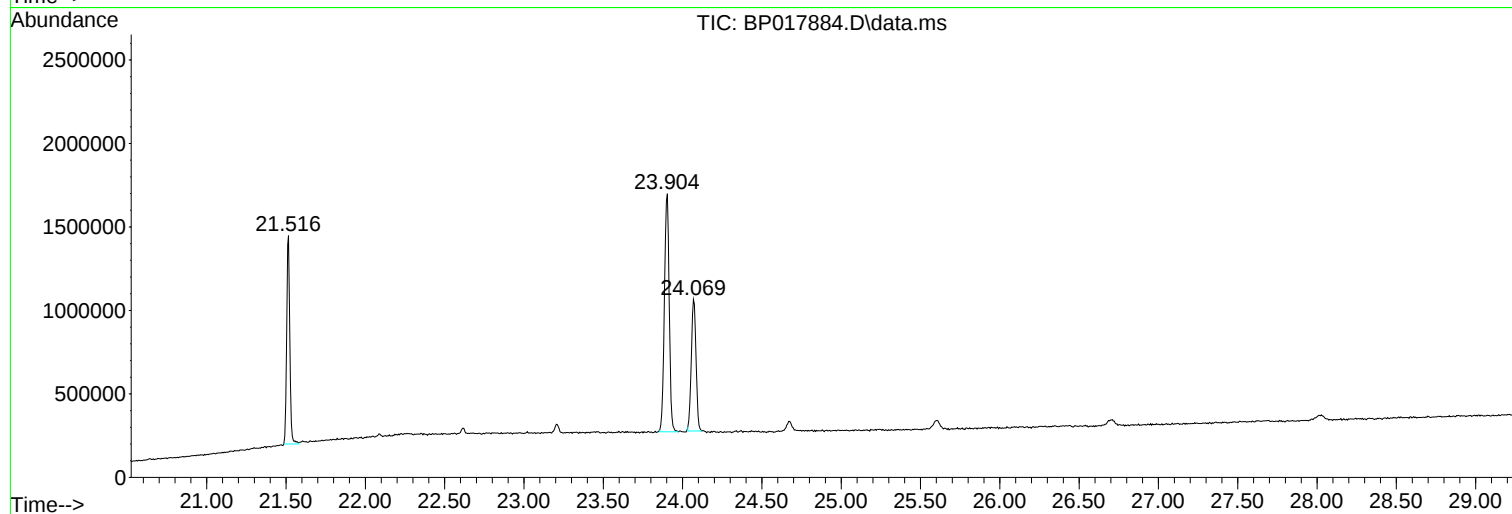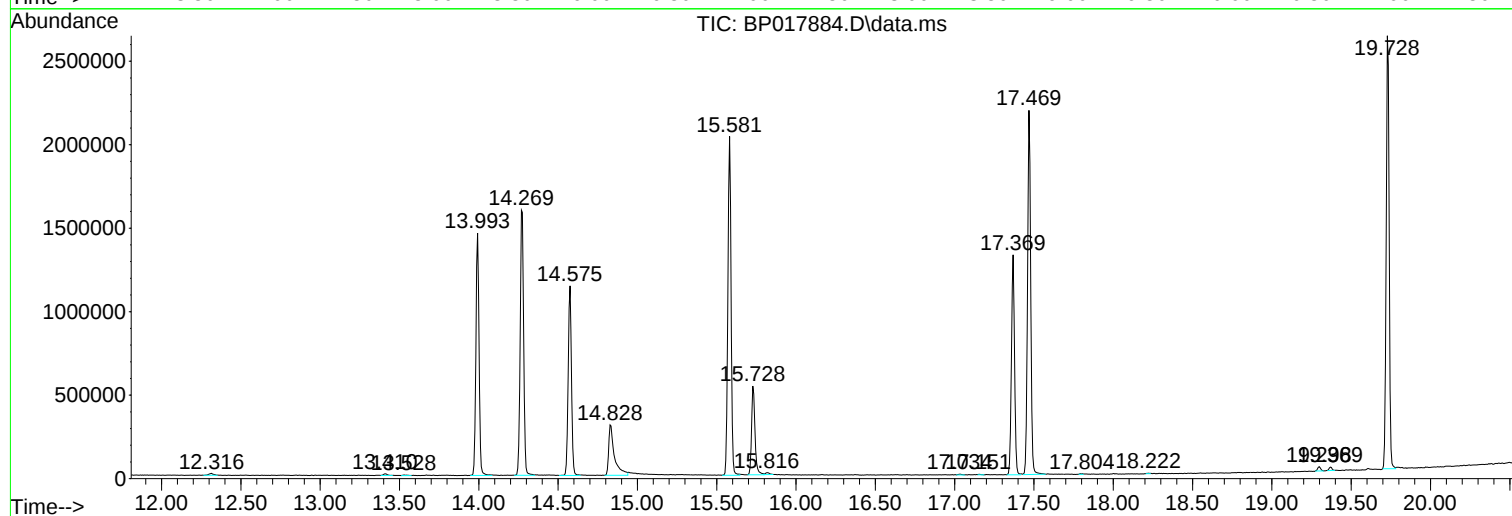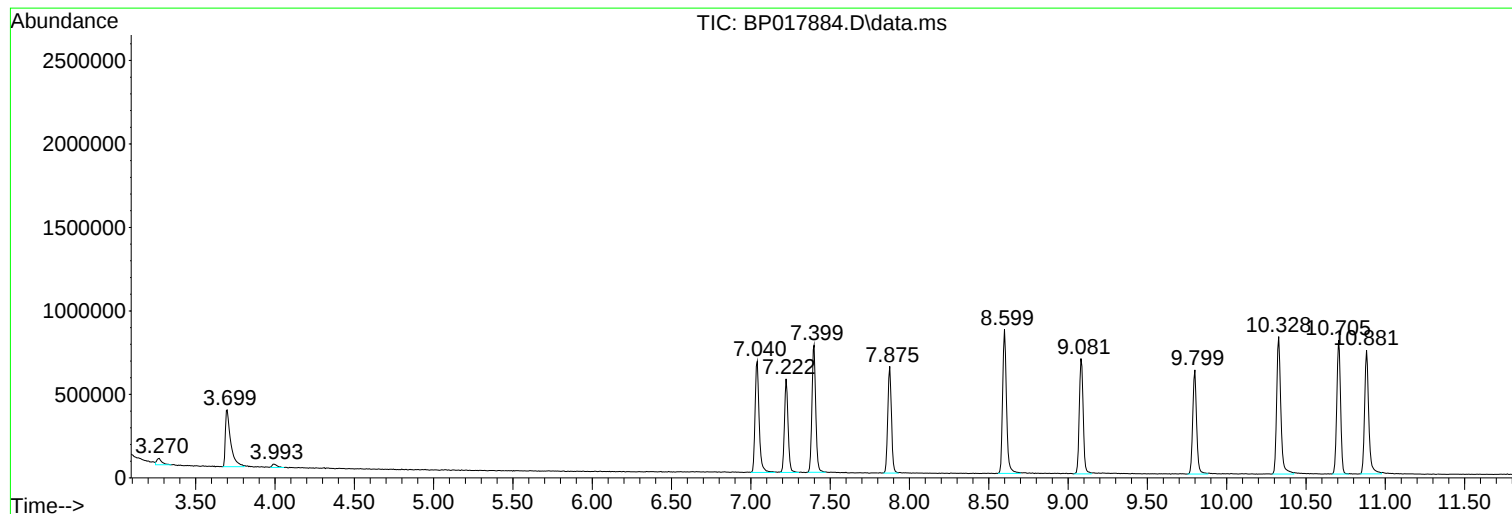

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
Data File : BP017884.D
Acq On : 02 Nov 2023 13:51
Operator : MA/JU
Sample : PB156595BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK595

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
Data File : BP017884.D
Acq On : 02 Nov 2023 13:51
Operator : MA/JU
Sample : PB156595BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK595

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc