

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
 Data File : BP017903.D
 Acq On : 03 Nov 2023 01:06
 Operator : MA/JU
 Sample : PB156797BL
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK797

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017903.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.276	28	32	45	rVB	30786	78641	2.74%	0.220%
2	3.705	100	105	125	rBV	326730	815229	28.43%	2.279%
3	3.999	151	155	161	rBV6	7128	14403	0.50%	0.040%
4	4.928	310	313	314	rBV3	2590	3146	0.11%	0.009%
5	6.246	534	537	542	rBV7	2580	3566	0.12%	0.010%
6	6.593	594	596	599	rBV4	2745	3793	0.13%	0.011%
7	6.640	603	604	608	rBV4	2913	3755	0.13%	0.010%
8	7.040	666	672	687	rBV	658948	1147069	40.00%	3.206%
9	7.222	697	703	714	rBV	518120	840004	29.29%	2.348%
10	7.399	726	733	747	rBV	752153	1221094	42.58%	3.413%
11	7.875	807	814	824	rBV	673506	1069643	37.30%	2.990%
12	8.487	914	918	921	rBV6	2136	2992	0.10%	0.008%
13	8.599	929	937	952	rBV	812993	1388405	48.41%	3.881%
14	9.087	1012	1020	1030	rBV	669432	1124563	39.21%	3.143%
15	9.799	1135	1141	1153	rBV	598448	1006703	35.10%	2.814%
16	10.328	1224	1231	1254	rBV	797543	1424118	49.66%	3.981%
17	10.705	1286	1295	1304	rBV	823263	1366855	47.66%	3.821%
18	10.881	1315	1325	1341	rBV	740826	1359228	47.40%	3.799%
19	11.716	1464	1467	1470	rBV5	1981	3054	0.11%	0.009%
20	12.063	1523	1526	1532	rBV8	2057	4063	0.14%	0.011%
21	12.305	1561	1567	1575	rBV	11673	23820	0.83%	0.067%
22	13.404	1746	1754	1761	rVB4	14068	25758	0.90%	0.072%
23	13.504	1768	1771	1772	rBV3	2495	3140	0.11%	0.009%
24	13.922	1839	1842	1844	rVB4	2484	2976	0.10%	0.008%
25	13.993	1847	1854	1864	rVV	1399273	1868279	65.15%	5.222%
26	14.063	1864	1866	1871	rVB6	2498	4132	0.14%	0.012%
27	14.151	1877	1881	1883	rVB5	2101	3089	0.11%	0.009%
28	14.275	1895	1902	1912	rBV	1483291	2211881	77.13%	6.183%
29	14.428	1925	1928	1931	rVB5	2709	3384	0.12%	0.009%
30	14.575	1946	1953	1963	rBV	1151822	1630940	56.87%	4.559%
31	14.834	1991	1997	2013	rBV	312991	727274	25.36%	2.033%
32	15.369	2083	2088	2091	rBV7	2844	3890	0.14%	0.011%
33	15.581	2115	2124	2135	rBV	1856861	2582046	90.04%	7.217%
34	15.734	2143	2150	2161	rBV	325714	471851	16.45%	1.319%
35	15.816	2161	2164	2170	rVB5	9423	15167	0.53%	0.042%
36	15.922	2178	2182	2189	rVB9	1992	4893	0.17%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
 Data File : BP017903.D
 Acq On : 03 Nov 2023 01:06
 Operator : MA/JU
 Sample : PB156797BL
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK797

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Title : SVOA CALIBRATION

37	16.157	2219	2222	2226	rBV5	2545	3798	0.13%	0.011%
38	16.634	2298	2303	2308	rBV9	1946	3705	0.13%	0.010%
39	16.681	2308	2311	2316	rVB7	2210	2954	0.10%	0.008%
40	17.157	2387	2392	2397	rBV8	5195	9431	0.33%	0.026%
41	17.369	2418	2428	2437	rBV	1280989	1817877	63.39%	5.081%
42	17.469	2439	2445	2461	rVB	1979992	2689231	93.77%	7.517%
43	17.692	2478	2483	2491	rBV	7762	22413	0.78%	0.063%
44	19.292	2752	2755	2760	rBV3	22271	26195	0.91%	0.073%
45	19.369	2764	2768	2772	rVB3	20517	28779	1.00%	0.080%
46	19.728	2824	2829	2837	rBV	2185642	2867809	100.00%	8.016%
47	21.516	3128	3133	3139	rBV	1324961	1661454	57.93%	4.644%
48	23.904	3531	3539	3548	rBV2	1244686	2561505	89.32%	7.160%
49	24.074	3561	3568	3579	rVB	772825	1617223	56.39%	4.521%




Sum of corrected areas: 35775218

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
Data File : BP017903.D
Acq On : 03 Nov 2023 01:06
Operator : MA/JU
Sample : PB156797BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK797

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

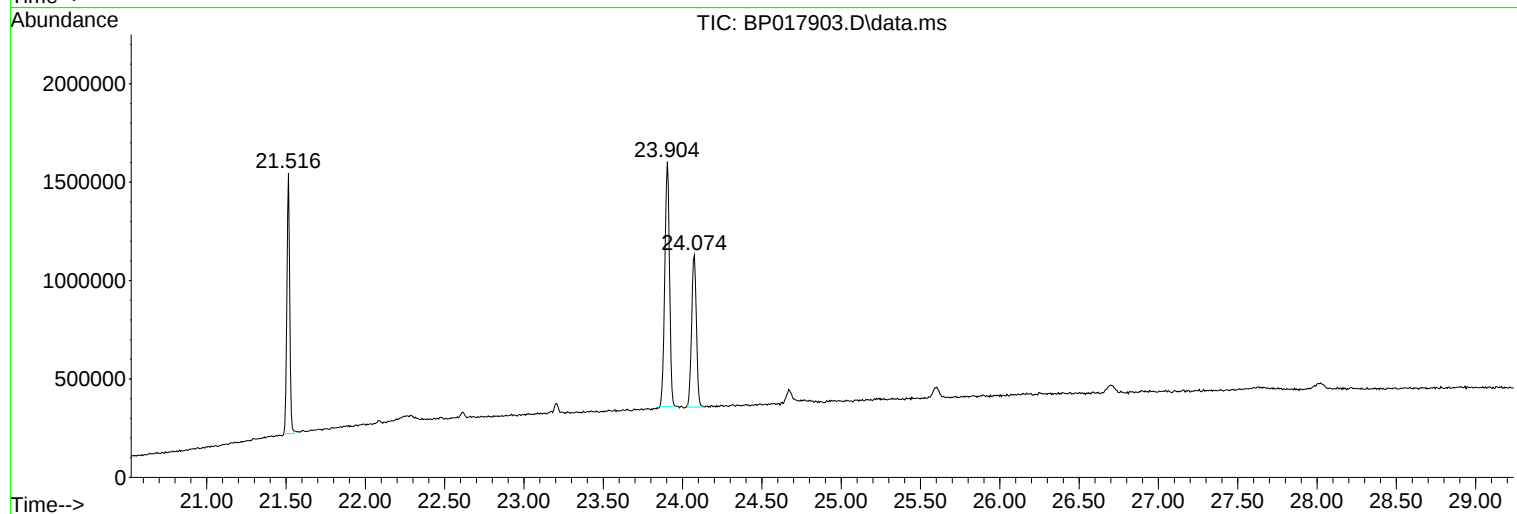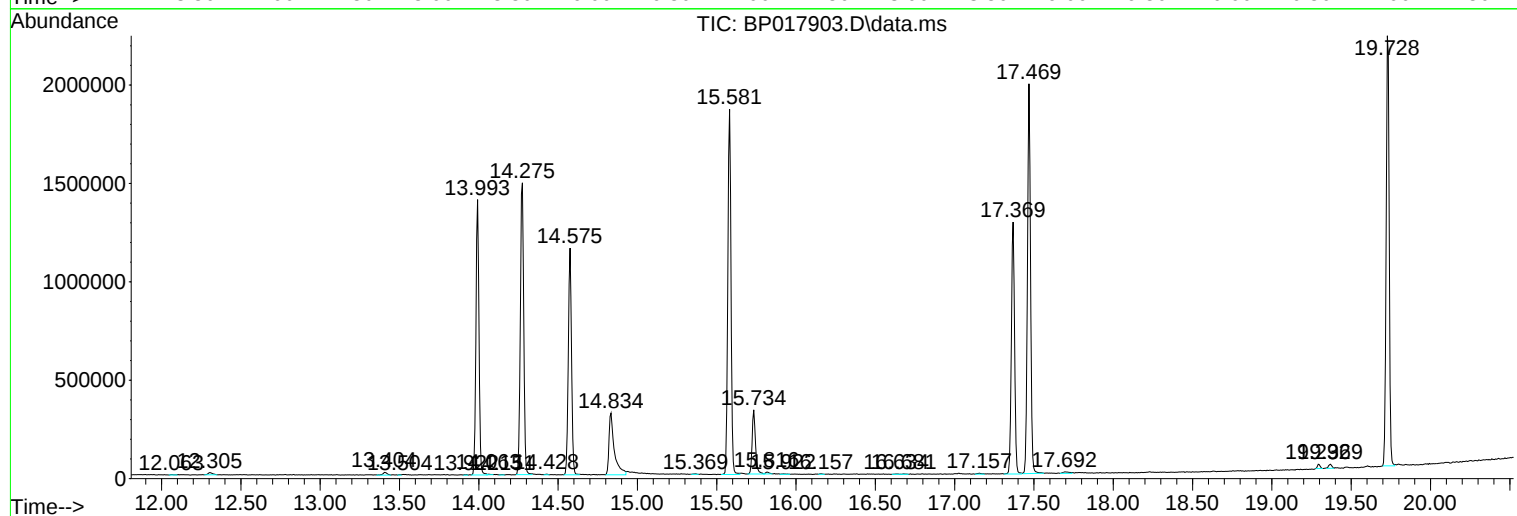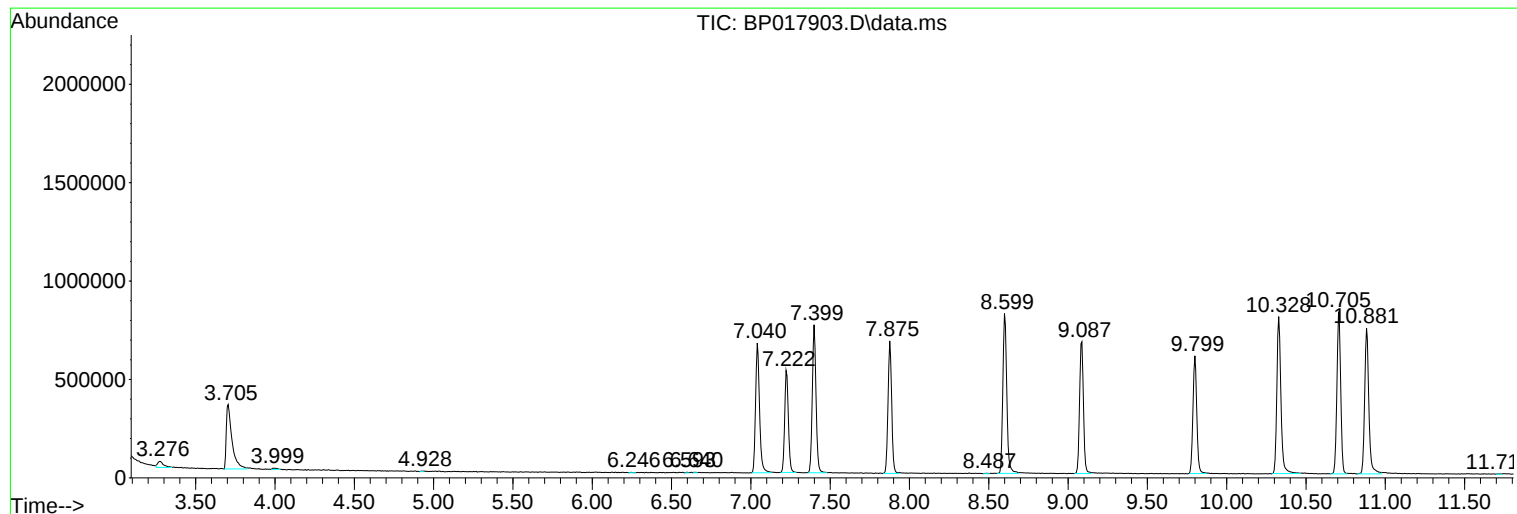

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
Data File : BP017903.D
Acq On : 03 Nov 2023 01:06
Operator : MA/JU
Sample : PB156797BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK797

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110123\
Data File : BP017903.D
Acq On : 03 Nov 2023 01:06
Operator : MA/JU
Sample : PB156797BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK797

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------