
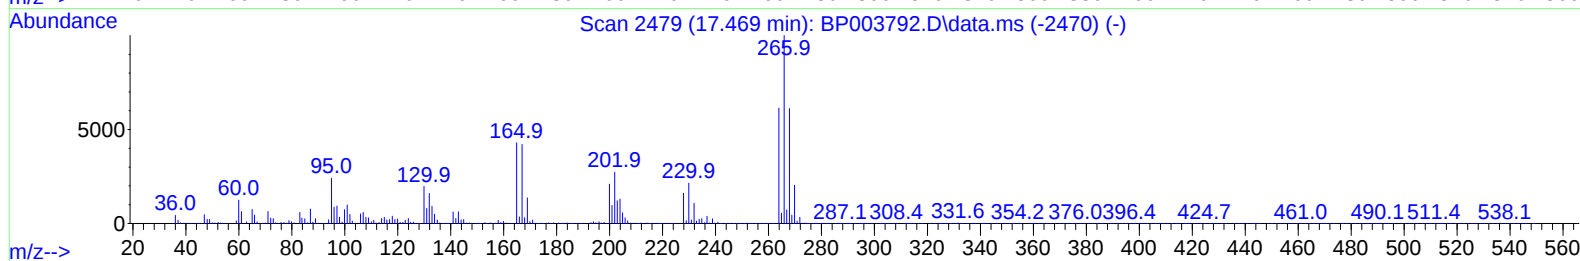
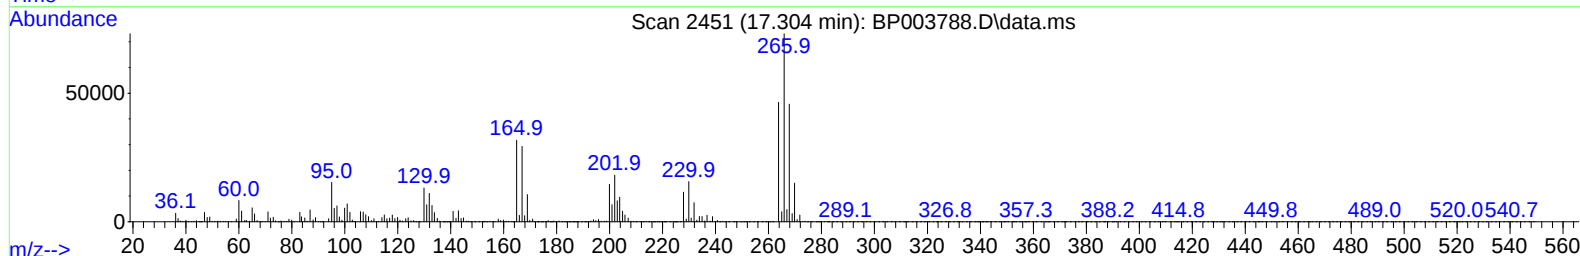


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110320\
 Data File : BP003788.D
 Acq On : 03 Nov 2020 11:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 11 08:56:35 2020
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270-BP110220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 02 16:42:53 2020
 Response via : Initial Calibration

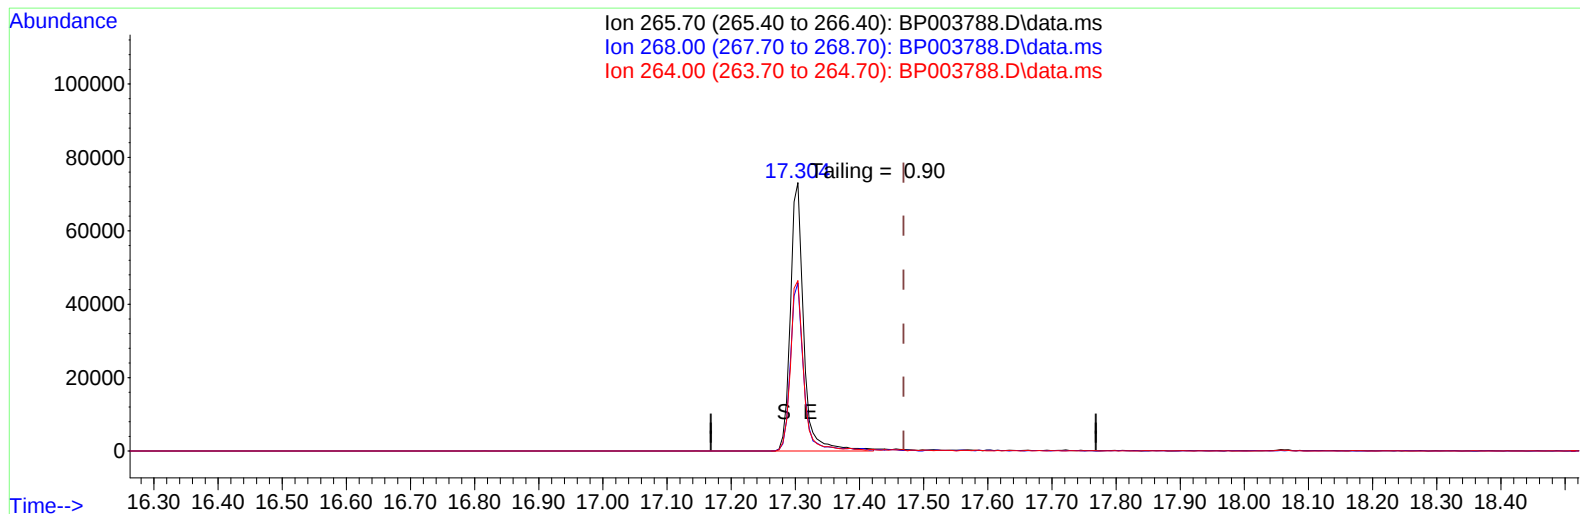

TIC: BP003788.D\data.ms

(70) Pentachlorophenol (C)




17.304min (-0.165) 504902.97 ng

response 106131

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	62.58
264.00	63.30	63.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110320\
Data File : BP003788.D
Acq On : 03 Nov 2020 11:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 11 08:56:35 2020
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270-BP110220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 02 16:42:53 2020
Response via : Initial Calibration

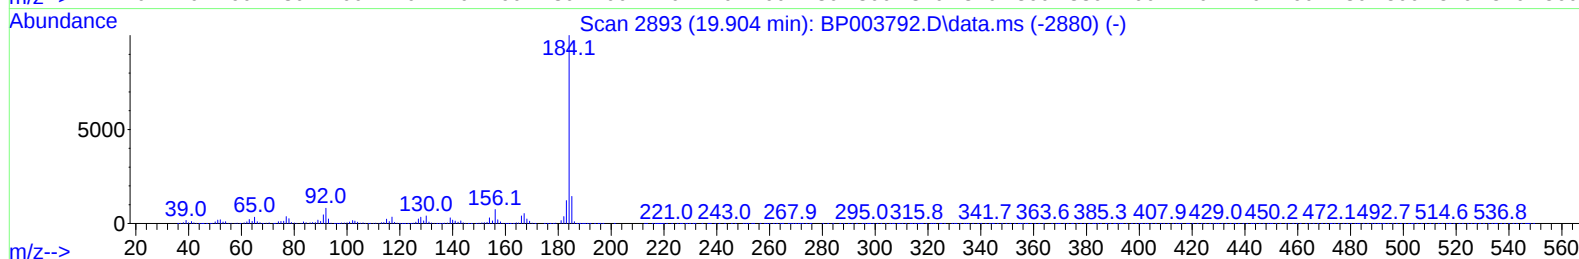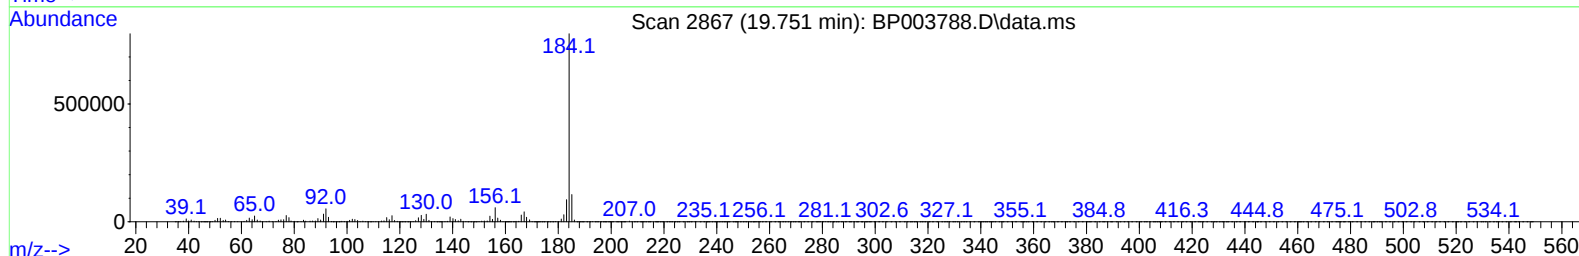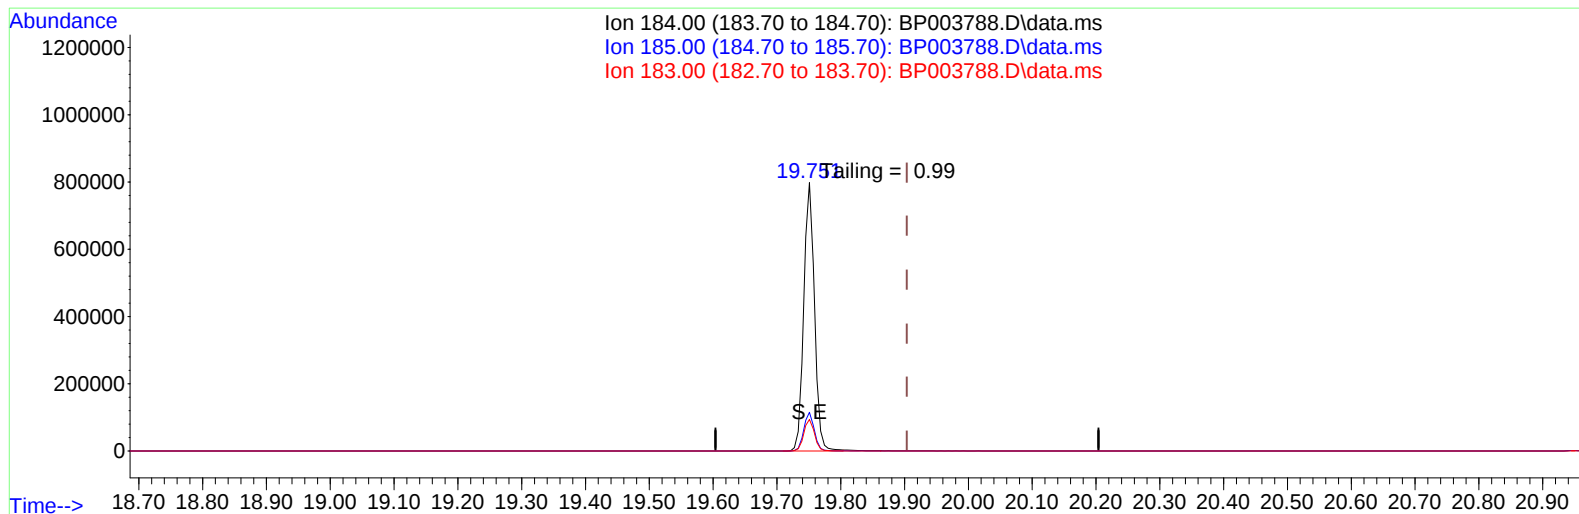

TIC: BP003788.D\data.ms

(77) Benzidine**19.751min (-0.153) 986208.10 ng****response 937241**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.45
183.00	12.00	11.76
0.00	0.00	0.00