


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110320\
Data File : BP003788.D
Acq On : 03 Nov 2020 11:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 12 15:22:47 2020

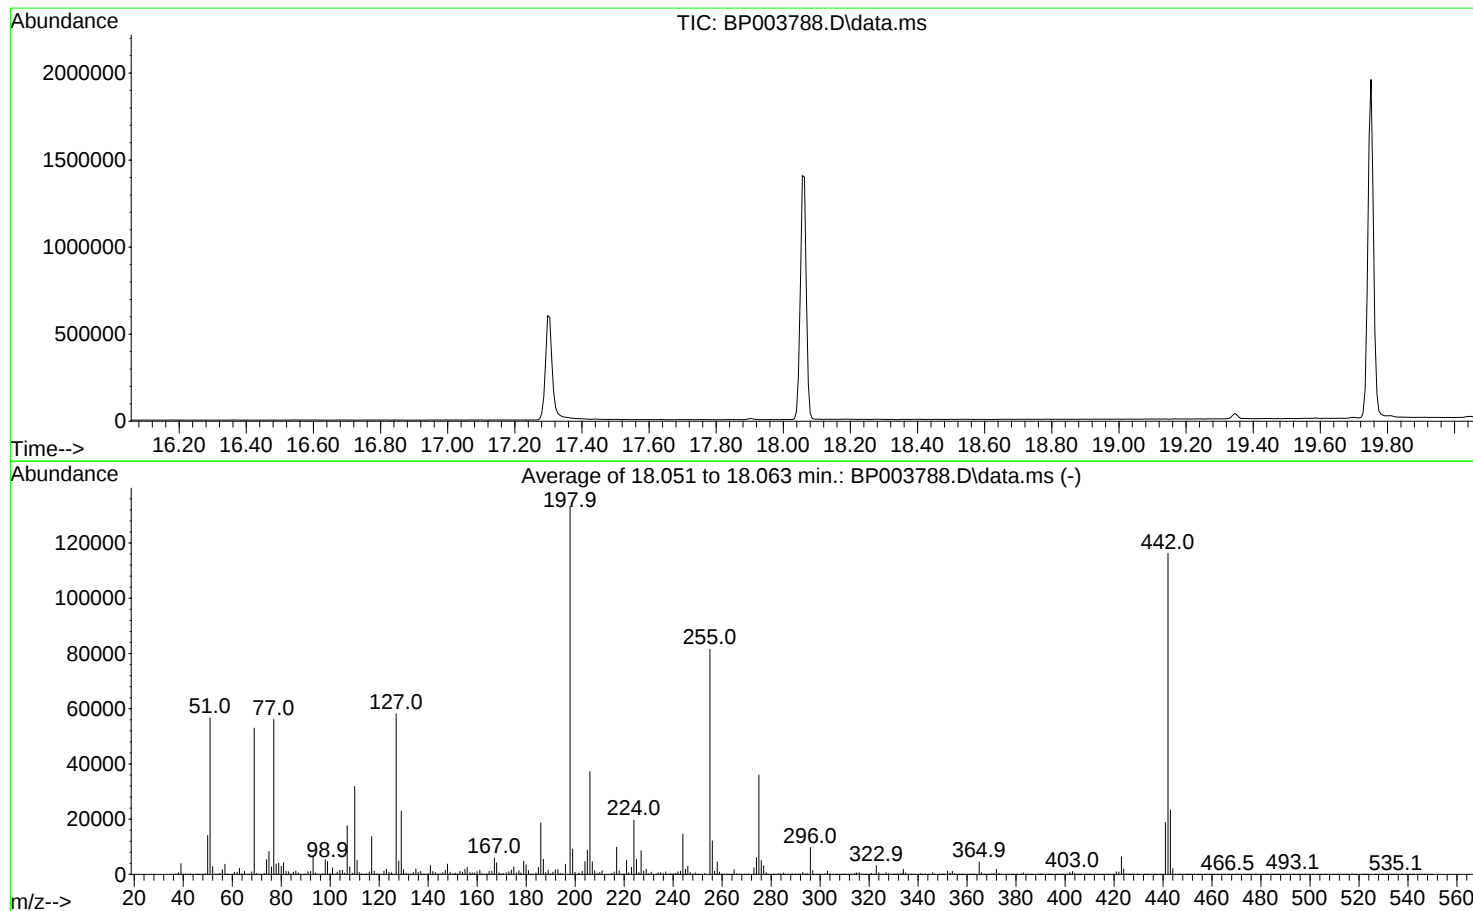

AutoFind: Scans 2578, 2579, 2580; Background Corrected with Scan 2571

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.6	56701	PASS
68	69	0.00	2	1.8	942	PASS
69	198	0.00	100	39.7	52960	PASS
70	69	0.00	2	0.6	312	PASS
127	198	10	80	43.6	58107	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	133235	PASS
199	198	5	9	6.9	9151	PASS
275	198	10	60	27.0	35984	PASS
365	198	1	100	3.3	4456	PASS
441	198	0.01	100	14.1	18834	PASS
442	198	50	100	87.2	116235	PASS
443	442	15	24	20.1	23319	PASS