
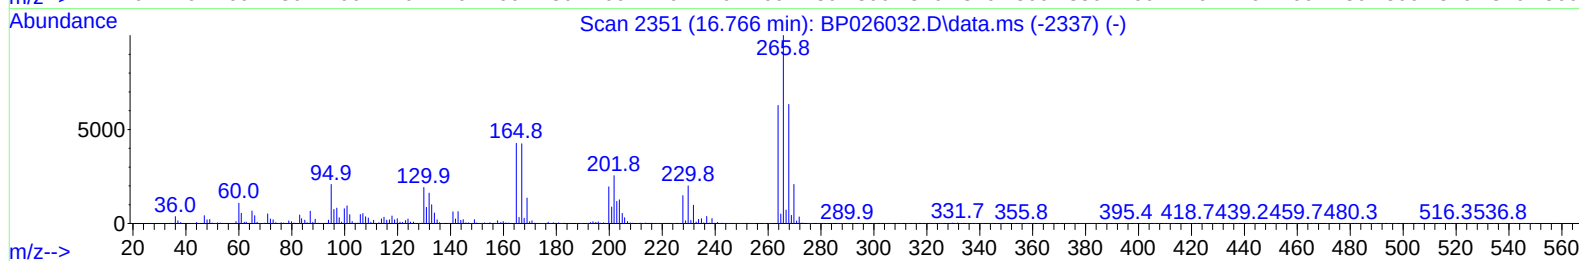
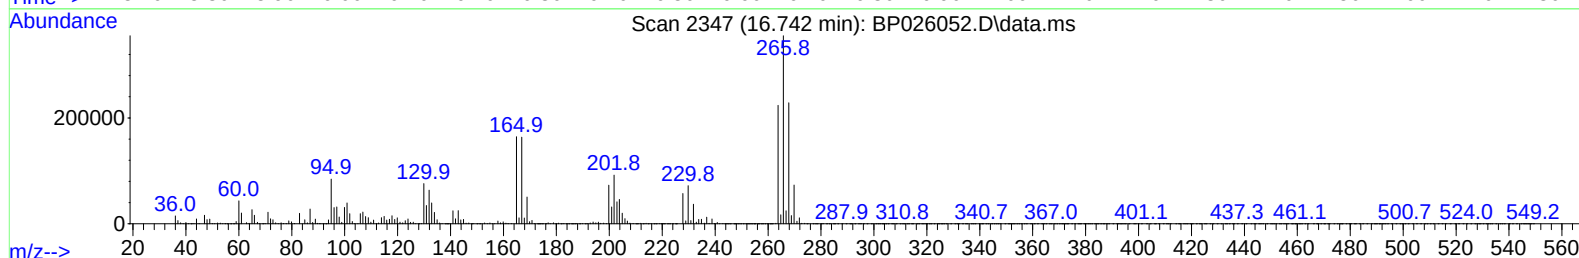


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110325\
Data File : BP026052.D
Acq On : 03 Nov 2025 10:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 11:20:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 30 11:51:34 2025
Response via : Initial Calibration

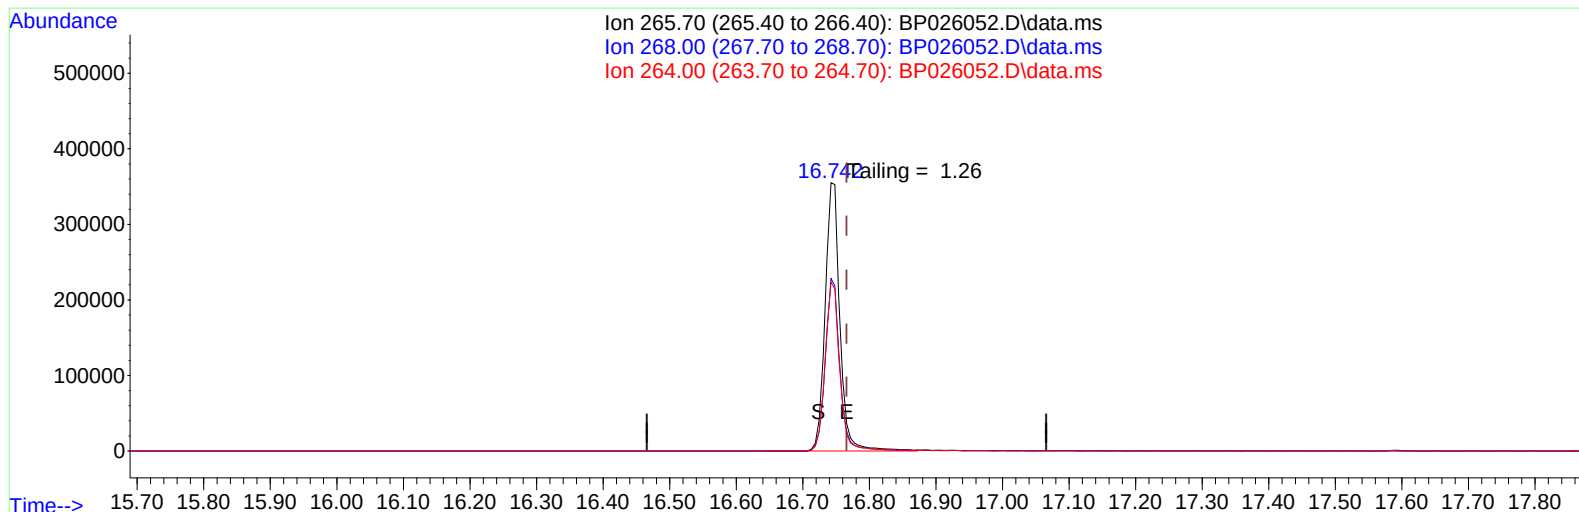

TIC: BP026052.D\data.ms

(70) Pentachlorophenol (C)




16.742min (-0.023) 2966656.68 ng

response 549178

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	64.31
264.00	62.80	62.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110325\
Data File : BP026052.D
Acq On : 03 Nov 2025 10:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 11:20:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 30 11:51:34 2025
Response via : Initial Calibration

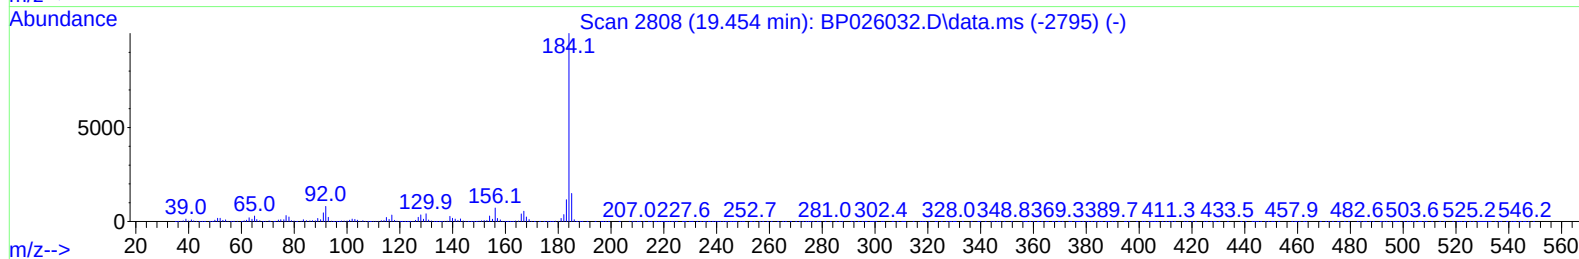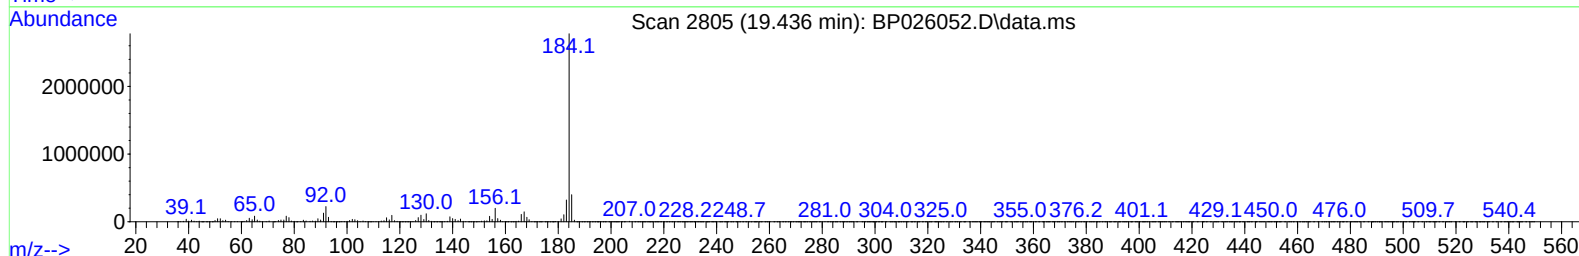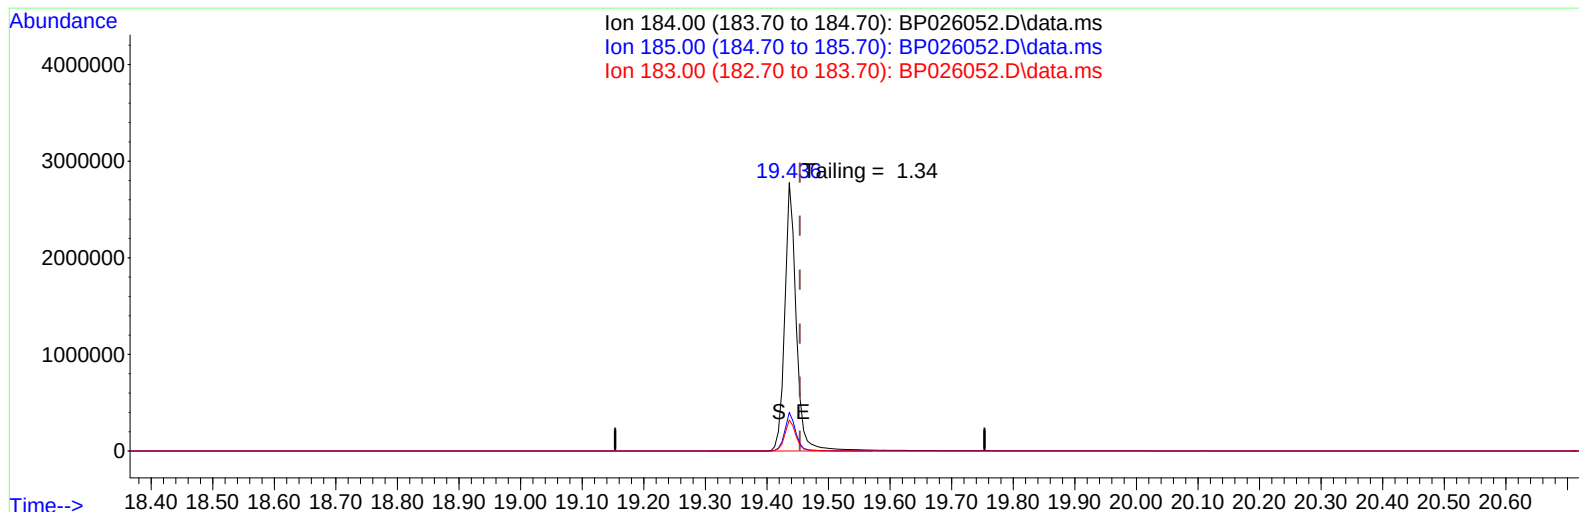

TIC: BP026052.D\data.ms

(77) Benzidine

19.436min (-0.017) 1459112.87 ng

response 3666573

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.38
183.00	11.50	11.60
0.00	0.00	0.00