

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110325\
 Data File : BP026060.D
 Acq On : 03 Nov 2025 16:13
 Operator : RC/JU
 Sample : Q3495-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SB-1025-2

Quant Time: Nov 03 16:33:50 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 30 11:51:34 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.684	152	335609	20.000	ng	0.00
21) Naphthalene-d8	10.455	136	1339601	20.000	ng	0.00
39) Acenaphthene-d10	14.325	164	820932	20.000	ng	0.00
64) Phenanthrene-d10	17.125	188	1674460	20.000	ng	0.00
76) Chrysene-d12	21.572	240	1797769	20.000	ng	0.00
86) Perylene-d12	24.895	264	2045798	20.000	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.302	112	1506944	74.092	ng	0.00
7) Phenol-d6	6.855	99	1931703	74.620	ng	0.00
23) Nitrobenzene-d5	8.819	82	1094006	50.911	ng	0.00
42) 2,4,6-Tribromophenol	15.831	330	756973	85.292	ng	0.00
45) 2-Fluorobiphenyl	12.931	172	2550471	44.642	ng	0.00
79) Terphenyl-d14	19.866	244	3935857	44.480	ng	0.00
Target Compounds						
84) Bis(2-ethylhexyl)phtha...	21.519	149	11378	2.746	ng	Qvalue # 84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110325\
Data File : BP026060.D
Acq On : 03 Nov 2025 16:13
Operator : RC/JU
Sample : Q3495-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SB-1025-2

Quant Time: Nov 03 16:33:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 30 11:51:34 2025
Response via : Initial Calibration




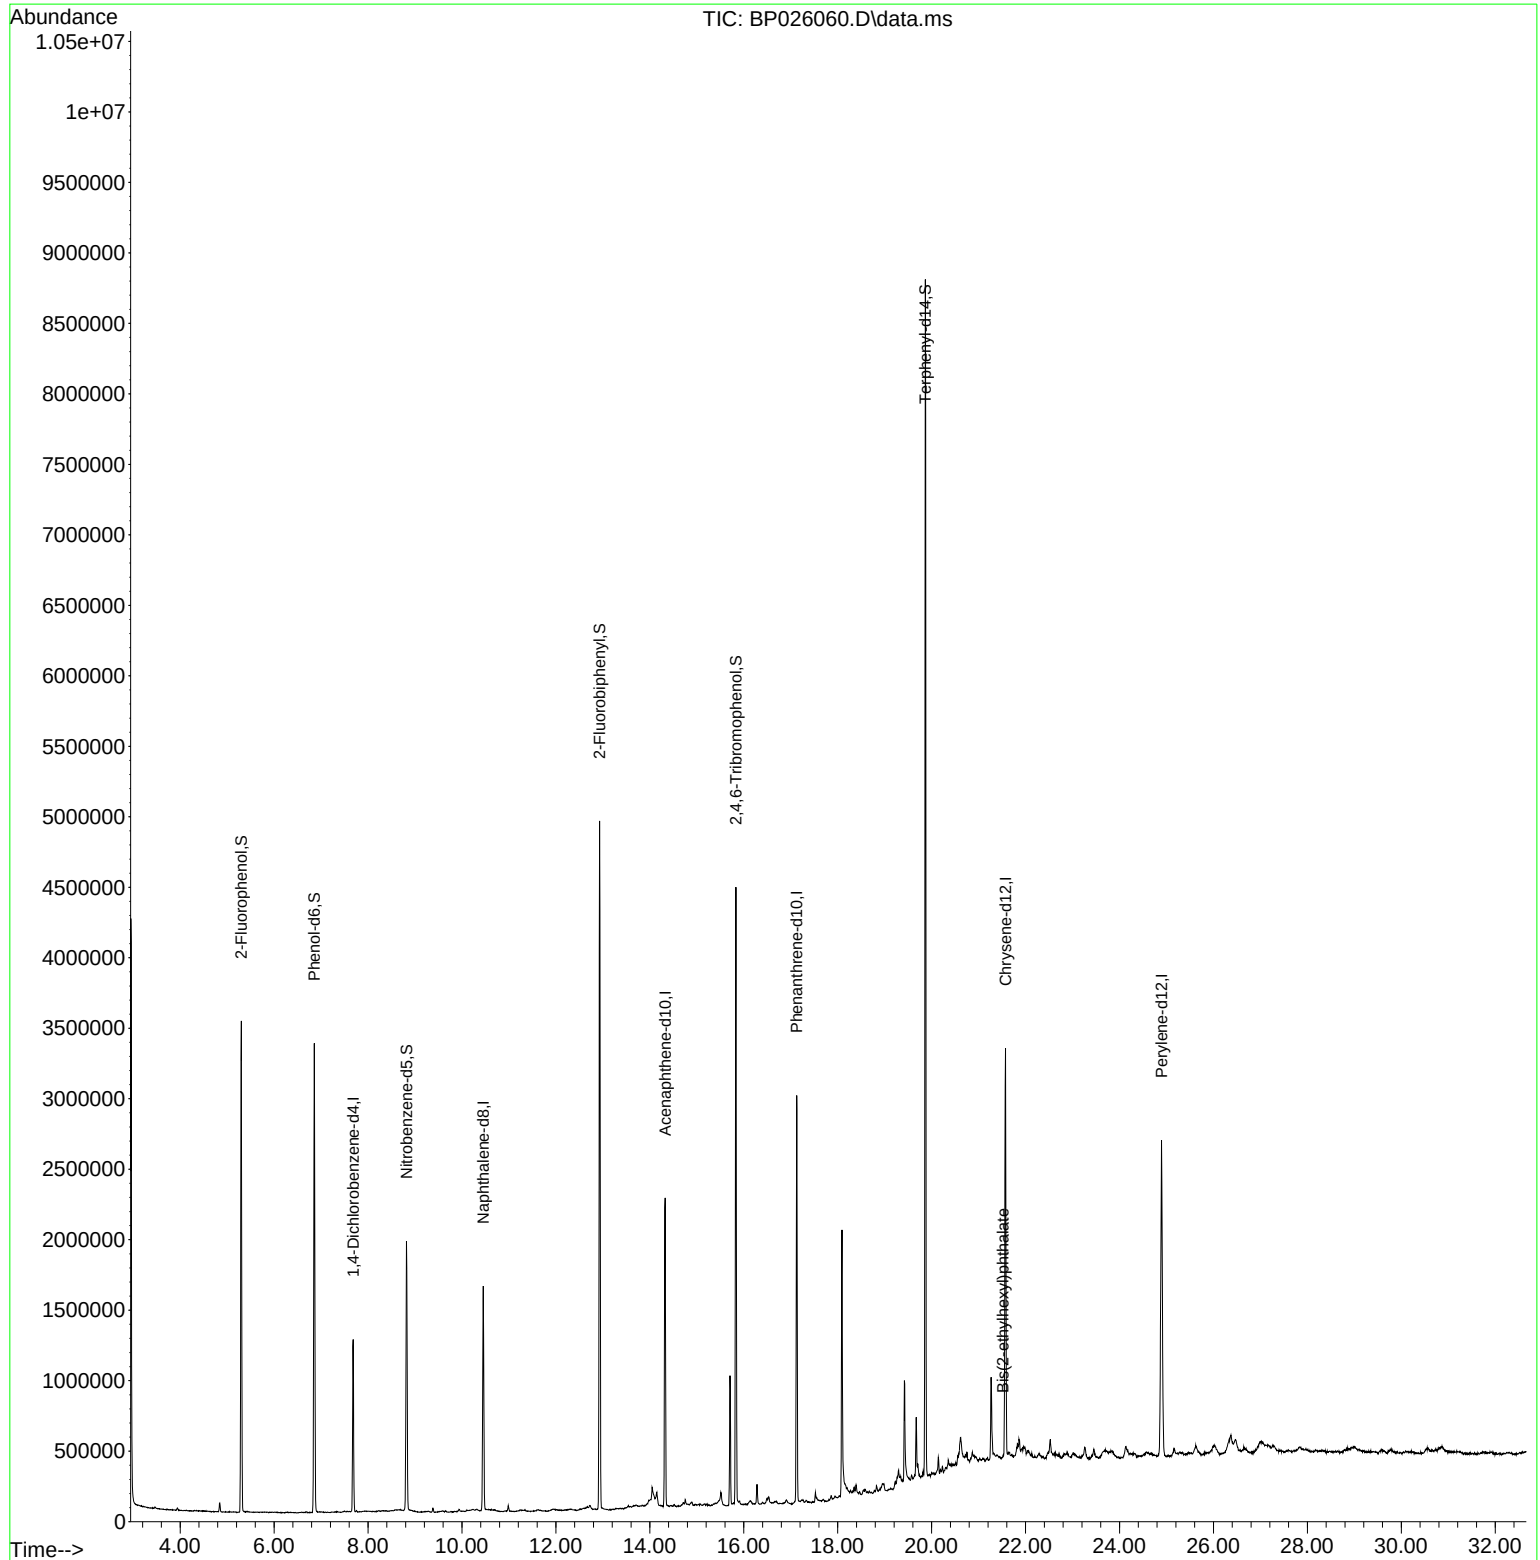


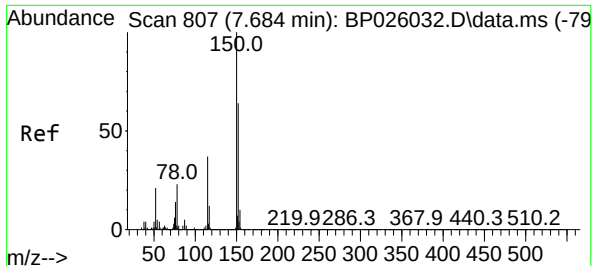

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 7.684 min Scan# 807
 Delta R.T. -0.006 min
 Lab File: BP026060.D
 Acq: 03 Nov 2025 16:13




Instrument :
 BNA_P
 ClientSampleId :
 SB-1025-2


Tgt Ion:152 Resp: 335609
 Ion Ratio Lower Upper
 152 100
 150 153.6 125.7 188.5
 115 58.3 46.4 69.6

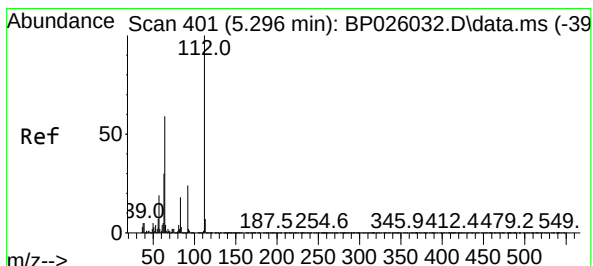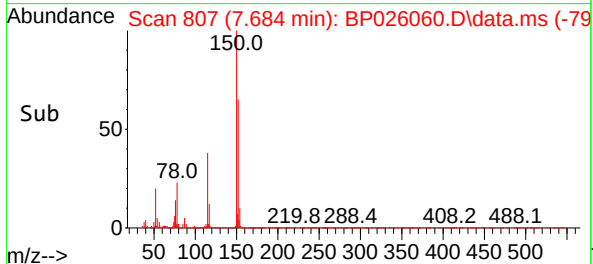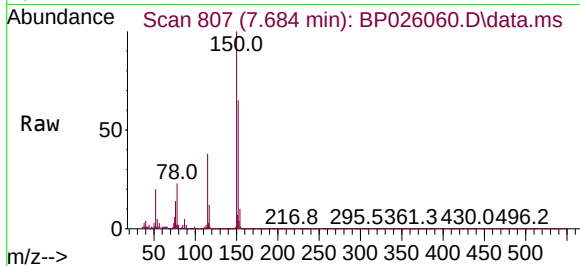

#5
 2-Fluorophenol
 Concen: 74.092 ng
 RT: 5.302 min Scan# 402
 Delta R.T. 0.006 min
 Lab File: BP026060.D
 Acq: 03 Nov 2025 16:13

Tgt Ion:112 Resp: 1506944
 Ion Ratio Lower Upper
 112 100
 64 57.2 47.4 71.2
 63 29.3 24.2 36.4


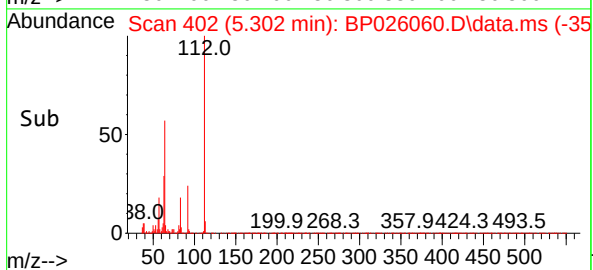

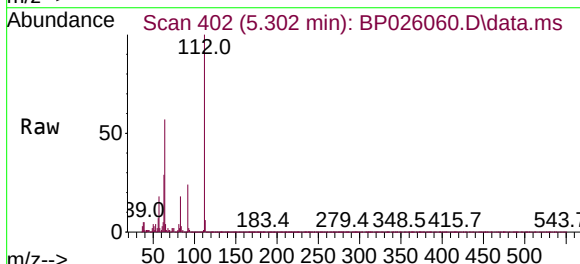




#7
Phenol-d6
Concen: 74.620 ng
RT: 6.855 min Scan# 60
Delta R.T. 0.000 min
Lab File: BP026060.D
Acq: 03 Nov 2025 16:13




Instrument :
BNA_P
ClientSampleId :
SB-1025-2


Tgt Ion: 99 Resp: 1931703
Ion Ratio Lower Upper
99 100
42 17.0 13.7 20.5
71 30.7 24.4 36.6

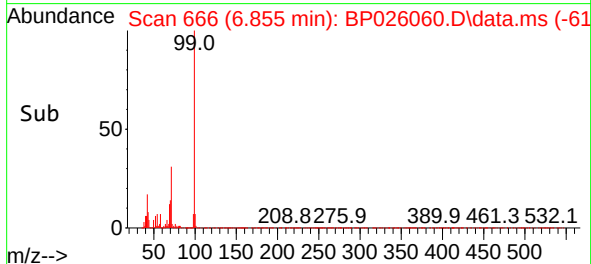

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.455 min Scan# 1278
Delta R.T. 0.001 min
Lab File: BP026060.D
Acq: 03 Nov 2025 16:13

Tgt Ion:136 Resp: 1339601
Ion Ratio Lower Upper
136 100
137 10.5 8.8 13.2
54 8.4 6.6 10.0
68 5.7 4.7 7.1


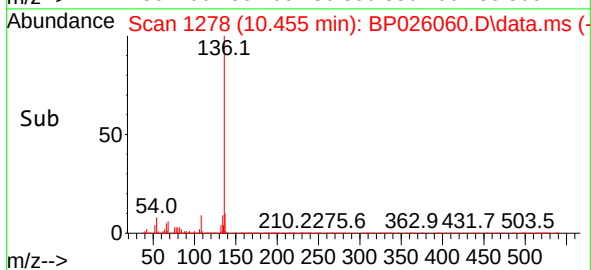

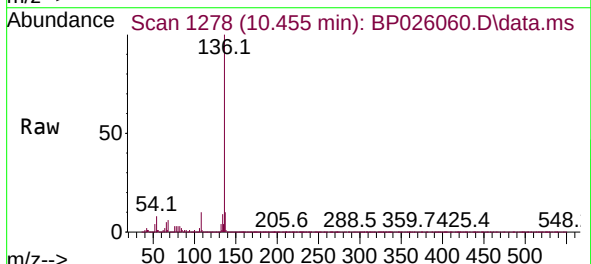




#23
Nitrobenzene-d5
Concen: 50.911 ng
RT: 8.819 min Scan# 10
Delta R.T. -0.006 min
Lab File: BP026060.D
Acq: 03 Nov 2025 16:13




Instrument :
BNA_P
ClientSampleId :
SB-1025-2


Tgt Ion: 82 Resp: 1094006
Ion Ratio Lower Upper
82 100
128 46.7 37.4 56.0
54 51.6 42.7 64.1

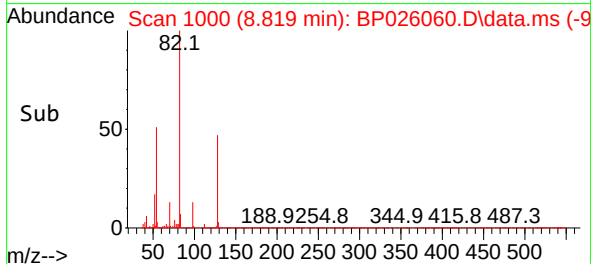

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.325 min Scan# 1936
Delta R.T. 0.006 min
Lab File: BP026060.D
Acq: 03 Nov 2025 16:13

Tgt Ion: 164 Resp: 820932
Ion Ratio Lower Upper
164 100
162 99.2 81.5 122.3
160 44.2 36.2 54.4


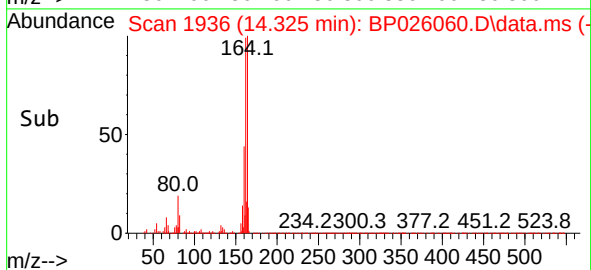

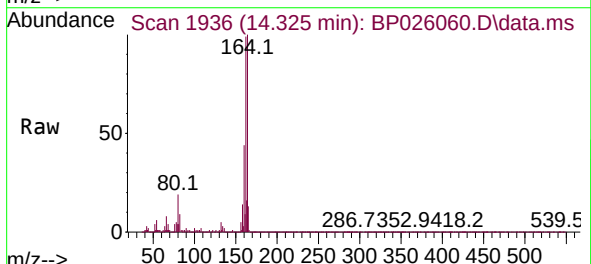




#42
2,4,6-Tribromophenol
Concen: 85.292 ng
RT: 15.831 min Scan# 2192
Delta R.T. 0.000 min
Lab File: BP026060.D
Acq: 03 Nov 2025 16:13




Instrument :
BNA_P
ClientSampleId :
SB-1025-2


Tgt Ion: 330 Resp: 756973
Ion Ratio Lower Upper
330 100
332 96.2 77.3 115.9
141 34.4 28.6 42.8

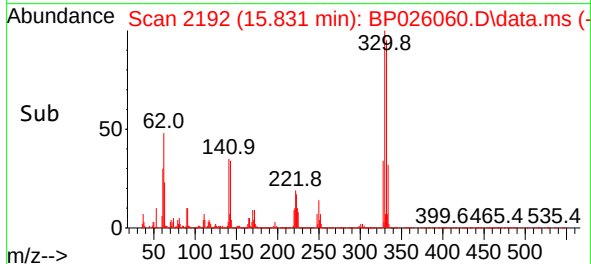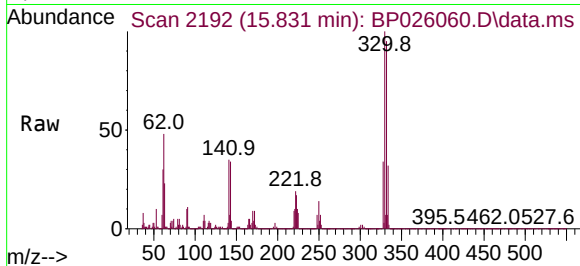

#45
2-Fluorobiphenyl
Concen: 44.642 ng
RT: 12.931 min Scan# 1699
Delta R.T. -0.000 min
Lab File: BP026060.D
Acq: 03 Nov 2025 16:13

Tgt Ion: 172 Resp: 2550471
Ion Ratio Lower Upper
172 100
171 35.0 27.9 41.9
170 23.4 19.0 28.4


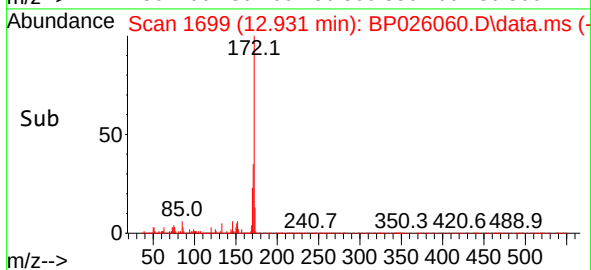

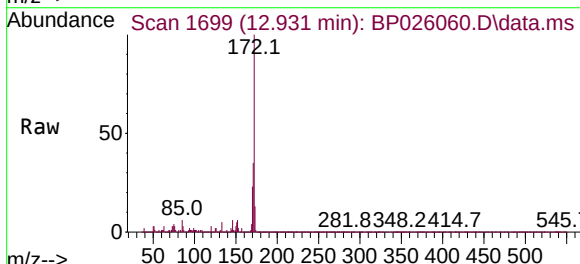




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.125 min Scan# 2412
Delta R.T. 0.000 min
Lab File: BP026060.D
Acq: 03 Nov 2025 16:13




Instrument :
BNA_P
ClientSampleId :
SB-1025-2


Tgt Ion:188 Resp: 1674460
Ion Ratio Lower Upper
188 100
94 9.5 7.1 10.7
80 10.5 7.9 11.9

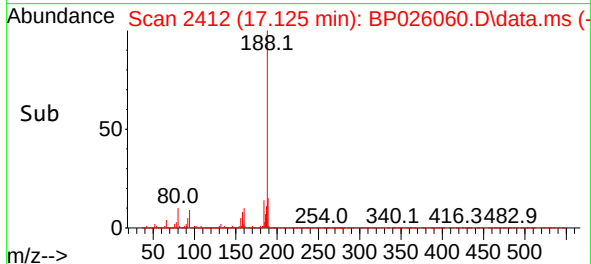

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.572 min Scan# 3168
Delta R.T. 0.006 min
Lab File: BP026060.D
Acq: 03 Nov 2025 16:13

Tgt Ion:240 Resp: 1797769
Ion Ratio Lower Upper
240 100
120 11.4 8.9 13.3
236 25.2 20.6 31.0


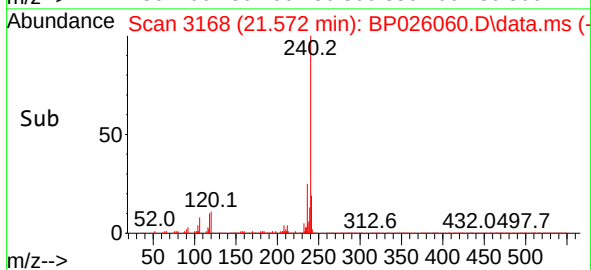

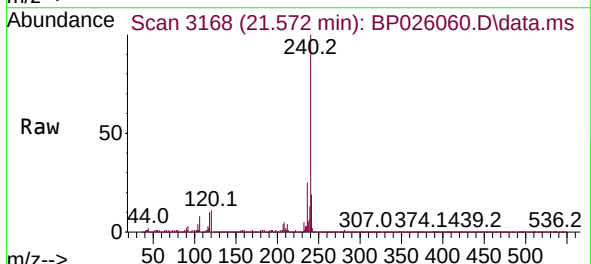




#79
 Terphenyl-d14
 Concen: 44.480 ng
 RT: 19.866 min Scan# 2878
 Delta R.T. 0.000 min
 Lab File: BP026060.D
 Acq: 03 Nov 2025 16:13




Instrument :
 BNA_P
 ClientSampleId :
 SB-1025-2


Tgt Ion:244 Resp: 3935857
 Ion Ratio Lower Upper
 244 100
 212 7.2 6.0 9.0
 122 11.3 9.0 13.6

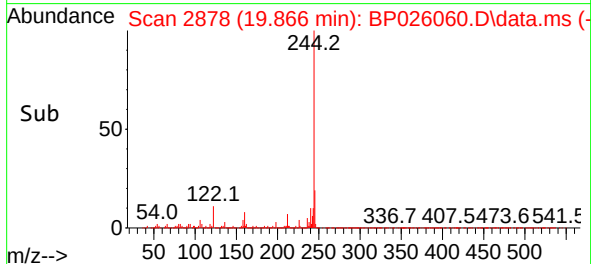

#84
 Bis(2-ethylhexyl)phthalate
 Concen: 2.746 ng
 RT: 21.519 min Scan# 3159
 Delta R.T. 0.001 min
 Lab File: BP026060.D
 Acq: 03 Nov 2025 16:13

Tgt Ion:149 Resp: 11378
 Ion Ratio Lower Upper
 149 100
 167 35.7 21.5 32.3#
 279 6.4 3.0 4.6#

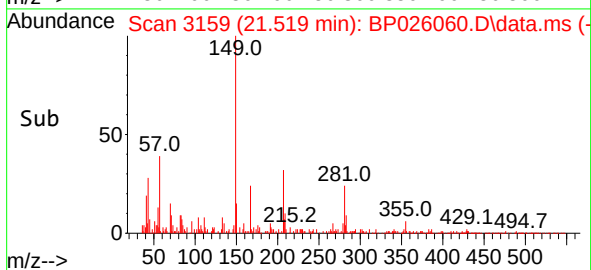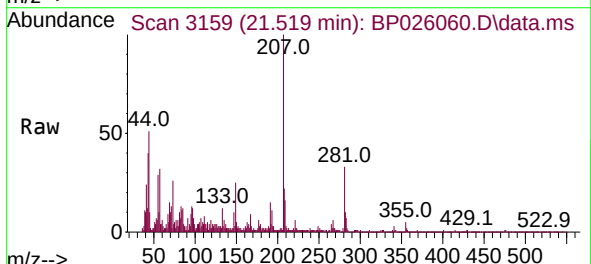



#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.895 min Scan# 31
 Delta R.T. 0.012 min
 Lab File: BP026060.D
 Acq: 03 Nov 2025 16:13

Instrument :
 BNA_P
 ClientSampleId :
 SB-1025-2

Tgt Ion:264 Resp: 2045798
 Ion Ratio Lower Upper
 264 100
 260 23.3 19.1 28.7
 265 21.8 17.2 25.8

