

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110325\
 Data File : BP026054.D
 Acq On : 03 Nov 2025 11:47
 Operator : RC/JU
 Sample : PB170342BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB170342BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP026054.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.302	395	402	416	rBV	5873931	8805803	41.28%	9.911%
2	6.855	657	666	691	rBV	5422804	8818785	41.35%	9.926%
3	7.678	797	806	815	rBV	1280569	1938090	9.09%	2.181%
4	8.819	991	1000	1020	rBV	3206875	5501607	25.79%	6.192%
5	10.443	1266	1276	1290	rBV	1473010	2616131	12.27%	2.944%
6	12.925	1690	1698	1709	rBV	9410615	13075333	61.30%	14.716%
7	14.313	1926	1934	1942	rBV	2345476	3351110	15.71%	3.772%
8	15.825	2182	2191	2214	rBV	6278239	8869062	41.58%	9.982%
9	17.119	2404	2411	2422	rBV2	2834333	4163681	19.52%	4.686%
10	19.860	2871	2877	2892	rBV	17194756	21329650	100.00%	24.006%
11	21.560	3160	3166	3178	rBV	3170711	5010735	23.49%	5.640%
12	24.877	3720	3730	3743	rBV	2162523	5369770	25.18%	6.044%




Sum of corrected areas: 88849757

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110325\
Data File : BP026054.D
Acq On : 03 Nov 2025 11:47
Operator : RC/JU
Sample : PB170342BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB170342BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

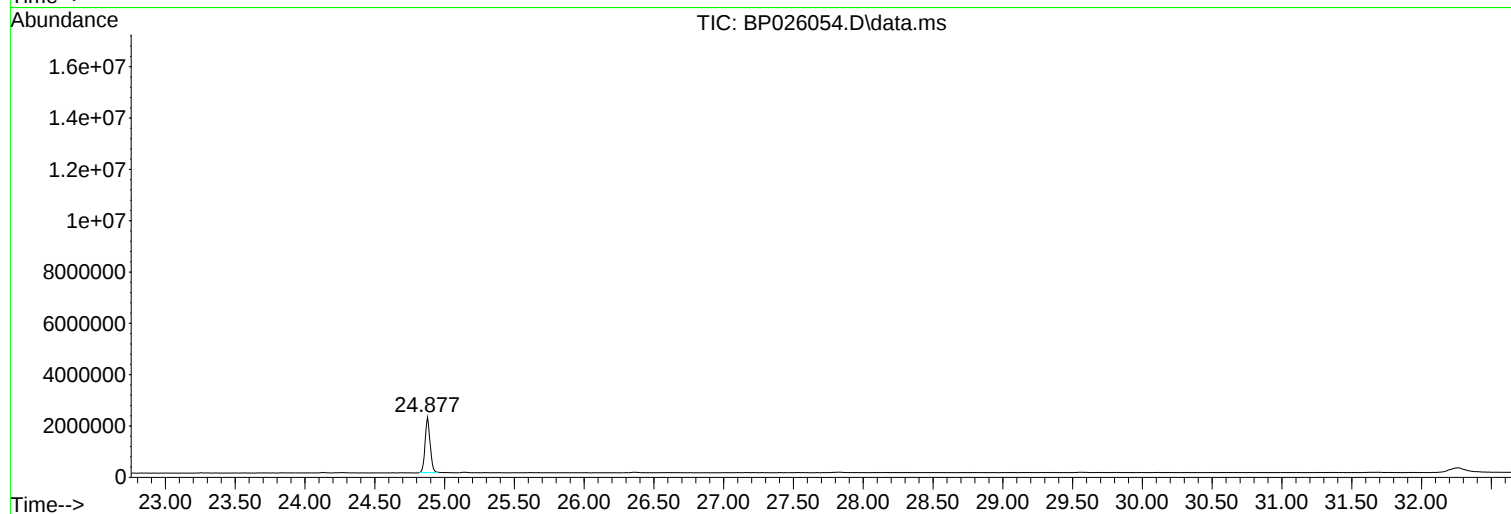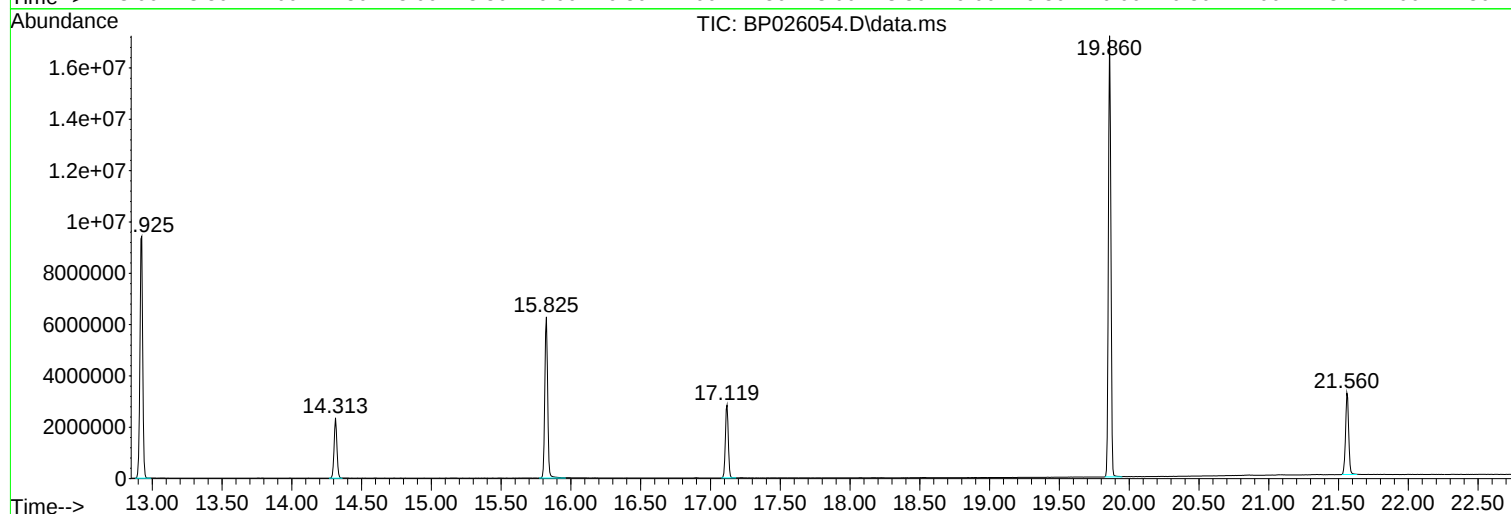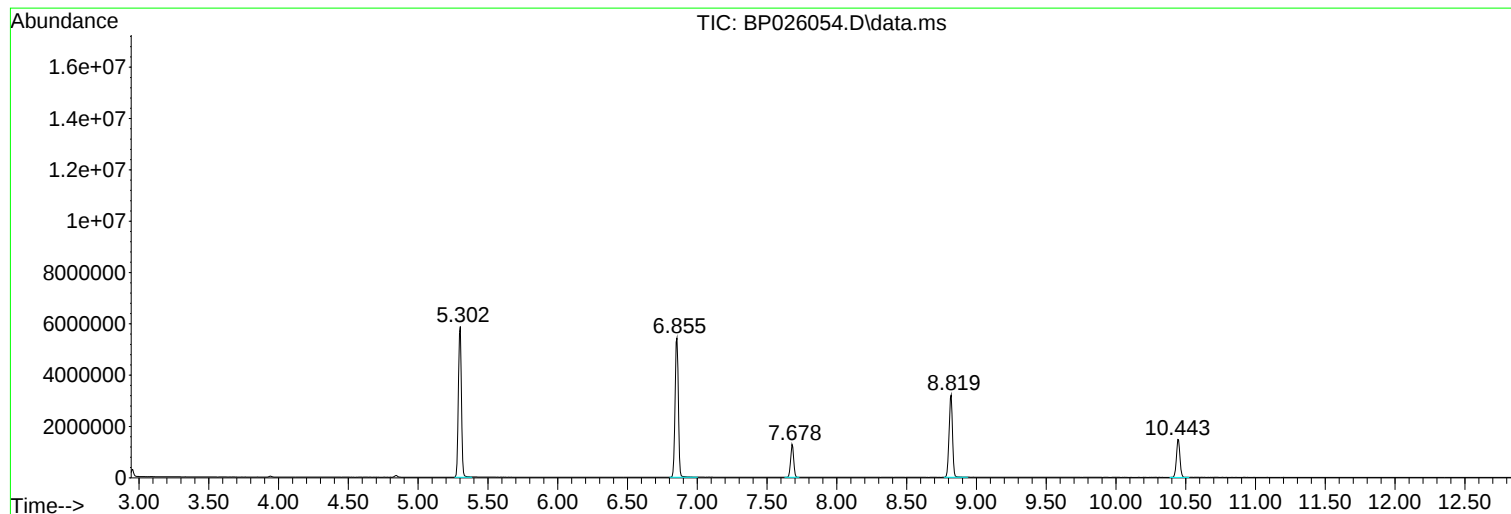

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110325\
Data File : BP026054.D
Acq On : 03 Nov 2025 11:47
Operator : RC/JU
Sample : PB170342BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB170342BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110325\
Data File : BP026054.D
Acq On : 03 Nov 2025 11:47
Operator : RC/JU
Sample : PB170342BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB170342BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------