


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110619\
 Data File : BP000984.D
 Acq On : 06 Nov 2019 12:36
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 06 17:07:13 2019

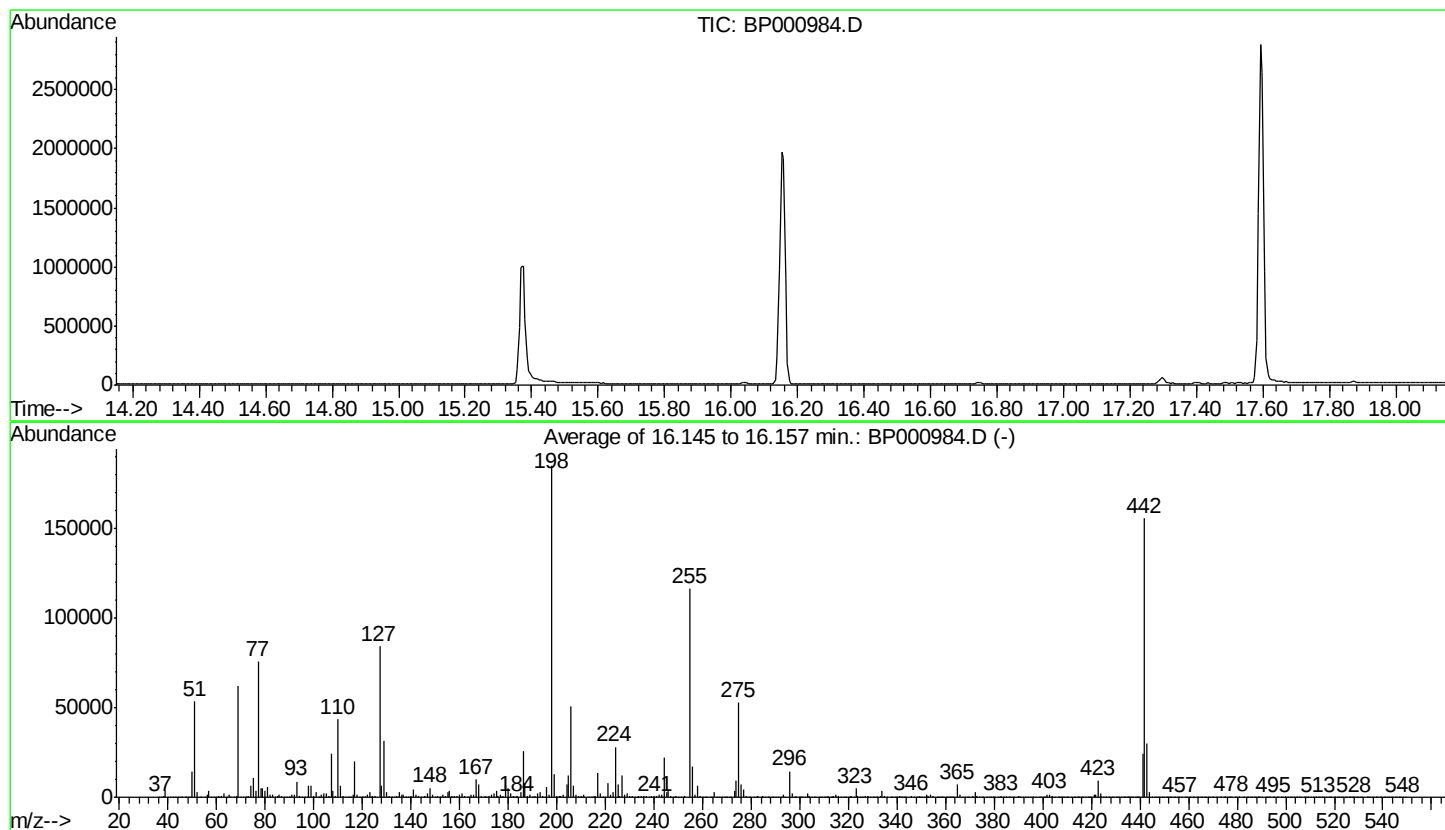

AutoFind: Scans 2390, 2391, 2392; Background Corrected with Scan 2382

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.9	53427	PASS
68	69	0.00	2	1.2	760	PASS
69	198	0.00	100	33.4	61741	PASS
70	69	0.00	2	0.5	304	PASS
127	198	10	80	45.5	84106	PASS
197	198	0.00	2	0.7	1294	PASS
198	198	100	100	100.0	184741	PASS
199	198	5	9	7.0	12874	PASS
275	198	10	60	28.4	52522	PASS
365	198	1	100	3.7	6924	PASS
441	198	0.01	100	13.3	24574	PASS
442	198	50	100	84.0	155194	PASS
443	442	15	24	19.3	30018	PASS