

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110623\
 Data File : BP017917.D
 Acq On : 06 Nov 2023 17:03
 Operator : MA/JU
 Sample : SST04043
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SST040606

Quant Time: Nov 07 03:08:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 07 03:03:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.863	152	74453	20.000	ng/u1	0.00
20) Naphthalene-d8	10.681	136	316859	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.522	164	202126	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.298	188	440855	20.000	ng/u1	0.00
79) Chrysene-d12	21.416	240	404944	20.000	ng/u1	0.00
88) Perylene-d12	23.898	264	423021	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.240	96	32419	16.423	ng/uL	0.00
4) Pyridine-d5	3.675	84	230054	42.612	ng/u1	0.00
7) Phenol-d5	7.028	99	294687	42.207	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.210	67	177515	42.149	ng/u1	0.00
11) 2-Chlorophenol-d4	7.387	132	235828	43.019	ng/u1	0.00
15) 4-Methylphenol-d8	8.587	113	245579	42.556	ng/u1	0.00
21) Nitrobenzene-d5	9.063	128	119135	43.818	ng/u1	0.00
24) 2-Nitrophenol-d4	9.775	143	139023	44.136	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.299	165	241710	42.085	ng/u1	0.00
31) 4-Chloroaniline-d4	10.851	131	332002	42.850	ng/u1	0.00
46) Dimethylphthalate-d6	13.945	166	763439	40.828	ng/u1	0.00
49) Acenaphthylene-d8	14.228	160	854196	41.789	ng/u1	0.00
54) 4-Nitrophenol-d4	14.775	143	122180	44.836	ng/u1	0.00
60) Fluorene-d10	15.522	176	634830	40.739	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.675	200	139898	43.394	ng/u1	0.00
73) Anthracene-d10	17.398	188	995833	41.514	ng/u1	0.00
81) Pyrene-d10	19.645	212	1141408	42.307	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.733	264	1029068	41.387	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.281	88	35605	16.281	ng/uL	96
5) Pyridine	3.693	79	236330	42.103	ng/u1	96
6) Benzaldehyde	7.028	77	175461	45.183	ng/u1	97
8) Phenol	7.058	94	291273	42.409	ng/u1	96
10) Bis(2-Chloroethyl)ether	7.305	93	231019	41.998	ng/u1	97
12) 2-Chlorophenol	7.416	128	237794	43.530	ng/u1	98
13) 2-Methylphenol	8.310	108	224818	42.577	ng/u1	98
14) 2,2'-oxybis(1-Chloropr...	8.375	45	140928	22.255	ng/u1	98
16) Acetophenone	8.716	105	389423	42.050	ng/u1	100
17) N-Nitroso-di-n-propyla...	8.687	70	211552	42.031	ng/u1	99
18) 4-Methylphenol	8.652	108	240037	42.258	ng/u1	92
19) Hexachloroethane	8.916	117	113625	40.850	ng/u1	94
22) Nitrobenzene	9.110	77	326565	44.783	ng/u1	98
23) Isophorone	9.622	82	586405	43.982	ng/u1	99
25) 2-Nitrophenol	9.810	139	141494	43.563	ng/u1	98
26) 2,4-Dimethylphenol	9.851	107	296077	43.634	ng/u1	98
27) Bis(2-Chloroethoxy)met...	10.104	93	317754	43.143	ng/u1	98
29) 2,4-Dichlorophenol	10.328	162	233819	41.586	ng/u1	94
30) Naphthalene	10.728	128	784028	40.917	ng/u1	99
32) 4-Chloroaniline	10.875	127	316802	42.575	ng/u1	97
33) Hexachlorobutadiene	10.946	225	169763	37.254	ng/u1	98
34) Caprolactam	11.716	113	39972	24.025	ng/u1	98
35) 4-Chloro-3-methylphenol	11.987	107	274549	43.607	ng/u1	95
36) 2-Methylnaphthalene	12.340	142	540465	40.932	ng/u1	98

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110623\
 Data File : BP017917.D
 Acq On : 06 Nov 2023 17:03
 Operator : MA/JU
 Sample : SST04043
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SST040606

Quant Time: Nov 07 03:08:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 07 03:03:13 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.563	142	551297	40.587	ng/ul	100
39) 1,2,4,5-Tetrachloroben...	12.693	216	290468	39.832	ng/ul	99
40) Hexachlorocyclopentadiene	12.628	237	152783	40.976	ng/ul	99
41) 2,4,6-Trichlorophenol	12.957	196	193926	41.731	ng/ul	99
42) 2,4,5-Trichlorophenol	13.028	196	202502	41.665	ng/ul	96
43) 1,1'-Biphenyl	13.357	154	724379	41.902	ng/ul	99
44) 2-Chloronaphthalene	13.404	162	571662	41.310	ng/ul	97
45) 2-Nitroaniline	13.651	65	194962	47.298	ng/ul	93
47) Dimethylphthalate	13.992	163	755296	40.965	ng/ul	100
48) 2,6-Dinitrotoluene	14.145	165	155915	42.741	ng/ul	92
50) Acenaphthylene	14.257	152	954482	41.653	ng/ul	100
51) 3-Nitroaniline	14.487	138	147167	45.035	ng/ul	93
52) Acenaphthene	14.592	153	627728	41.258	ng/ul	99
53) 2,4-Dinitrophenol	14.698	184	87107	42.658	ng/ul#	84
55) 4-Nitrophenol	14.787	109	161764	49.396	ng/ul	93
56) Dibenzofuran	14.928	168	862290	40.796	ng/ul	99
57) 2,4-Dinitrotoluene	14.939	165	233734	43.207	ng/ul	93
58) 2,3,4,6-Tetrachlorophenol	15.151	232	177772	39.352	ng/ul	94
59) Diethylphthalate	15.351	149	797004	41.425	ng/ul	99
61) Fluorene	15.581	166	728182	40.819	ng/ul	98
62) 4-Chlorophenyl-phenyle...	15.575	204	364255	39.539	ng/ul	98
63) 4-Nitroaniline	15.663	138	138493	45.337	ng/ul	96
66) 4,6-Dinitro-2-methylph...	15.692	198	144913	43.026	ng/ul#	99
67) N-Nitrosodiphenylamine	15.804	169	602913	42.545	ng/ul	98
68) 4-Bromophenyl-phenylether	16.475	248	213044	39.096	ng/ul	93
69) Hexachlorobenzene	16.557	284	235131	37.789	ng/ul#	90
70) Atrazine	16.763	200	223847	43.196	ng/ul	99
71) Pentachlorophenol	16.928	266	145387	40.169	ng/ul	95
72) Phenanthrene	17.345	178	1128464	41.495	ng/ul	99
74) Anthracene	17.433	178	1159540	41.966	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.310	216	292951	40.711	ng/uL	99
76) Pentachlorobenzene	14.822	250	281345	39.255	ng/uL	99
77) Carbazole	17.728	167	1022137	43.503	ng/ul	99
78) Di-n-butylphthalate	18.233	149	1375725	44.713	ng/ul	100
80) Fluoranthene	19.316	202	1346509	42.756	ng/ul	98
82) Pyrene	19.674	202	1398437	42.668	ng/ul	100
83) Butylbenzylphthalate	20.539	149	641106	44.511	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.345	252	437163	43.186	ng/ul	99
85) Benzo(a)anthracene	21.398	228	1357601	41.455	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.274	149	929191	44.949	ng/ul	99
87) Chrysene	21.457	228	1253645	41.352	ng/ul	99
89) Di-n-octyl phthalate	22.227	149	1553842	43.492	ng/ul	100
90) Benzo(b)fluoranthene	23.127	252	1271962	41.339	ng/ul	100
91) Benzo(k)fluoranthene	23.180	252	1272675	41.488	ng/ul	99
93) Benzo(a)pyrene	23.786	252	1189543	41.767	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.533	276	1392063	40.785	ng/ul	99
95) Dibenzo(a,h)anthracene	26.556	278	1163502	41.049	ng/ul	99
96) Benzo(g,h,i)perylene	27.356	276	1110602	40.843	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110623\
 Data File : BP017917.D
 Acq On : 06 Nov 2023 17:03
 Operator : MA/JU
 Sample : SST04043
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SST040606

Quant Time: Nov 07 03:08:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 07 03:03:13 2023
 Response via : Initial Calibration




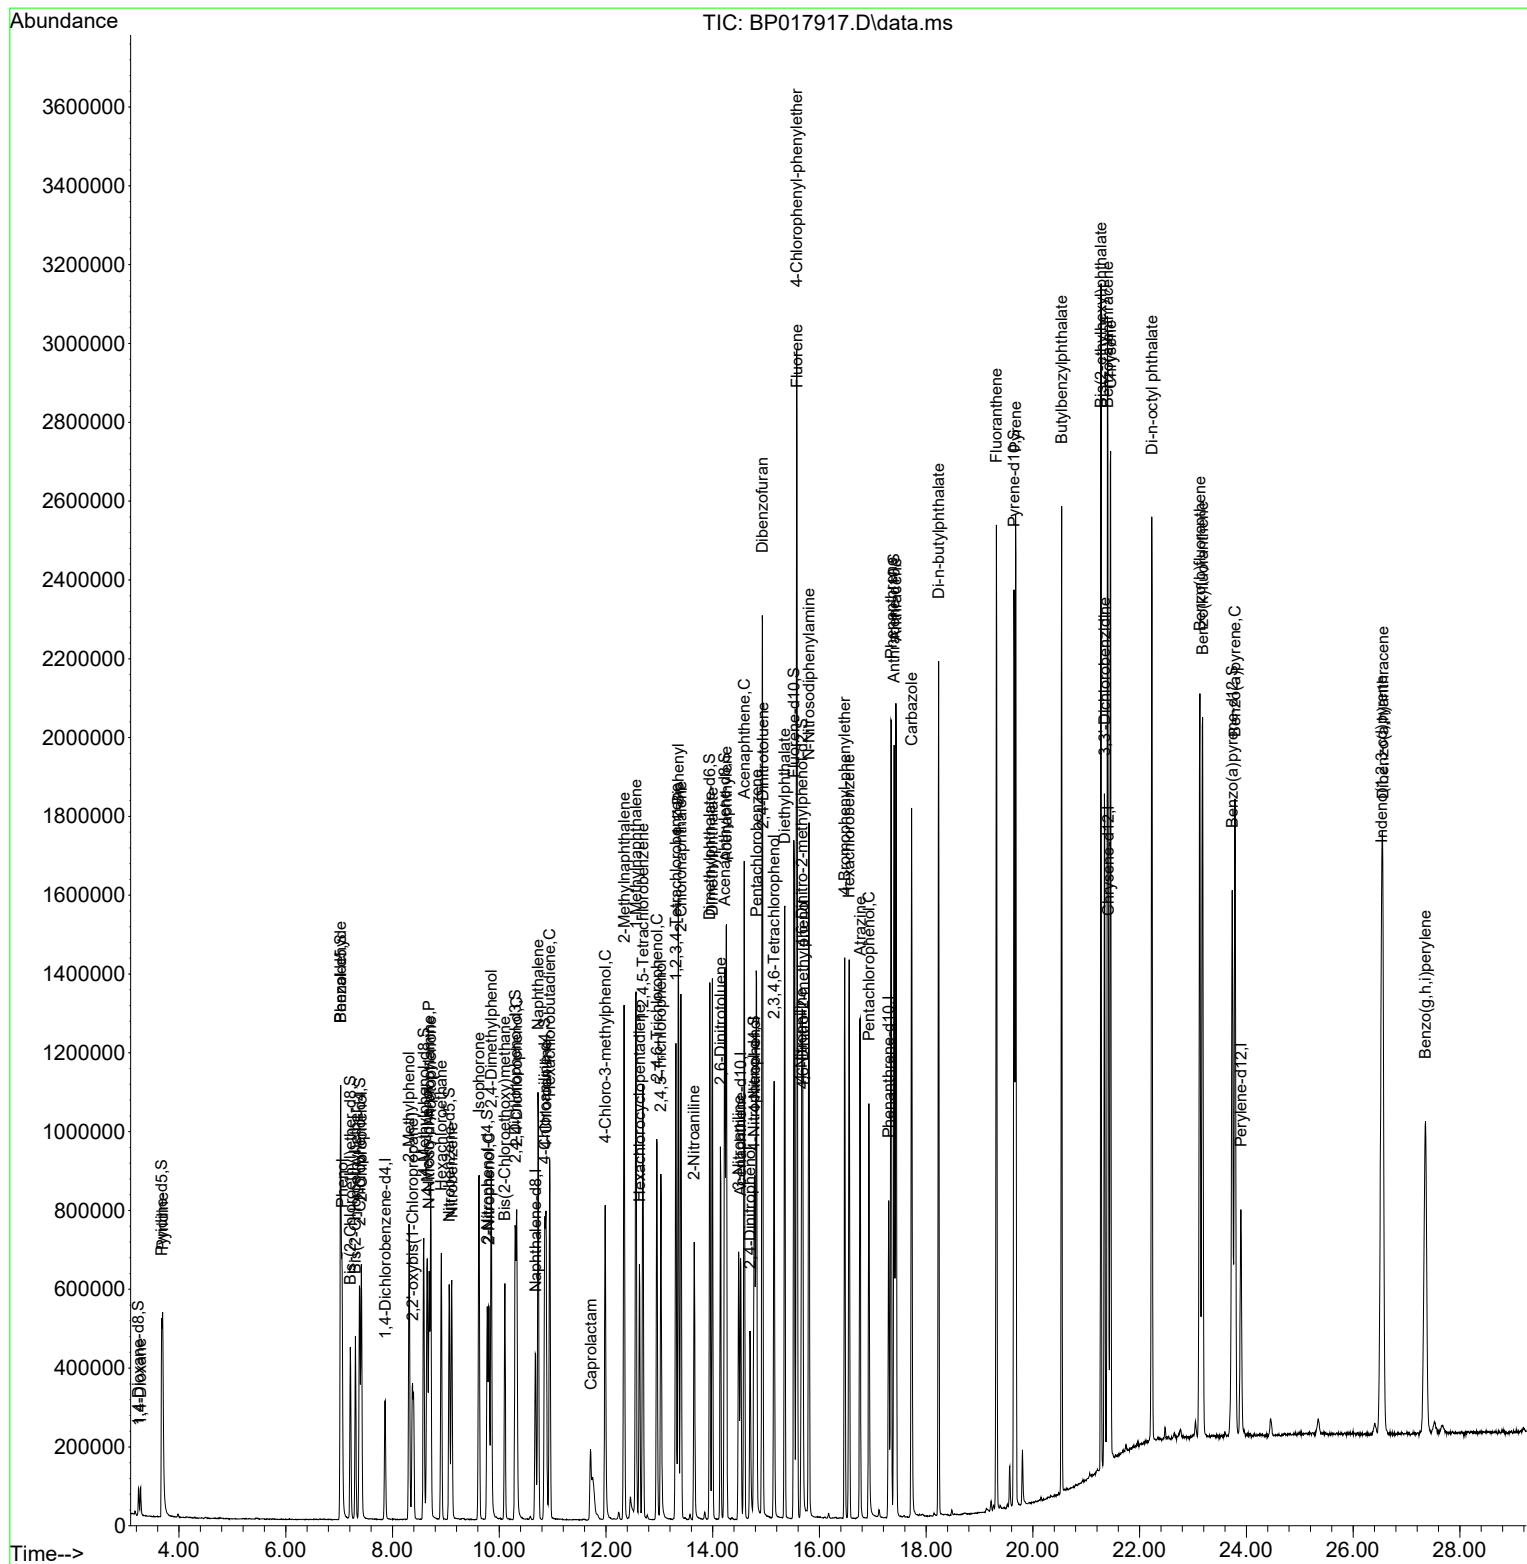


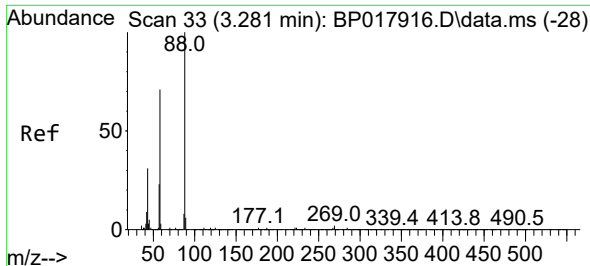

#2
1,4-Dioxane
Concen: 16.281 ng/uL
RT: 3.281 min Scan# 31
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03




Instrument :
BNA_P
ClientSampleId :
SSTD040606


Tgt Ion: 88 Resp: 35605
Ion Ratio Lower Upper
88 100
43 30.7 26.2 39.4
58 66.3 55.6 83.4

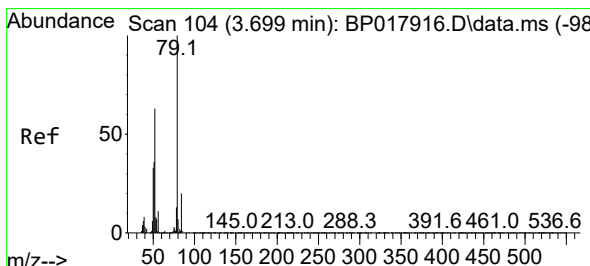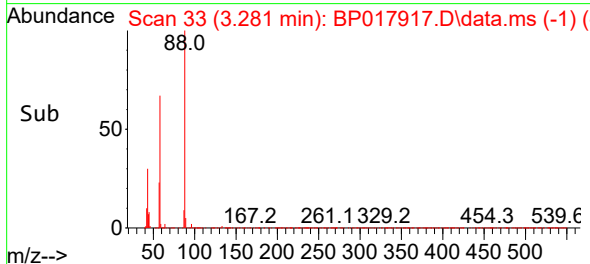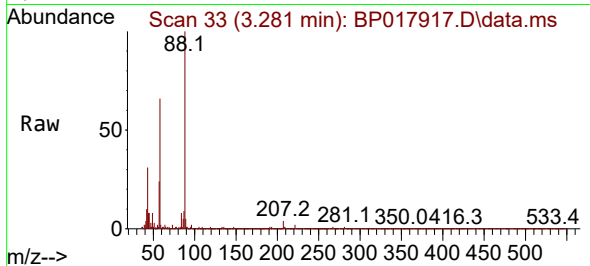

#5
Pyridine
Concen: 42.103 ng/uL
RT: 3.693 min Scan# 103
Delta R.T. -0.006 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03

Tgt Ion: 79 Resp: 236330
Ion Ratio Lower Upper
79 100
52 67.5 51.0 76.6
51 35.9 29.8 44.8



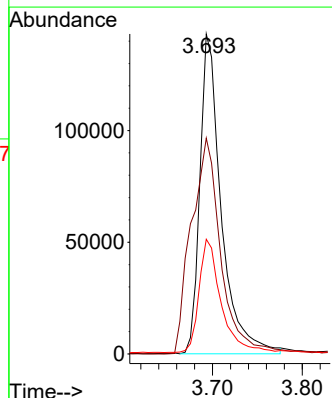
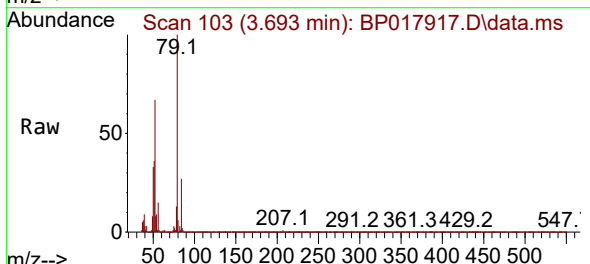




#6
Benzaldehyde
Concen: 45.183 ng/ul
RT: 7.028 min Scan# 61
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03




Instrument :
BNA_P
ClientSampleId :
SSTD040606


Tgt Ion: 77 Resp: 175461
Ion Ratio Lower Upper
77 100
105 90.1 69.0 103.6
106 85.0 66.2 99.4

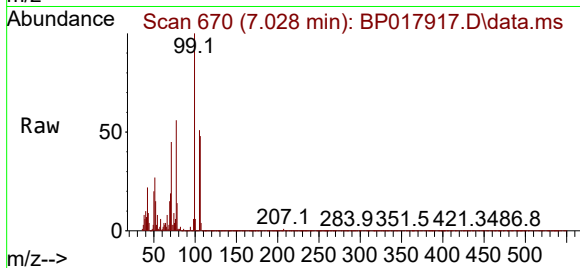

#8
Phenol
Concen: 42.409 ng/ul
RT: 7.058 min Scan# 675
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03

Tgt Ion: 94 Resp: 291273
Ion Ratio Lower Upper
94 100
65 33.6 27.7 41.5
66 48.7 41.7 62.5



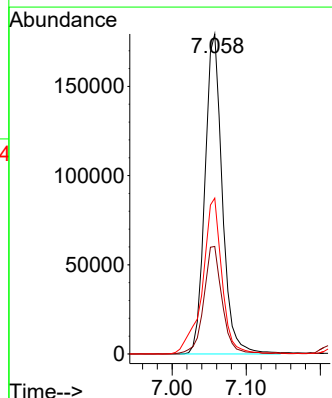
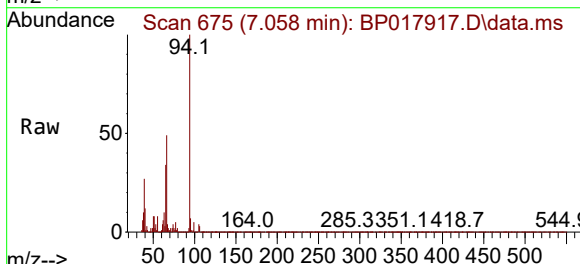




#10
Bis(2-Chloroethyl)ether
Concen: 41.998 ng/ul
RT: 7.305 min Scan# 717
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03




Instrument :
BNA_P
ClientSampleId :
SSTD040606


Tgt Ion: 93 Resp: 231019
Ion Ratio Lower Upper
93 100
63 74.4 57.2 85.8
95 31.7 26.2 39.4



#12
2-Chlorophenol
Concen: 43.530 ng/ul
RT: 7.416 min Scan# 736
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03

Tgt Ion:128 Resp: 237794
Ion Ratio Lower Upper
128 100
64 47.6 39.8 59.6
130 31.9 25.8 38.8



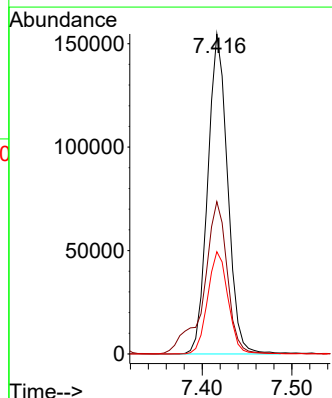





#13
2-Methylphenol
Concen: 42.577 ng/ul
RT: 8.310 min Scan# 889
Delta R.T. -0.006 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03




Instrument :
BNA_P
ClientSampleId :
SSTD040606


Tgt Ion:108 Resp: 224818
Ion Ratio Lower Upper
108 100
107 90.1 70.7 106.1



#14
2,2'-oxybis(1-Chloropropane)
Concen: 22.255 ng/ul
RT: 8.375 min Scan# 899
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03

Tgt Ion: 45 Resp: 140928
Ion Ratio Lower Upper
45 100
77 19.9 14.8 22.2
79 14.6 11.2 16.8









#16
Acetophenone
Concen: 42.050 ng/ul
RT: 8.716 min Scan# 91
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03




Instrument :
BNA_P
ClientSampleId :
SSTD040606


Tgt Ion:105 Resp: 389423
Ion Ratio Lower Upper
105 100
77 85.0 67.7 101.5
51 29.0 23.4 35.2



#17
N-Nitroso-di-n-propylamine
Concen: 42.031 ng/ul
RT: 8.687 min Scan# 952
Delta R.T. 0.006 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03

Tgt Ion: 70 Resp: 211552
Ion Ratio Lower Upper
70 100
42 56.9 45.7 68.5
101 9.6 7.9 11.9
130 19.4 14.6 21.8



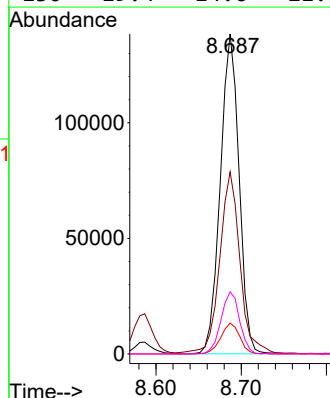





#18
4-Methylphenol
Concen: 42.258 ng/ul
RT: 8.652 min Scan# 946
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03




Instrument :
BNA_P
ClientSampleId :
SSTD040606


Tgt Ion:108 Resp: 240037
Ion Ratio Lower Upper
108 100
107 117.0 87.2 130.8



#19
Hexachloroethane
Concen: 40.850 ng/ul
RT: 8.916 min Scan# 991
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03

Tgt Ion:117 Resp: 113625
Ion Ratio Lower Upper
117 100
201 94.6 79.6 119.4
199 58.3 51.4 77.0









#22
Nitrobenzene
Concen: 44.783 ng/ul
RT: 9.110 min Scan# 1024
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03




Instrument :
BNA_P
ClientSampleId :
SSTD040606


Tgt Ion: 77 Resp: 326565
Ion Ratio Lower Upper
77 100
123 40.4 31.2 46.8
65 13.9 11.5 17.3



#23
Isophorone
Concen: 43.982 ng/ul
RT: 9.622 min Scan# 1111
Delta R.T. 0.006 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03

Tgt Ion: 82 Resp: 586405
Ion Ratio Lower Upper
82 100
95 8.5 7.2 10.8
138 16.6 13.4 20.2









#25
2-Nitrophenol
Concen: 43.563 ng/ul
RT: 9.810 min Scan# 1143
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03




Instrument :
BNA_P
ClientSampleId :
SSTD040606


Tgt Ion:139 Resp: 141494
Ion Ratio Lower Upper
139 100
65 59.8 49.0 73.6
109 42.2 32.8 49.2



#26
2,4-Dimethylphenol
Concen: 43.634 ng/ul
RT: 9.851 min Scan# 1150
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03

Tgt Ion:107 Resp: 296077
Ion Ratio Lower Upper
107 100
121 45.1 37.8 56.8
122 75.9 61.9 92.9





#27

Bis(2-Chloroethoxy)methane

Concen: 43.143 ng/ul

RT: 10.104 min Scan# 1193

Delta R.T. -0.000 min

Lab File: BP017917.D

Acq: 06 Nov 2023 17:03

Instrument :

BNA_P

ClientSampleId :

SSTD040606





Tgt Ion: 93 Resp: 317754

Ion Ratio Lower Upper

93 100

95 31.9 26.2 39.4

123 10.9 9.2 13.8

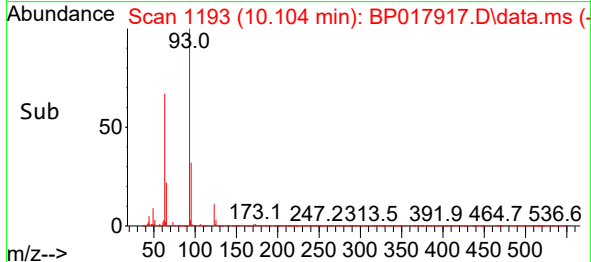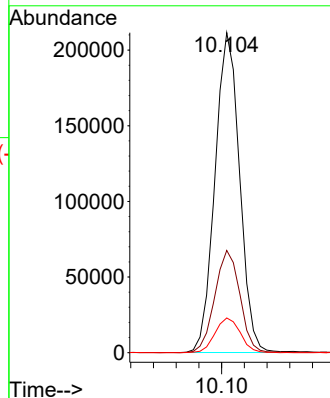

#29

2,4-Dichlorophenol

Concen: 41.586 ng/ul

RT: 10.328 min Scan# 1231

Delta R.T. -0.000 min

Lab File: BP017917.D

Acq: 06 Nov 2023 17:03




Tgt Ion:162 Resp: 233819


Ion Ratio Lower Upper

162 100

164 66.6 49.4 74.2

98 38.2 27.6 41.4


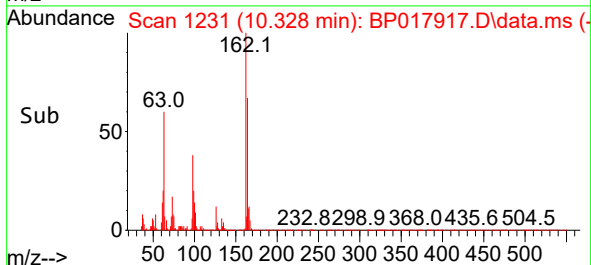
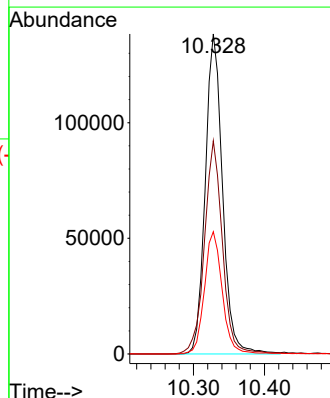
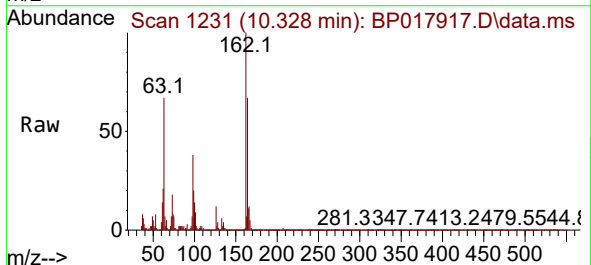




#30
Naphthalene
Concen: 40.917 ng/ul
RT: 10.728 min Scan# 1299
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03




Instrument :
BNA_P
ClientSampleId :
SSTD040606


Tgt Ion:128 Resp: 784028
Ion Ratio Lower Upper
128 100
129 11.2 9.1 13.7
127 13.4 10.6 15.8

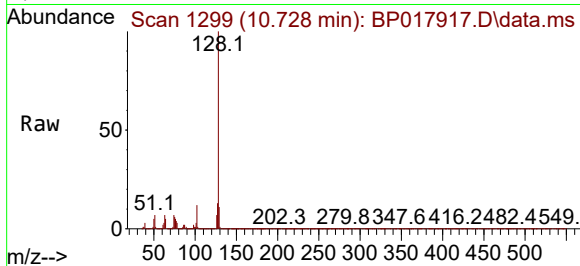

#32
4-Chloroaniline
Concen: 42.575 ng/ul
RT: 10.875 min Scan# 1324
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03

Tgt Ion:127 Resp: 316802
Ion Ratio Lower Upper
127 100
129 30.9 26.2 39.2




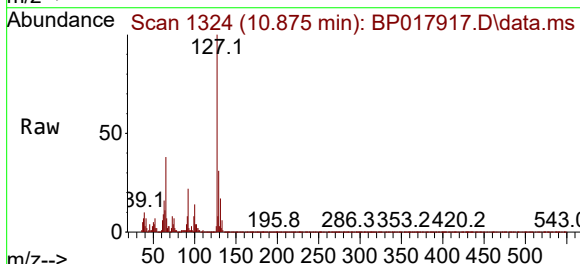




#33
Hexachlorobutadiene
Concen: 37.254 ng/ul
RT: 10.946 min Scan# 1336
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03




Instrument :
BNA_P
ClientSampleId :
SSTD040606


Tgt Ion:225 Resp: 169763
Ion Ratio Lower Upper
225 100
223 62.4 47.7 71.5
227 63.1 50.8 76.2

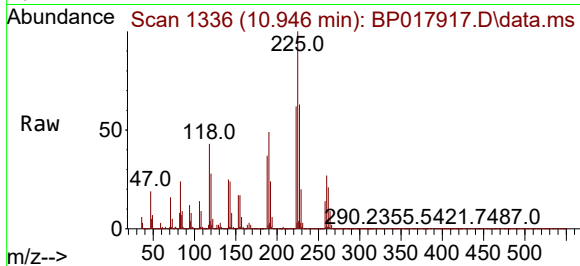

#34
Caprolactam
Concen: 24.025 ng/ul
RT: 11.716 min Scan# 1467
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03

Tgt Ion:113 Resp: 39972
Ion Ratio Lower Upper
113 100
55 141.3 114.1 171.1
56 118.9 91.7 137.5









#35
4-Chloro-3-methylphenol
Concen: 43.607 ng/ul
RT: 11.987 min Scan# 1513
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03




Instrument :
BNA_P
ClientSampleId :
SSTD040606


Tgt Ion:107 Resp: 274549
Ion Ratio Lower Upper
107 100
144 24.2 20.8 31.2
142 72.6 62.2 93.2

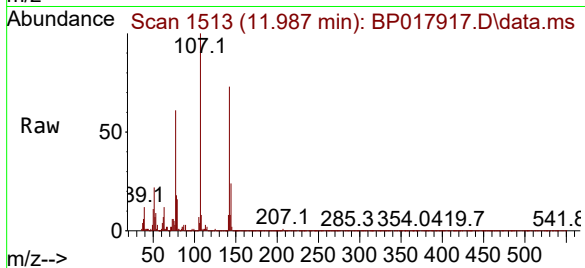

#36
2-Methylnaphthalene
Concen: 40.932 ng/ul
RT: 12.340 min Scan# 1573
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03

Tgt Ion:142 Resp: 540465
Ion Ratio Lower Upper
142 100
141 90.4 70.9 106.3

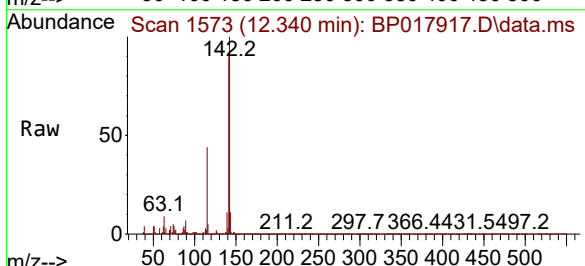

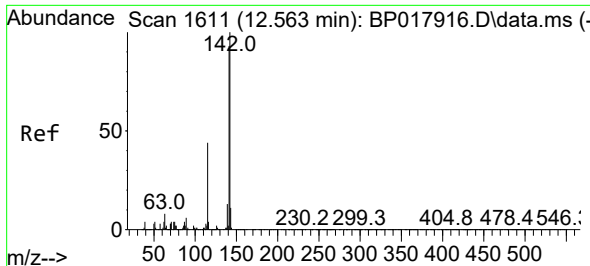

#37

1-Methylnaphthalene

Concen: 40.587 ng/ul

RT: 12.563 min Scan# 1611

Delta R.T. -0.000 min

Lab File: BP017917.D

Acq: 06 Nov 2023 17:03

Instrument :

BNA_P

ClientSampleId :

SSTD040606





Tgt Ion:142 Resp: 551297

Ion Ratio Lower Upper

142 100

141 92.8 74.3 111.5

116 4.8 3.6 5.4

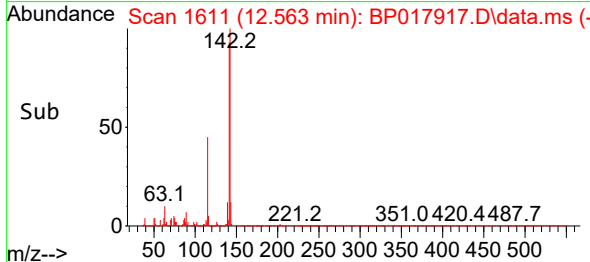

#39

1,2,4,5-Tetrachlorobenzene

Concen: 39.832 ng/ul

RT: 12.693 min Scan# 1633

Delta R.T. -0.000 min

Lab File: BP017917.D

Acq: 06 Nov 2023 17:03

Tgt Ion:216 Resp: 290468




Ion Ratio Lower Upper


216 100

214 78.7 63.4 95.2

179 23.4 18.9 28.3

108 19.5 15.3 22.9


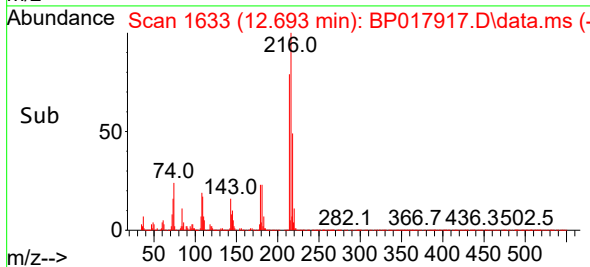
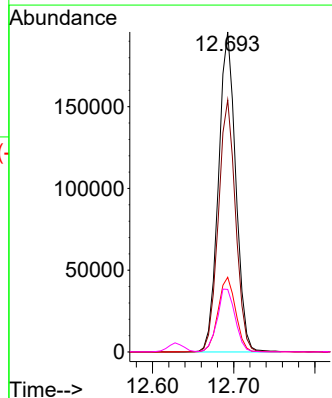
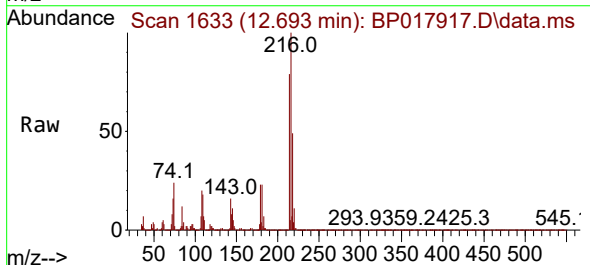




#40
Hexachlorocyclopentadiene
Concen: 40.976 ng/ul
RT: 12.628 min Scan# 1622
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03




Instrument :
BNA_P
ClientSampleId :
SSTD040606


Tgt Ion:237 Resp: 152783
Ion Ratio Lower Upper
237 100
235 63.2 51.3 76.9
272 11.5 9.4 14.2



#41
2,4,6-Trichlorophenol
Concen: 41.731 ng/ul
RT: 12.957 min Scan# 1678
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03

Tgt Ion:196 Resp: 193926
Ion Ratio Lower Upper
196 100
198 96.8 78.5 117.7
200 31.2 24.1 36.1





#42

2,4,5-Trichlorophenol

Concen: 41.665 ng/ul

RT: 13.028 min Scan# 1

Delta R.T. -0.006 min

Lab File: BP017917.D

Acq: 06 Nov 2023 17:03

Instrument :

BNA_P

ClientSampleId :

SSTD040606





Tgt Ion:196 Resp: 202502

Ion Ratio Lower Upper

196 100

198 93.0 78.5 117.7

200 30.8 25.3 37.9

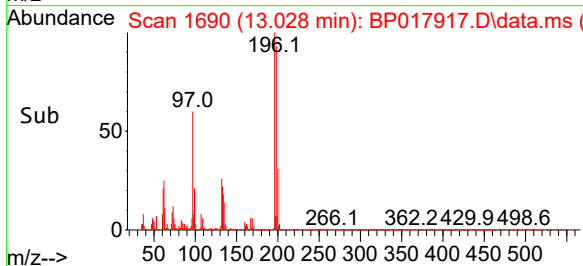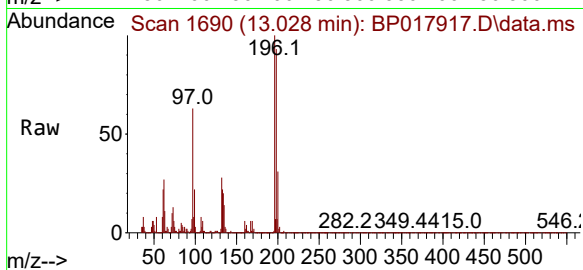

#43

1,1'-Biphenyl

Concen: 41.902 ng/ul

RT: 13.357 min Scan# 1746

Delta R.T. -0.000 min

Lab File: BP017917.D

Acq: 06 Nov 2023 17:03




Tgt Ion:154 Resp: 724379


Ion Ratio Lower Upper

154 100

153 40.2 31.8 47.8

76 12.1 8.5 12.7


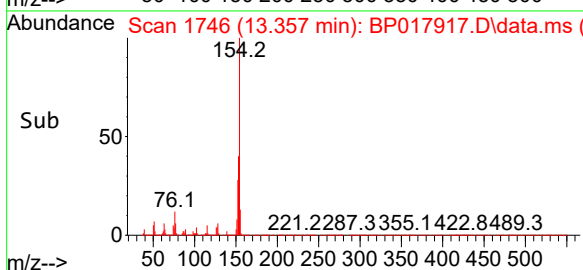

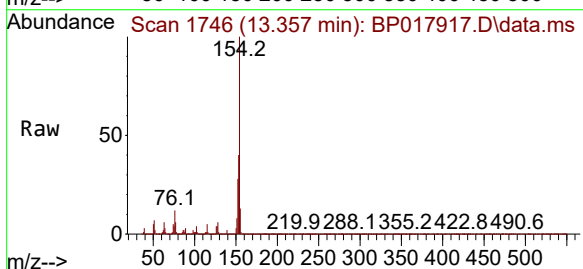




#44
2-Chloronaphthalene
Concen: 41.310 ng/ul
RT: 13.404 min Scan# 1754
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03




Instrument :
BNA_P
ClientSampleId :
SSTD040606


Tgt Ion:162 Resp: 571662
Ion Ratio Lower Upper
162 100
164 32.7 26.7 40.1
127 43.9 33.0 49.6



#45
2-Nitroaniline
Concen: 47.298 ng/ul
RT: 13.651 min Scan# 1796
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03

Tgt Ion: 65 Resp: 194962
Ion Ratio Lower Upper
65 100
92 64.3 53.9 80.9
138 90.3 79.1 118.7









#47
Dimethylphthalate
Concen: 40.965 ng/ul
RT: 13.992 min Scan# 1854
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03




Instrument :
BNA_P
ClientSampleId :
SSTD040606


Tgt Ion:163 Resp: 755296
Ion Ratio Lower Upper
163 100
194 4.0 3.2 4.8
164 10.4 8.2 12.4



#48
2,6-Dinitrotoluene
Concen: 42.741 ng/ul
RT: 14.145 min Scan# 1880
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03

Tgt Ion:165 Resp: 155915
Ion Ratio Lower Upper
165 100
89 76.7 54.9 82.3
121 23.4 19.0 28.6









#50
Acenaphthylene
Concen: 41.653 ng/ul
RT: 14.257 min Scan# 1899
Delta R.T. 0.006 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03




Instrument :
BNA_P
ClientSampleId :
SSTD040606


Tgt Ion:152 Resp: 954482
Ion Ratio Lower Upper
152 100
151 19.8 15.9 23.9
153 13.2 10.4 15.6



#51
3-Nitroaniline
Concen: 45.035 ng/ul
RT: 14.487 min Scan# 1938
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03

Tgt Ion:138 Resp: 147167
Ion Ratio Lower Upper
138 100
108 11.7 8.4 12.6
92 126.3 94.2 141.4





#52

Acenaphthene

Concen: 41.258 ng/ul

RT: 14.592 min Scan# 1956

Delta R.T. 0.006 min

Lab File: BP017917.D

Acq: 06 Nov 2023 17:03

Instrument :

BNA_P

ClientSampleId :

SSTD040606





Tgt Ion:153 Resp: 627728

Ion Ratio Lower Upper

153 100

152 47.9 37.7 56.5

154 87.1 70.4 105.6



#53

2,4-Dinitrophenol

Concen: 42.658 ng/ul

RT: 14.698 min Scan# 1974

Delta R.T. -0.006 min

Lab File: BP017917.D

Acq: 06 Nov 2023 17:03




Tgt Ion:184 Resp: 87107


Ion Ratio Lower Upper

184 100

63 84.3 54.5 81.7#

154 80.5 56.4 84.6









#55
4-Nitrophenol
Concen: 49.396 ng/ul
RT: 14.787 min Scan# 1989
Delta R.T. -0.006 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03




Instrument :
BNA_P
ClientSampleId :
SSTD040606


Tgt Ion:109 Resp: 161764
Ion Ratio Lower Upper
109 100
139 87.1 79.6 119.4
65 112.5 87.8 131.8



#56
Dibenzofuran
Concen: 40.796 ng/ul
RT: 14.928 min Scan# 2013
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03

Tgt Ion:168 Resp: 862290
Ion Ratio Lower Upper
168 100
139 43.1 33.8 50.6





#57

2,4-Dinitrotoluene

Concen: 43.207 ng/ul

RT: 14.939 min Scan# 2014

Delta R.T. 0.006 min

Lab File: BP017917.D

Acq: 06 Nov 2023 17:03

Instrument :

BNA_P

ClientSampleId :

SSTD040606





Tgt Ion:165 Resp: 233734

Ion Ratio Lower Upper

165 100

63 60.5 53.3 79.9

182 2.5 1.9 2.9

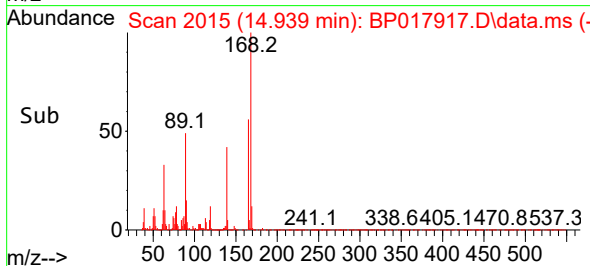

#58

2,3,4,6-Tetrachlorophenol

Concen: 39.352 ng/ul

RT: 15.151 min Scan# 2051

Delta R.T. -0.000 min

Lab File: BP017917.D

Acq: 06 Nov 2023 17:03

Tgt Ion:232 Resp: 177772




Ion Ratio Lower Upper


232 100

131 53.2 38.3 57.5

130 2.9 2.2 3.4

166 33.9 25.2 37.8


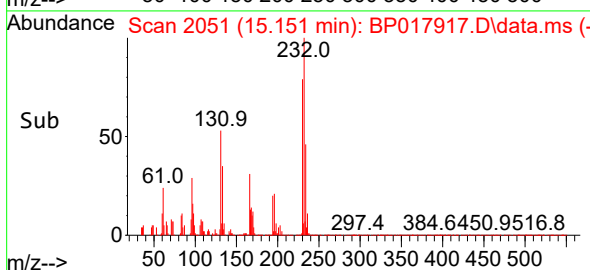

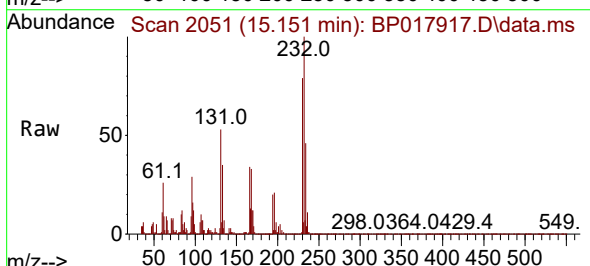




#59
Diethylphthalate
Concen: 41.425 ng/ul
RT: 15.351 min Scan# 2085
Delta R.T. 0.006 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03




Instrument :
BNA_P
ClientSampleId :
SSTD040606


Tgt Ion:149 Resp: 797004
Ion Ratio Lower Upper
149 100
177 21.2 16.4 24.6
150 12.6 9.7 14.5

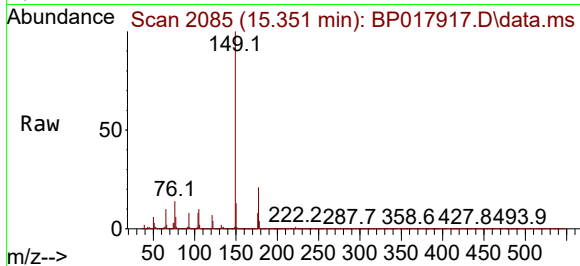

#61
Fluorene
Concen: 40.819 ng/ul
RT: 15.581 min Scan# 2124
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03

Tgt Ion:166 Resp: 728182
Ion Ratio Lower Upper
166 100
165 97.7 79.8 119.6
167 13.2 10.9 16.3









#62
4-Chlorophenyl-phenylether
Concen: 39.539 ng/ul
RT: 15.575 min Scan# 2123
Delta R.T. 0.006 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03




Instrument :
BNA_P
ClientSampleId :
SSTD040606


Tgt Ion:204 Resp: 364255
Ion Ratio Lower Upper
204 100
206 31.2 26.0 39.0
141 68.1 53.6 80.4

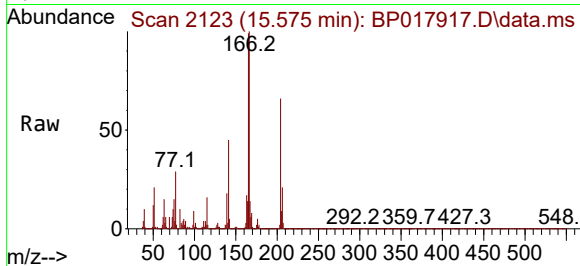

#63
4-Nitroaniline
Concen: 45.337 ng/ul
RT: 15.663 min Scan# 2138
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03

Tgt Ion:138 Resp: 138493
Ion Ratio Lower Upper
138 100
92 61.3 45.4 68.2
108 131.7 103.1 154.7




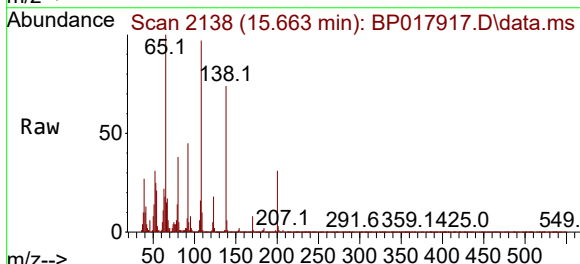




#66
4,6-Dinitro-2-methylphenol
Concen: 43.026 ng/ul
RT: 15.692 min Scan# 2143
Delta R.T. 0.006 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03




Instrument :
BNA_P
ClientSampleId :
SSTD040606


Tgt Ion:198 Resp: 144913
Ion Ratio Lower Upper
198 100
182 3.7 4.4 6.6#
77 30.9 24.6 37.0

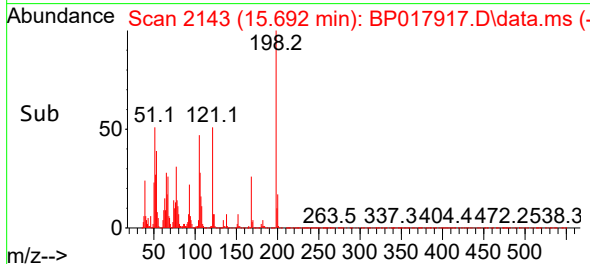

#67
N-Nitrosodiphenylamine
Concen: 42.545 ng/ul
RT: 15.804 min Scan# 2162
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03

Tgt Ion:169 Resp: 602913
Ion Ratio Lower Upper
169 100
168 66.6 53.4 80.0
167 37.7 28.0 42.0




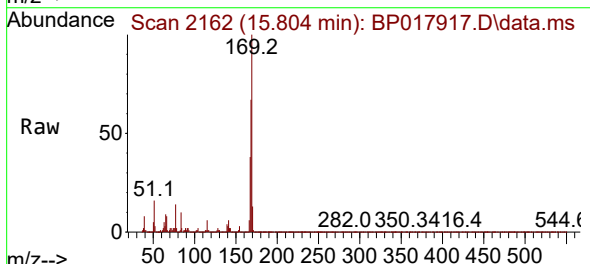




#68
4-Bromophenyl-phenylether
Concen: 39.096 ng/ul
RT: 16.475 min Scan# 21
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03




Instrument :
BNA_P
ClientSampleId :
SSTD040606


Tgt Ion:248 Resp: 213044
Ion Ratio Lower Upper
248 100
250 96.5 77.9 116.9
141 91.2 62.4 93.6

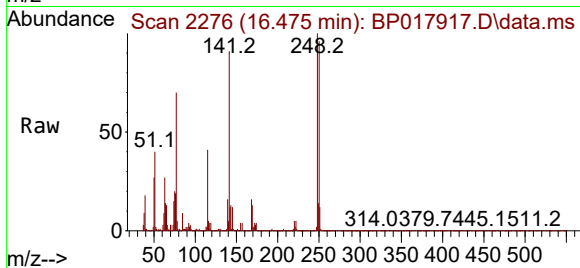

#69
Hexachlorobenzene
Concen: 37.789 ng/ul
RT: 16.557 min Scan# 2290
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03

Tgt Ion:284 Resp: 235131
Ion Ratio Lower Upper
284 100
142 44.9 29.0 43.6#
249 34.7 25.8 38.6

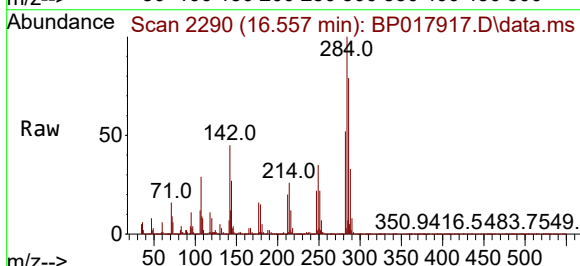



#70

Atrazine

Concen: 43.196 ng/ul

RT: 16.763 min Scan# 21

Delta R.T. 0.006 min

Lab File: BP017917.D

Acq: 06 Nov 2023 17:03

Instrument :

BNA_P

ClientSampleId :

SSTD040606





Tgt Ion:200 Resp: 223847

Ion Ratio Lower Upper

200 100

173 26.4 20.2 30.4

215 47.7 37.7 56.5

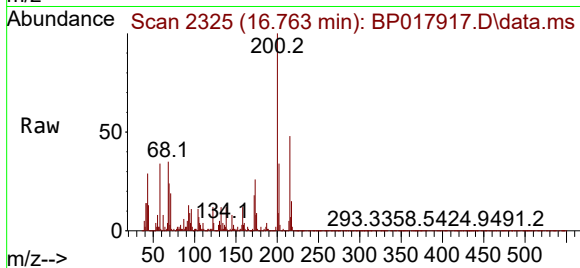

#71

Pentachlorophenol

Concen: 40.169 ng/ul

RT: 16.928 min Scan# 2353

Delta R.T. -0.000 min

Lab File: BP017917.D

Acq: 06 Nov 2023 17:03




Tgt Ion:266 Resp: 145387


Ion Ratio Lower Upper

266 100

264 61.4 53.8 80.6

268 63.0 52.4 78.6

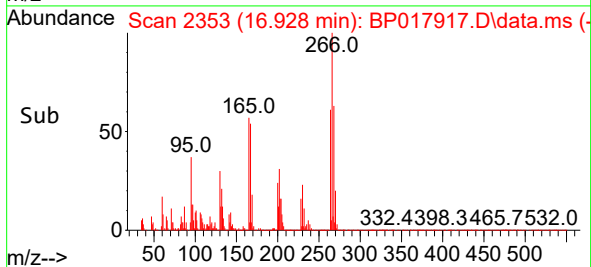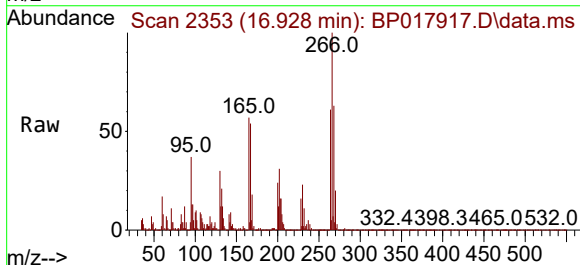



#72

Phenanthrene

Concen: 41.495 ng/ul

RT: 17.345 min Scan# 2423

Delta R.T. 0.006 min

Lab File: BP017917.D

Acq: 06 Nov 2023 17:03

Instrument :

BNA_P

ClientSampleId :

SSTD040606





Tgt Ion:178 Resp: 1128464

Ion Ratio Lower Upper

178 100

179 15.3 12.3 18.5

176 19.4 15.2 22.8

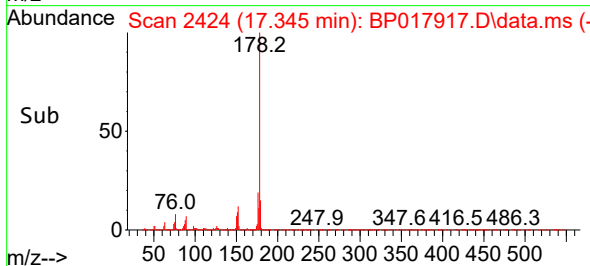

#74

Anthracene

Concen: 41.966 ng/ul

RT: 17.433 min Scan# 2439

Delta R.T. -0.000 min

Lab File: BP017917.D

Acq: 06 Nov 2023 17:03




Tgt Ion:178 Resp: 1159540


Ion Ratio Lower Upper

178 100

179 15.7 12.5 18.7

176 18.9 14.9 22.3


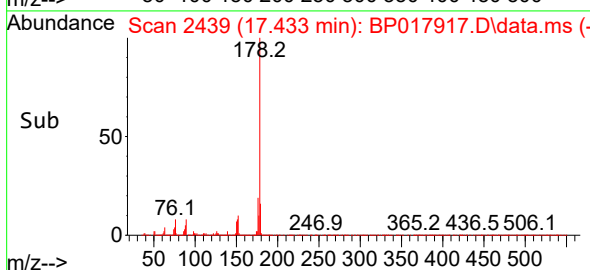

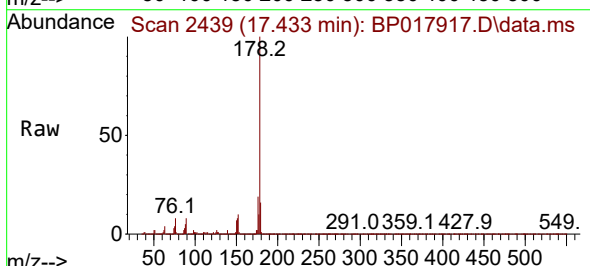




#75
1,2,3,4-Tetrachlorobenzene
Concen: 40.711 ng/uL
RT: 13.310 min Scan# 1738
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03




Instrument :
BNA_P
ClientSampleId :
SSTD040606


Tgt Ion:216 Resp: 292951
Ion Ratio Lower Upper
216 100
214 78.5 62.3 93.5
218 48.7 39.8 59.6



#76
Pentachlorobenzene
Concen: 39.255 ng/uL
RT: 14.822 min Scan# 1995
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03

Tgt Ion:250 Resp: 281345
Ion Ratio Lower Upper
250 100
248 62.5 48.5 72.7
252 62.8 50.2 75.4

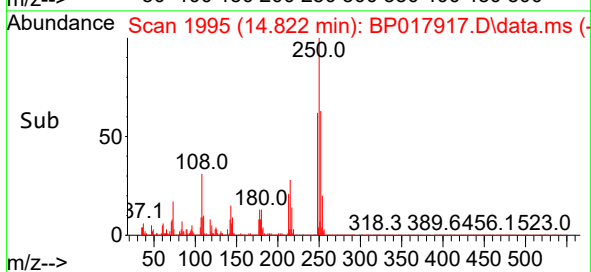



#77

Carbazole

Concen: 43.503 ng/ul

RT: 17.728 min Scan# 2489

Delta R.T. -0.000 min

Lab File: BP017917.D

Acq: 06 Nov 2023 17:03

Instrument :

BNA_P

ClientSampleId :

SSTD040606





Tgt Ion:167 Resp: 1022137

Ion Ratio Lower Upper

167 100

166 21.6 17.7 26.5

139 14.4 11.0 16.4



#78

Di-n-butylphthalate

Concen: 44.713 ng/ul

RT: 18.233 min Scan# 2575

Delta R.T. -0.000 min

Lab File: BP017917.D

Acq: 06 Nov 2023 17:03




Tgt Ion:149 Resp: 1375725


Ion Ratio Lower Upper

149 100

150 9.2 7.4 11.2

104 6.5 5.0 7.6





#80

Fluoranthene

Concen: 42.756 ng/ul

RT: 19.316 min Scan# 2759

Delta R.T. -0.000 min

Lab File: BP017917.D

Acq: 06 Nov 2023 17:03

Instrument :

BNA_P

ClientSampleId :

SSTD040606





Tgt Ion:202 Resp: 1346509

Ion Ratio Lower Upper

202 100

101 9.5 7.1 10.7

100 7.4 5.3 7.9



#82

Pyrene

Concen: 42.668 ng/ul

RT: 19.674 min Scan# 2820

Delta R.T. -0.000 min

Lab File: BP017917.D

Acq: 06 Nov 2023 17:03




Tgt Ion:202 Resp: 1398437


Ion Ratio Lower Upper

202 100

101 10.9 8.6 12.8

100 9.1 7.3 10.9



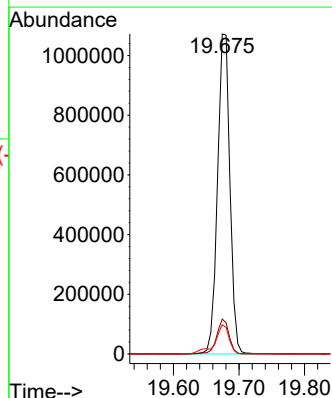
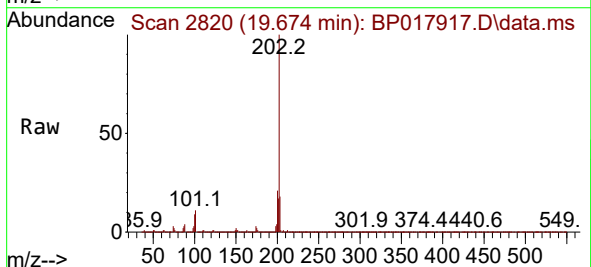




#83
Butylbenzylphthalate
Concen: 44.511 ng/ul
RT: 20.539 min Scan# 2967
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03




Instrument :
BNA_P
ClientSampleId :
SSTD040606


Tgt Ion:149 Resp: 641106
Ion Ratio Lower Upper
149 100
91 75.5 60.4 90.6
206 20.2 15.3 22.9



#84
3,3'-Dichlorobenzidine
Concen: 43.186 ng/ul
RT: 21.345 min Scan# 3104
Delta R.T. -0.000 min
Lab File: BP017917.D
Acq: 06 Nov 2023 17:03

Tgt Ion:252 Resp: 437163
Ion Ratio Lower Upper
252 100
254 64.2 50.7 76.1
126 11.0 7.9 11.9





#85

Benzo(a)anthracene

Concen: 41.455 ng/ul

RT: 21.398 min Scan# 3113

Delta R.T. -0.000 min

Lab File: BP017917.D

Acq: 06 Nov 2023 17:03

Instrument :

BNA_P

ClientSampleId :

SSTD040606





Tgt Ion:228 Resp: 1357601

Ion Ratio Lower Upper

228 100

229 19.8 15.4 23.2

226 27.7 21.6 32.4



#86

Bis(2-ethylhexyl)phthalate

Concen: 44.949 ng/ul

RT: 21.274 min Scan# 3092

Delta R.T. -0.000 min

Lab File: BP017917.D

Acq: 06 Nov 2023 17:03




Tgt Ion:149 Resp: 929191


Ion Ratio Lower Upper

149 100

167 25.8 21.0 31.6

279 3.6 3.0 4.6

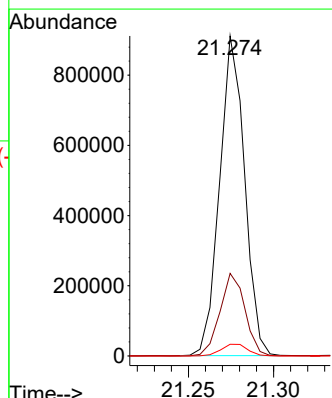



#87

Chrysene

Concen: 41.352 ng/ul

RT: 21.457 min Scan# 3122

Delta R.T. 0.006 min

Lab File: BP017917.D

Acq: 06 Nov 2023 17:03

Instrument :

BNA_P

ClientSampleId :

SSTD040606





Tgt Ion:228 Resp: 1253645

Ion Ratio Lower Upper

228 100

226 30.4 23.9 35.9

229 19.5 16.1 24.1



#89

Di-n-octyl phthalate

Concen: 43.492 ng/ul




RT: 22.227 min Scan# 3254


Delta R.T. -0.000 min

Lab File: BP017917.D

Acq: 06 Nov 2023 17:03

Tgt Ion:149 Resp: 1553842





#90

Benzo(b)fluoranthene

Concen: 41.339 ng/ul

RT: 23.127 min Scan# 3407

Delta R.T. -0.000 min

Lab File: BP017917.D

Acq: 06 Nov 2023 17:03

Instrument :

BNA_P

ClientSampleId :

SSTD040606





Tgt Ion:252 Resp: 1271962

Ion Ratio Lower Upper

252 100

253 22.3 17.9 26.9

125 8.4 6.6 10.0



#91

Benzo(k)fluoranthene

Concen: 41.488 ng/ul

RT: 23.180 min Scan# 3416

Delta R.T. 0.006 min

Lab File: BP017917.D

Acq: 06 Nov 2023 17:03




Tgt Ion:252 Resp: 1272675


Ion Ratio Lower Upper

252 100

253 21.5 17.2 25.8

125 8.0 7.0 10.6





#93

Benzo(a)pyrene

Concen: 41.767 ng/ul

RT: 23.786 min Scan# 3519

Delta R.T. 0.006 min

Lab File: BP017917.D

Acq: 06 Nov 2023 17:03

Instrument :

BNA_P

ClientSampleId :

SSTD040606





Tgt Ion:252 Resp: 1189543

Ion Ratio Lower Upper

252 100

253 22.0 17.3 25.9

125 9.5 7.5 11.3



#94

Indeno(1,2,3-cd)pyrene

Concen: 40.785 ng/ul

RT: 26.533 min Scan# 3986

Delta R.T. 0.006 min

Lab File: BP017917.D

Acq: 06 Nov 2023 17:03




Tgt Ion:276 Resp: 1392063


Ion Ratio Lower Upper

276 100

138 19.6 15.9 23.9

277 24.2 19.5 29.3

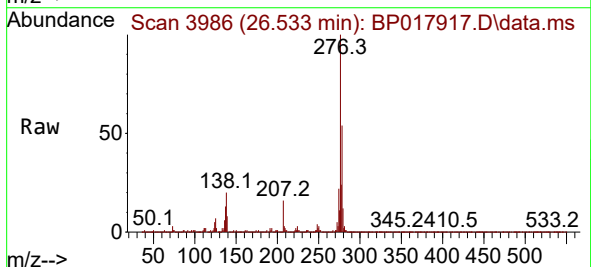



#95

Dibenzo(a,h)anthracene

Concen: 41.049 ng/ul

RT: 26.556 min Scan# 3989

Delta R.T. 0.006 min

Lab File: BP017917.D

Acq: 06 Nov 2023 17:03

Instrument :

BNA_P

ClientSampleId :

SSTD040606





Tgt Ion:278 Resp: 1163502

Ion Ratio Lower Upper

278 100

139 13.1 11.0 16.4

279 24.0 19.1 28.7

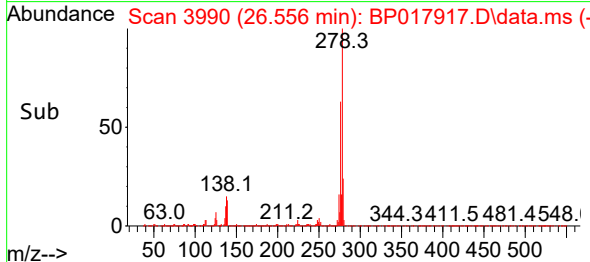

#96

Benzo(g,h,i)perylene

Concen: 40.843 ng/ul

RT: 27.356 min Scan# 4126

Delta R.T. 0.006 min

Lab File: BP017917.D

Acq: 06 Nov 2023 17:03

Tgt Ion:276 Resp: 1110602

Ion Ratio Lower Upper

276 100

138 17.4 14.7 22.1

277 24.0 19.2 28.8

