

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP110719\
 Data File : BP000996.D
 Acq On : 07 Nov 2019 10:38
 Operator : JU
 Sample : PB124575BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Nov 07 12:04:33 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP110619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 11:57:49 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.37	152	270564	20.00	ng	0.00
21) Naphthalene-d8	10.40	136	997857	20.00	ng	0.00
39) Acenaphthene-d10	13.26	164	580829	20.00	ng	0.00
64) Phenanthrene-d10	15.66	188	1222874	20.00	ng	0.00
76) Chrysene-d12	19.29	240	1081923	20.00	ng	0.00
87) Perylene-d12	21.08	264	1211618	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	6.30	112	1339674	90.12	ng	0.00
7) Phenol-d6	7.81	99	1147491	61.05	ng	0.00
23) Nitrobenzene-d5	9.25	82	1722830	95.51	ng	0.00
42) 2,4,6-Tribromophenol	14.56	330	1038280	149.74	ng	0.00
45) 2-Fluorobiphenyl	12.18	172	3621984	93.92	ng	0.00
79) Terphenyl-d14	17.94	244	5137130	94.45	ng	0.00
Target Compounds						
15) Benzyl Alcohol	8.62	79	30526	2.131	ng	# 52
19) n-Nitroso-di-n-propylamine	9.25	70	227396	20.147	ng	# 78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP110719\
Data File : BP000996.D
Acq On : 07 Nov 2019 10:38
Operator : JU
Sample : PB124575BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Nov 07 12:04:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP110619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 11:57:49 2019
Response via : Initial Calibration

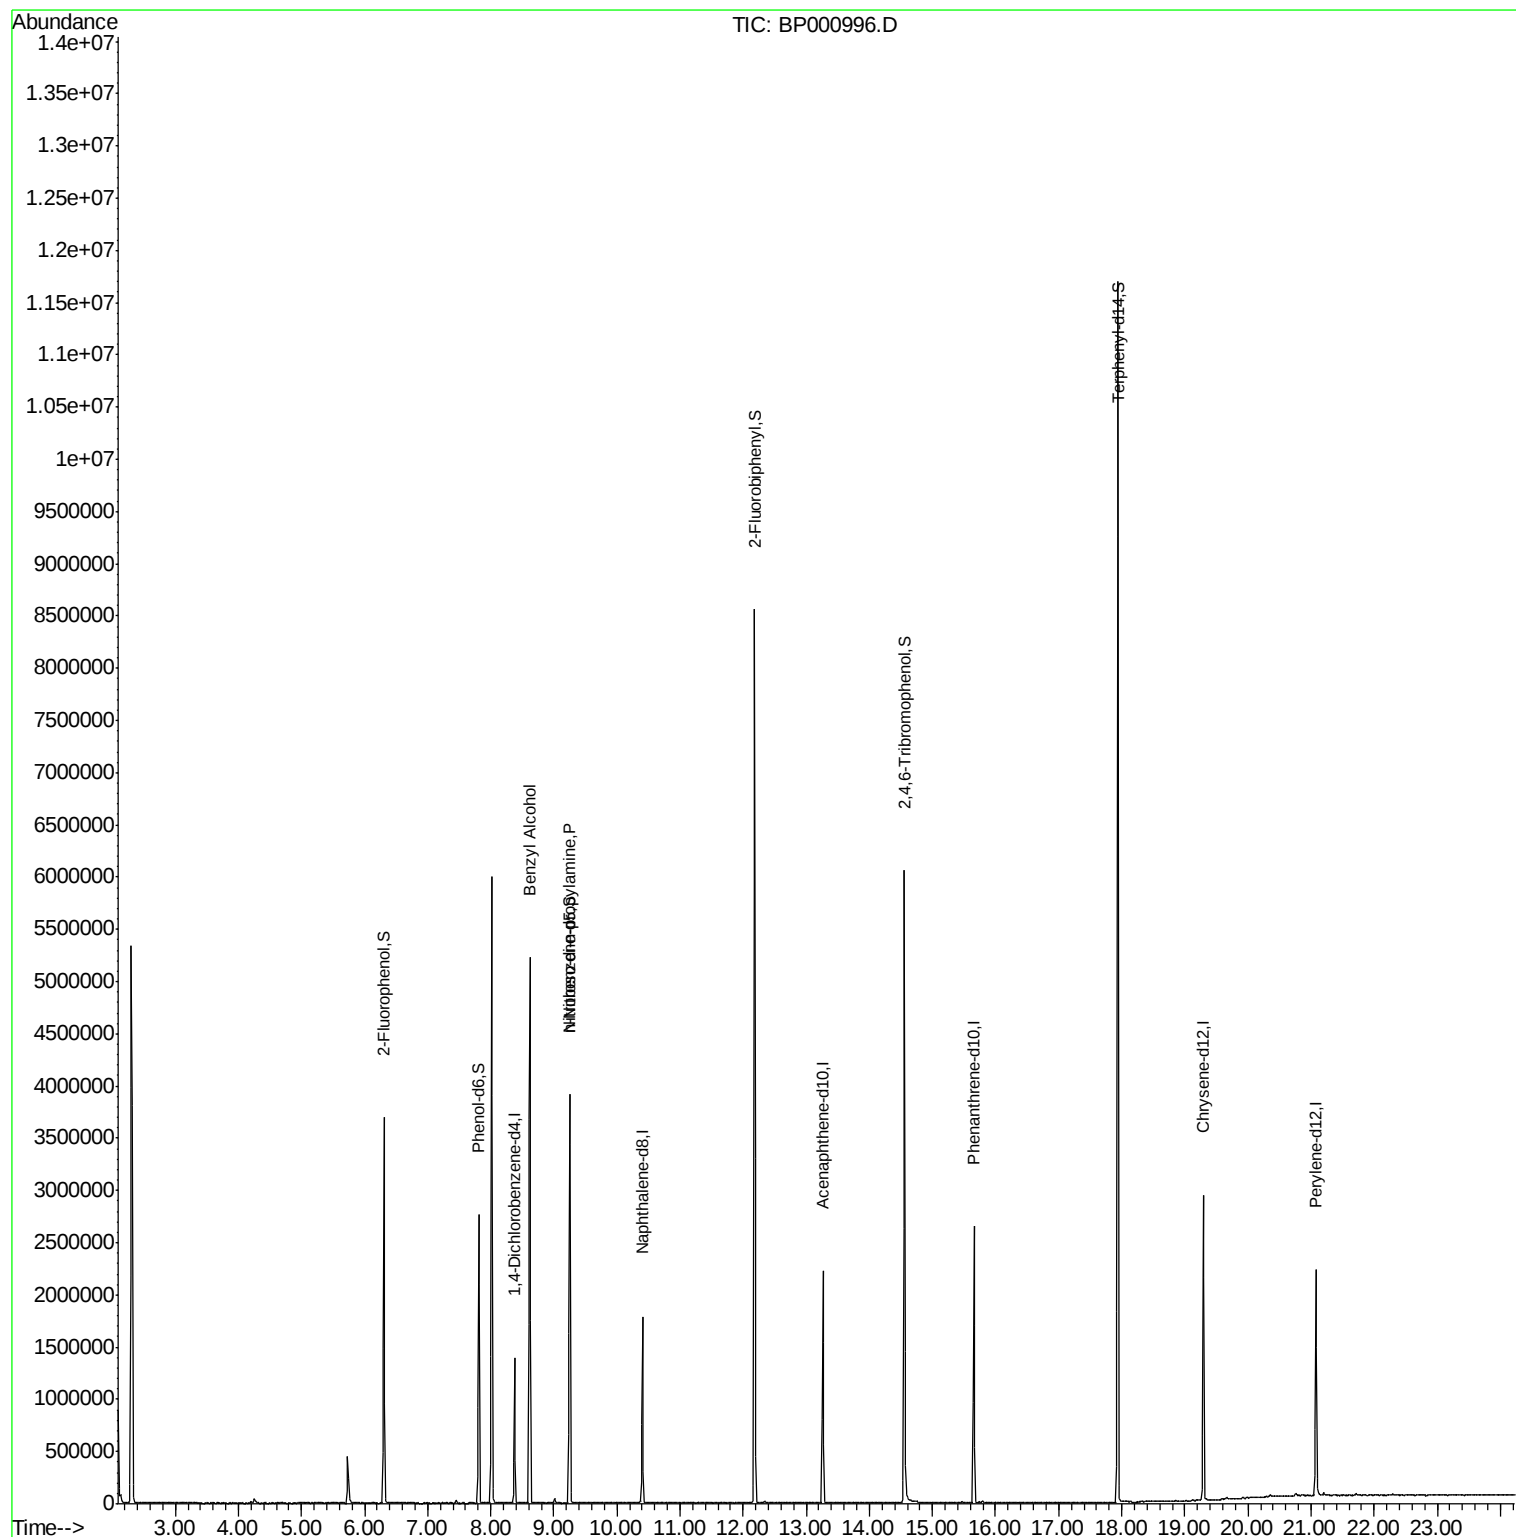

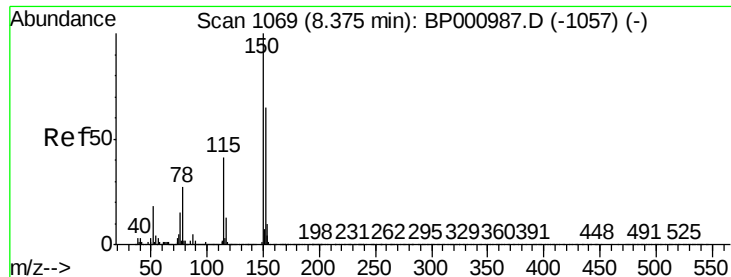

#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 8.37 min Scan# 1069

Delta R.T. -0.00 min

Lab File: BP000996.D

Acq: 07 Nov 2019 10:38

Instrument :

BNA_P

ClientSampled :


Tot Ion:152 Resp: 270564

Ion Ratio Lower Upper

152 100

150 153.5 123.6 185.4




115 60.4 50.1 75.1

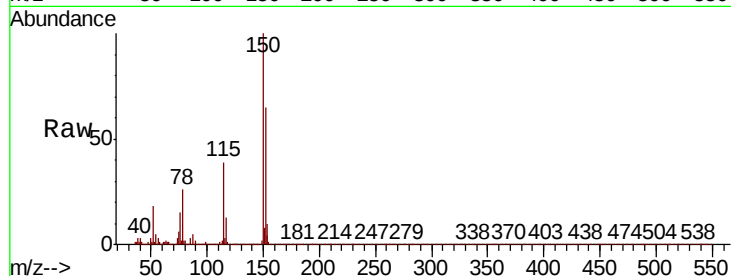

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

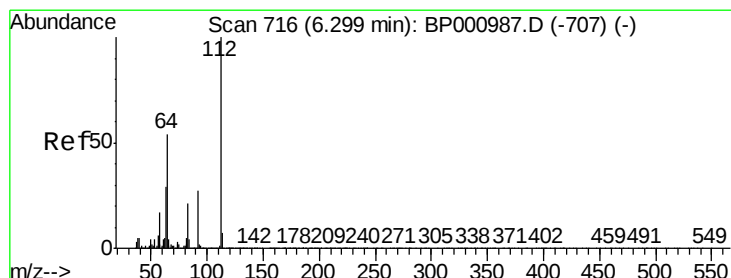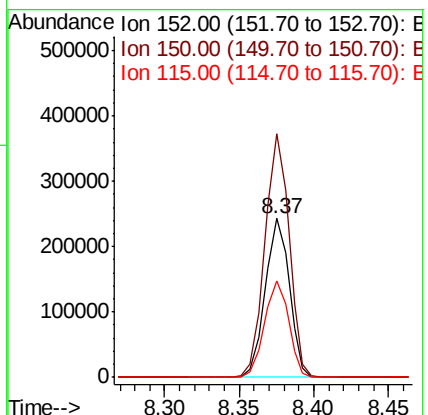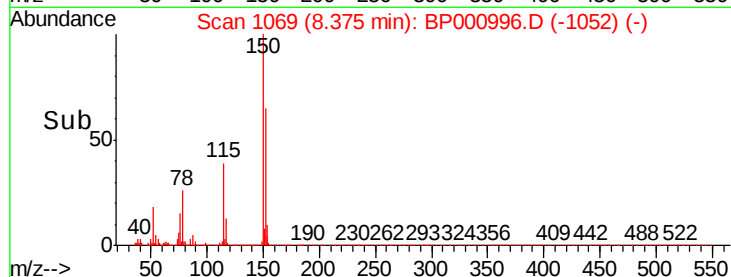

#5

2-Fluorophenol

Concen: 90.124 ng

RT: 6.30 min Scan# 717

Delta R.T. 0.01 min

Lab File: BP000996.D

Acq: 07 Nov 2019 10:38


Tgt Ion:112 Resp: 1339674

Ion Ratio Lower Upper

112 100

64 53.6 43.4 65.0



63 28.9 23.4 35.0

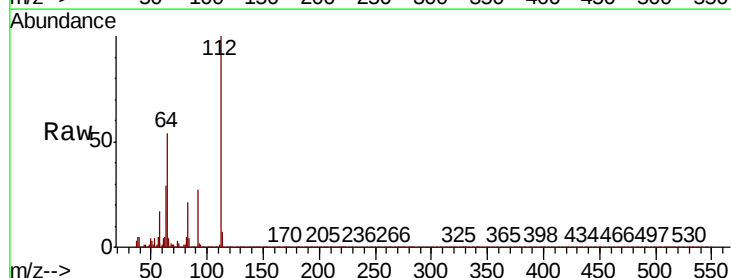


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BP0

Ion 63.00 (62.70 to 63.70): BP0

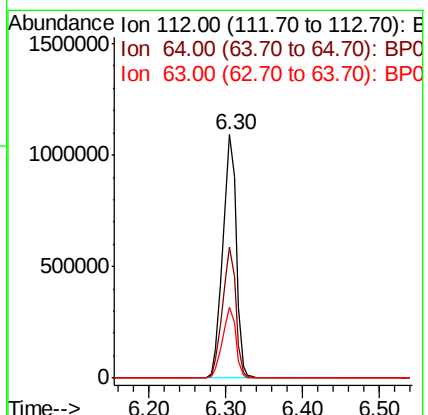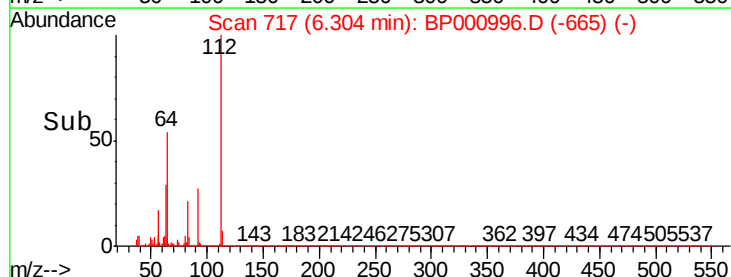

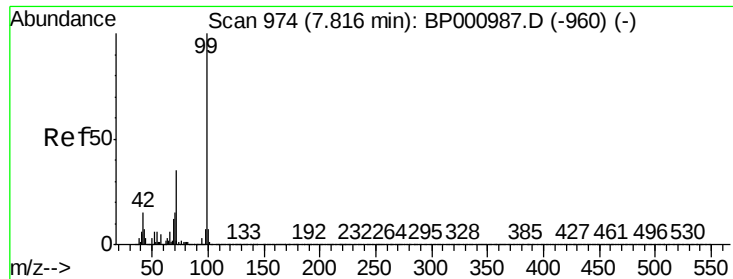

#7

Phenol-d6

Concen: 61.046 ng

RT: 7.81 min Scan# 973

Delta R.T. -0.01 min

Lab File: BP000996.D

Acq: 07 Nov 2019 10:38

Instrument :

BNA_P

ClientSampled :


Tot Ion: 99 Resp: 1147491

Ion Ratio Lower Upper

99 100

42 15.0 11.6 17.4




71 36.2 28.0 42.0

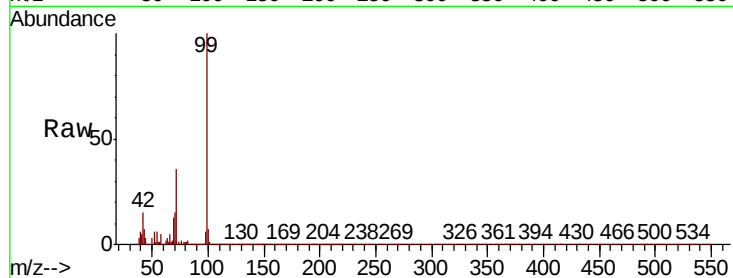

Abundance Ion 99.00 (98.70 to 99.70): BP0

Ion 42.00 (41.70 to 42.70): BP0

Ion 71.00 (70.70 to 71.70): BP0

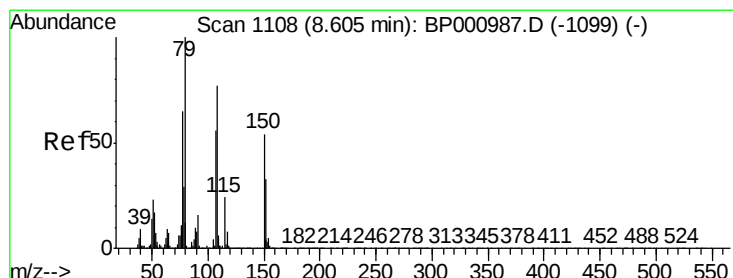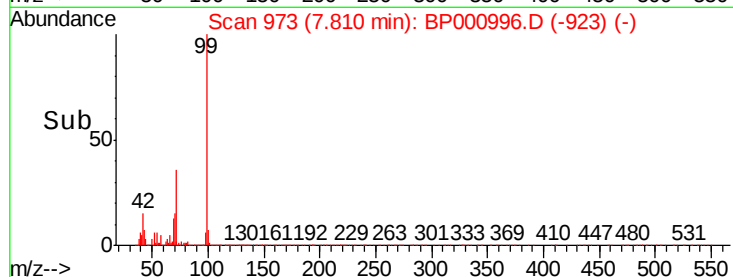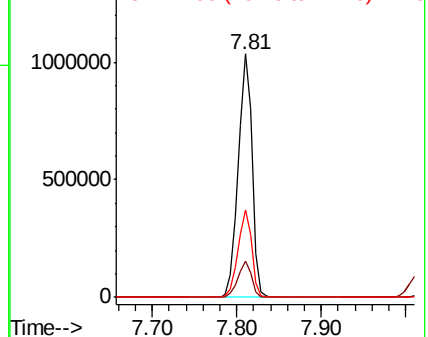

#15

Benzyl Alcohol

Concen: 2.131 ng

RT: 8.62 min Scan# 1110

Delta R.T. 0.01 min

Lab File: BP000996.D

Acq: 07 Nov 2019 10:38


Tgt Ion: 79 Resp: 30526

Ion Ratio Lower Upper

79 100

108 38.8 62.0 93.0#



77 105.7 51.9 77.9#

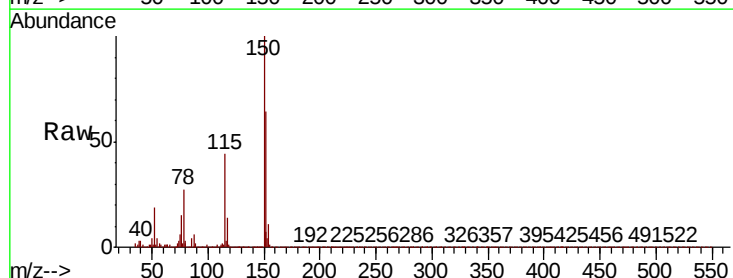


Abundance Ion 79.00 (78.70 to 79.70): BP0

Ion 108.00 (107.70 to 108.70): E

Ion 77.00 (76.70 to 77.70): BP0



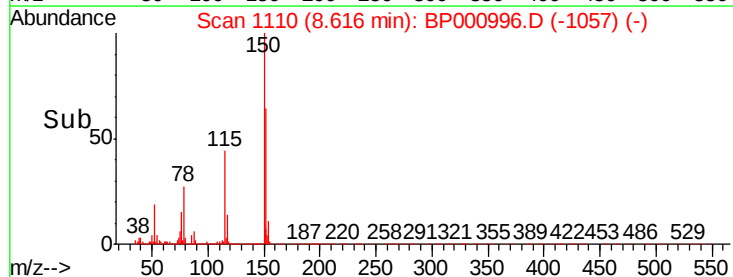
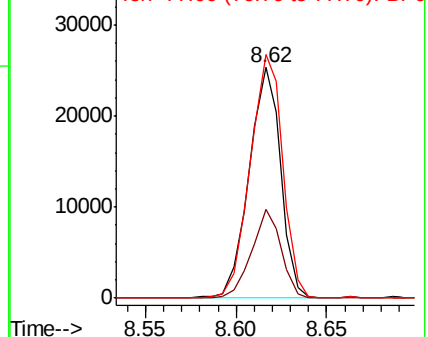


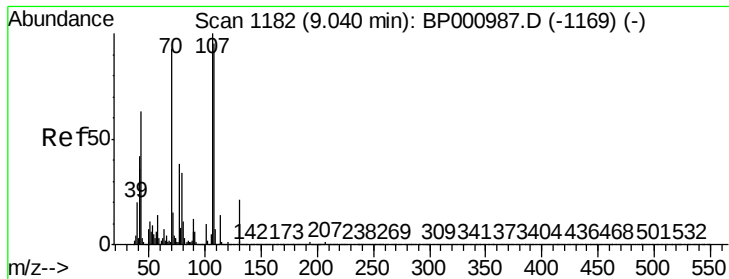

#19
n-Nitroso-di-n-propylamine
Concen: 20.147 ng
RT: 9.25 min Scan# 1218
Delta R.T. 0.21 min
Lab File: BP000996.D
Acq: 07 Nov 2019 10:38




Instrument :
BNA_P
ClientSampled :


Tot Ion: 70 Resp: 227396
Ion Ratio Lower Upper
70 100
42 39.1 36.3 54.5
101 0.0 8.7 13.1#
130 2.0 18.0 27.0#

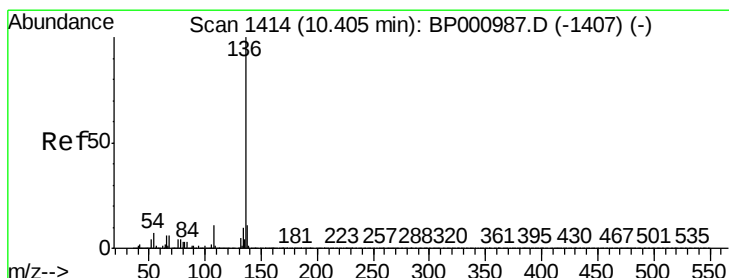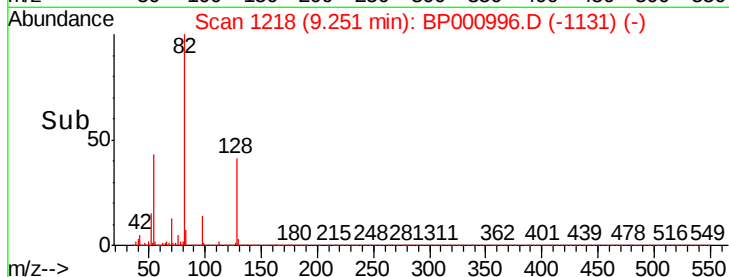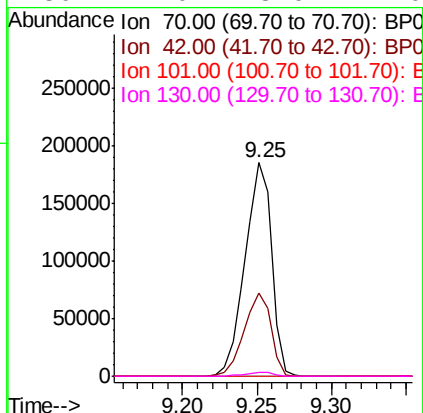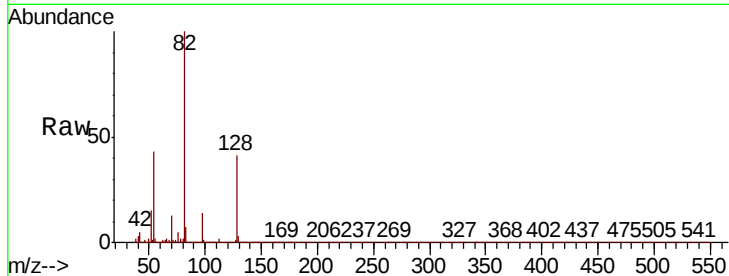

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.40 min Scan# 1414
Delta R.T. -0.00 min
Lab File: BP000996.D
Acq: 07 Nov 2019 10:38

Tgt Ion: 136 Resp: 997857
Ion Ratio Lower Upper
136 100
137 10.8 9.0 13.6
54 6.6 5.4 8.2
68 5.7 4.7 7.1


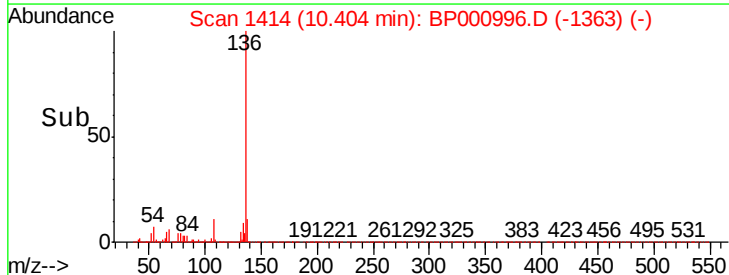
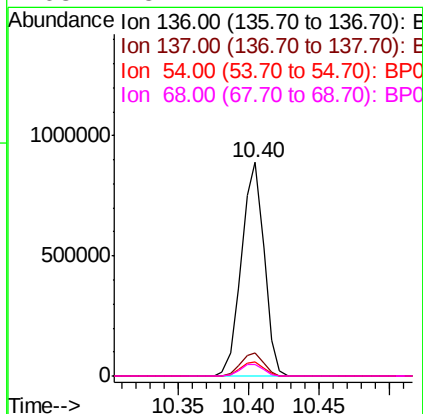
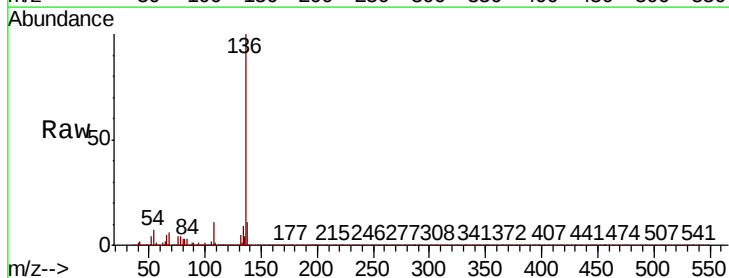


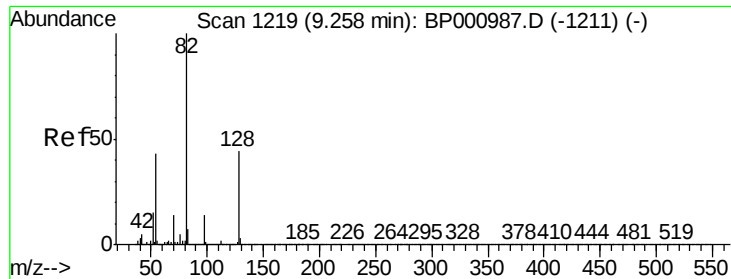

#23
Nitrobenzene-d5
Concen: 95.506 ng
RT: 9.25 min Scan# 1218
Delta R.T. -0.01 min
Lab File: BP000996.D
Acq: 07 Nov 2019 10:38




Instrument :
BNA_P
ClientSampleId :


Tot Ion: 82 Resp: 1722830
Ion Ratio Lower Upper
82 100
128 41.4 35.3 52.9
54 43.1 34.3 51.5

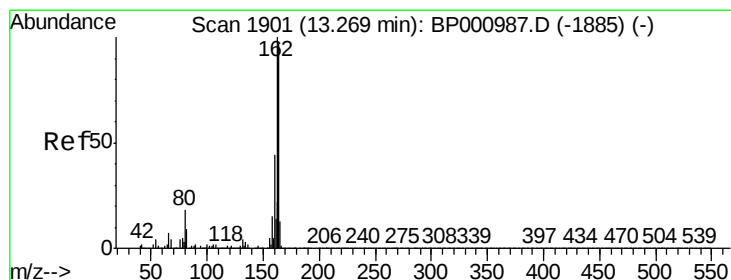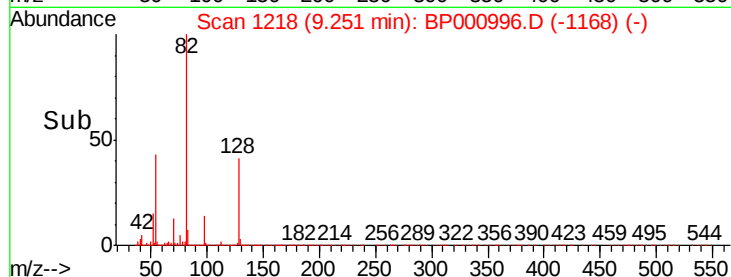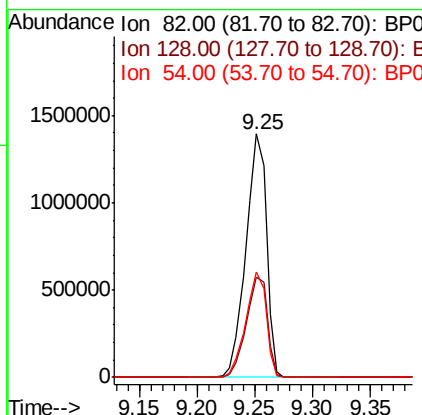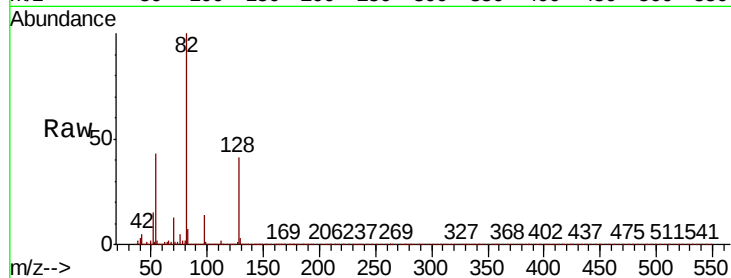

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 13.26 min Scan# 1900
Delta R.T. -0.01 min
Lab File: BP000996.D
Acq: 07 Nov 2019 10:38

Tgt Ion:164 Resp: 580829
Ion Ratio Lower Upper
164 100
162 100.9 82.6 123.8
160 45.0 36.5 54.7

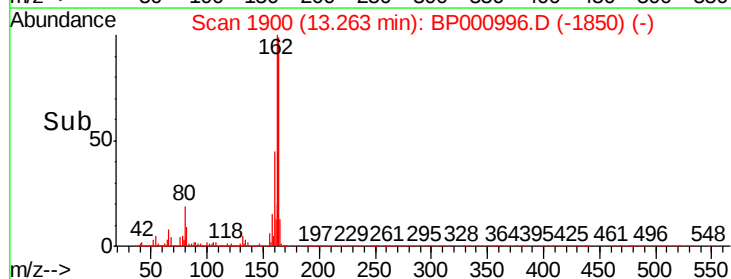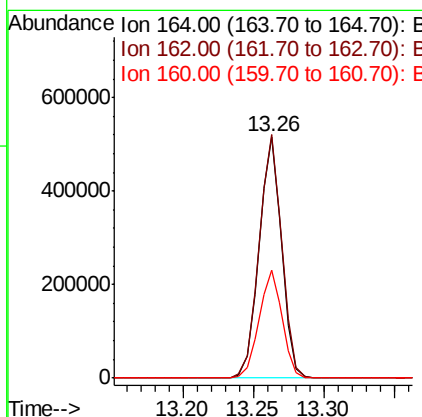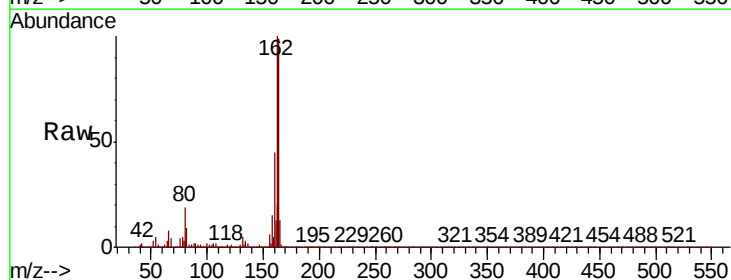


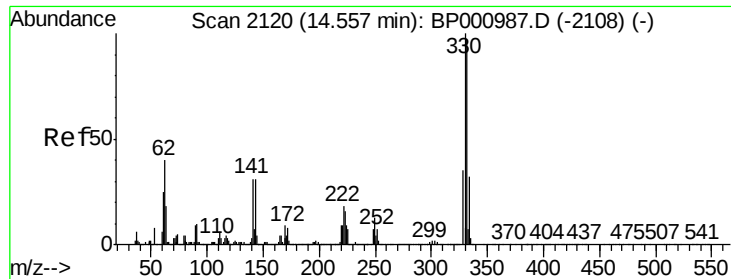




#42
2,4,6-Tribromophenol
Concen: 149.742 ng
RT: 14.56 min Scan# 2120
Delta R.T. -0.00 min
Lab File: BP000996.D
Acq: 07 Nov 2019 10:38

Instrument :
BNA_P
ClientSampleId :

Tot Ion:330 Resp: 1038280
Ion Ratio Lower Upper
330 100
332 97.3 78.3 117.5
141 32.2 25.0 37.4

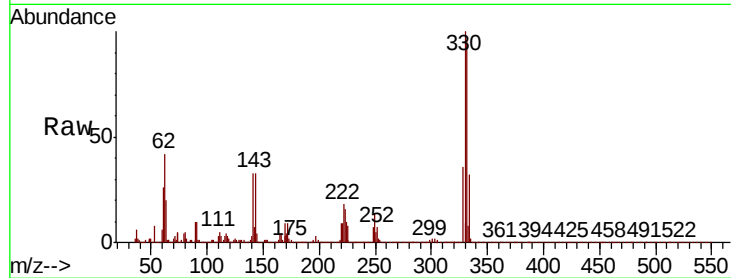


Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

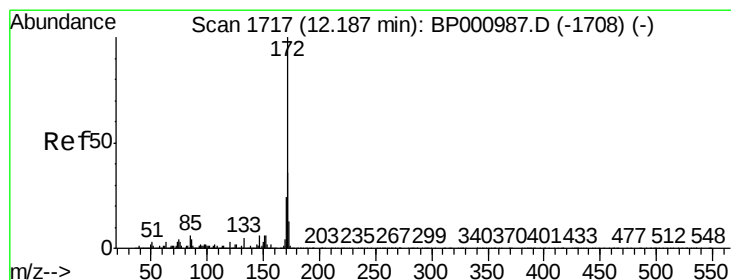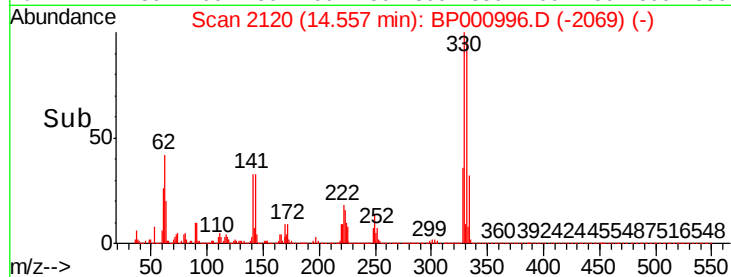
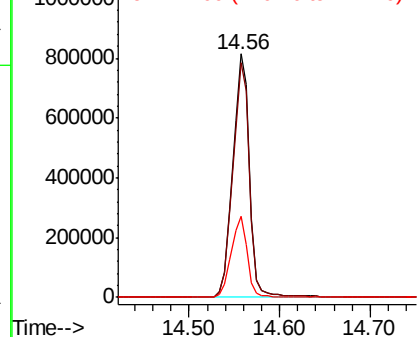



#45
2-Fluorobiphenyl
Concen: 93.918 ng
RT: 12.18 min Scan# 1716
Delta R.T. -0.01 min
Lab File: BP000996.D
Acq: 07 Nov 2019 10:38

Tgt Ion:172 Resp: 3621984
Ion Ratio Lower Upper
172 100
171 36.1 28.5 42.7
170 24.0 18.9 28.3

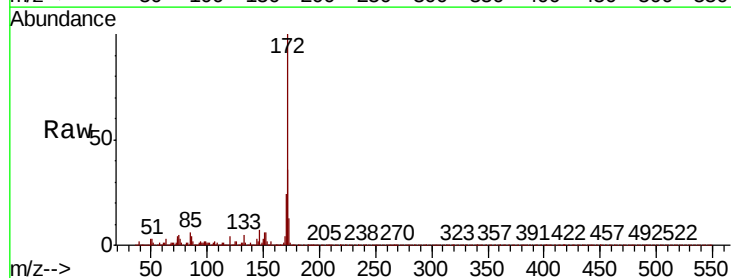

Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

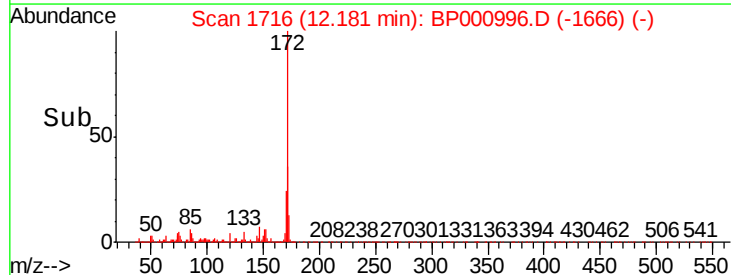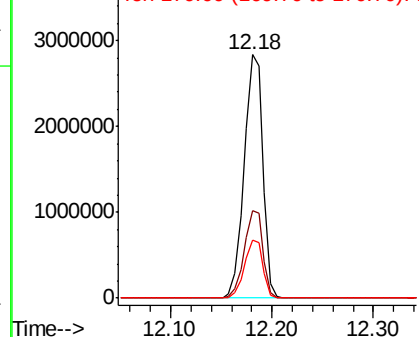

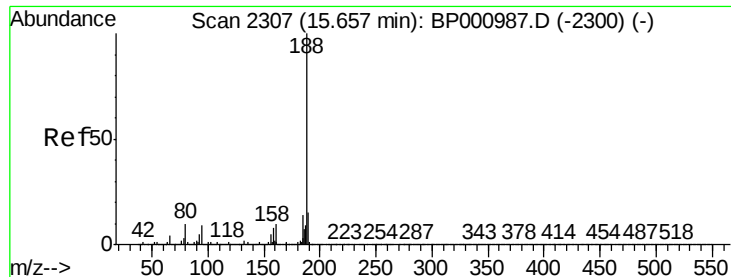

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 15.66 min Scan# 2307

Delta R.T. -0.00 min

Lab File: BP000996.D

Acq: 07 Nov 2019 10:38

Instrument :

BNA_P

ClientSampled :


Tot Ion:188 Resp: 1222874

Ion Ratio Lower Upper

188 100

94 8.4 7.4 11.2




80 8.9 7.9 11.9

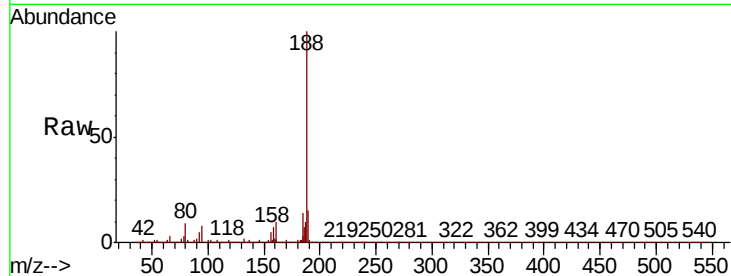

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BP0

Ion 80.00 (79.70 to 80.70): BP0

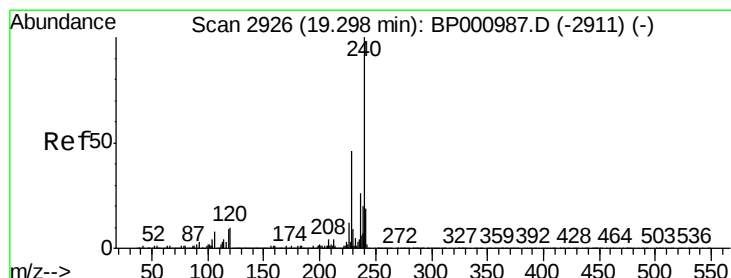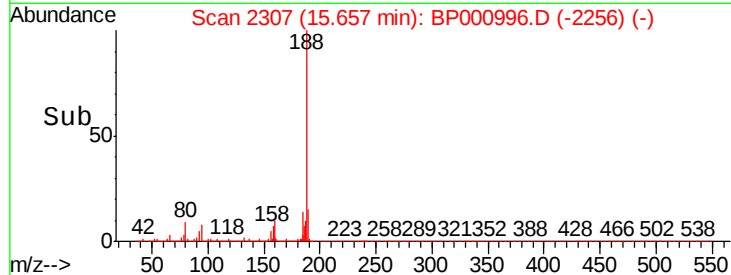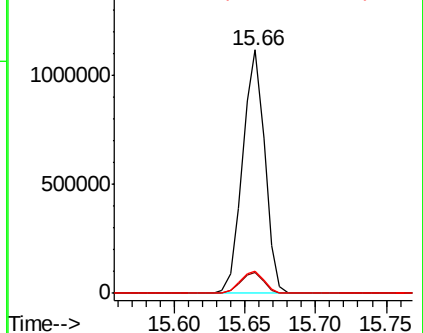

#76

Chrysene-d12

Concen: 20.000 ng

RT: 19.29 min Scan# 2925

Delta R.T. -0.01 min

Lab File: BP000996.D

Acq: 07 Nov 2019 10:38


Tgt Ion:240 Resp: 1081923

Ion Ratio Lower Upper

240 100

120 9.9 8.2 12.2



236 26.7 20.5 30.7

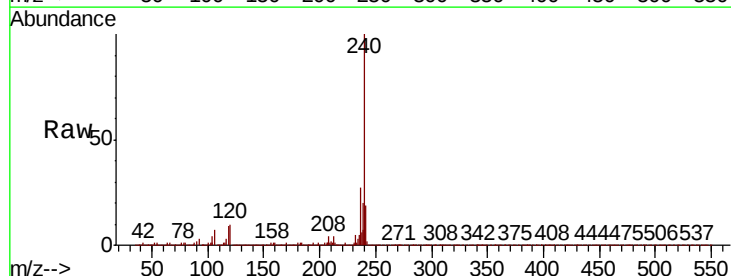


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

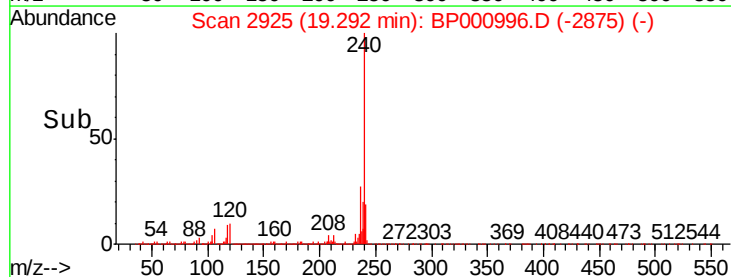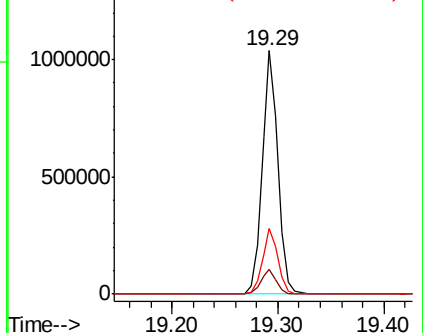

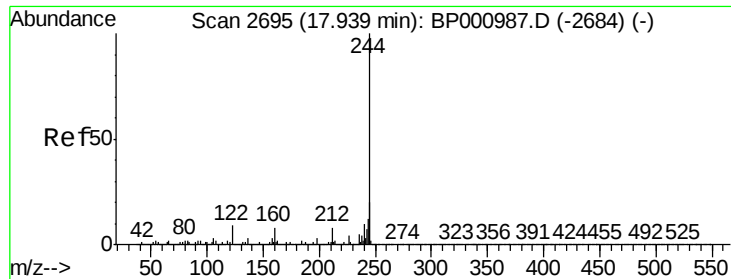

#79

Terphenyl-d14

Concen: 94.448 ng

RT: 17.94 min Scan# 2695

Delta R.T. -0.00 min

Lab File: BP000996.D

Acq: 07 Nov 2019 10:38

Instrument :

BNA_P

ClientSampleId :


Tot Ion:244 Resp: 5137130

Ion Ratio Lower Upper

244 100

212 8.2 6.0 9.0




122 9.6 7.4 11.2

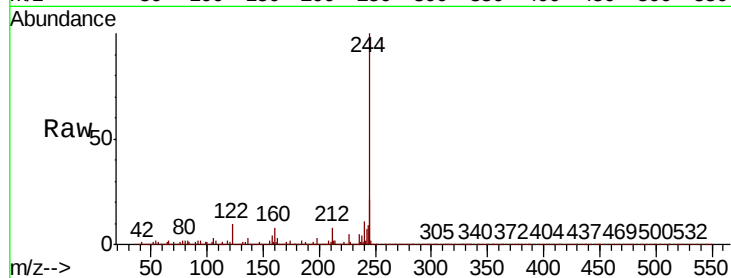

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

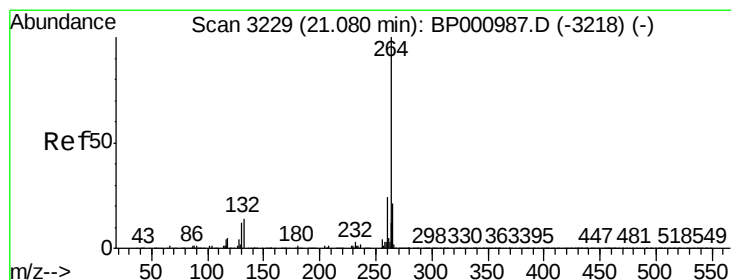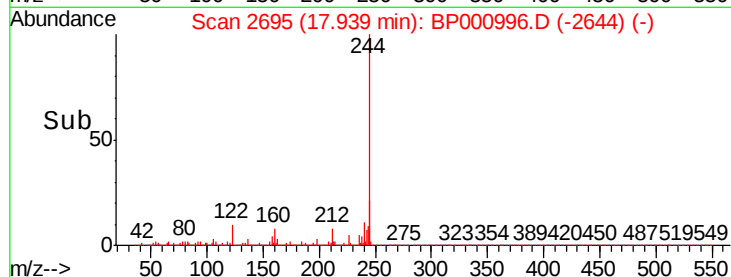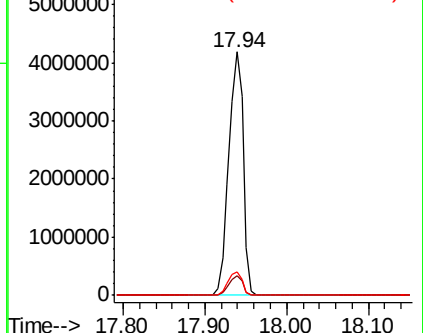

#87

Perylene-d12

Concen: 20.000 ng

RT: 21.08 min Scan# 3229

Delta R.T. -0.00 min

Lab File: BP000996.D

Acq: 07 Nov 2019 10:38


Tgt Ion:264 Resp: 1211618

Ion Ratio Lower Upper

264 100

260 23.5 18.8 28.2

265 21.4 17.1 25.7

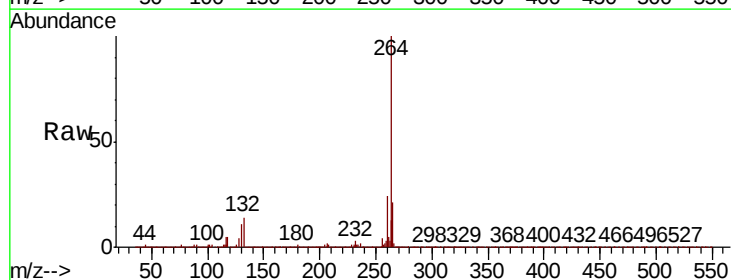

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

