
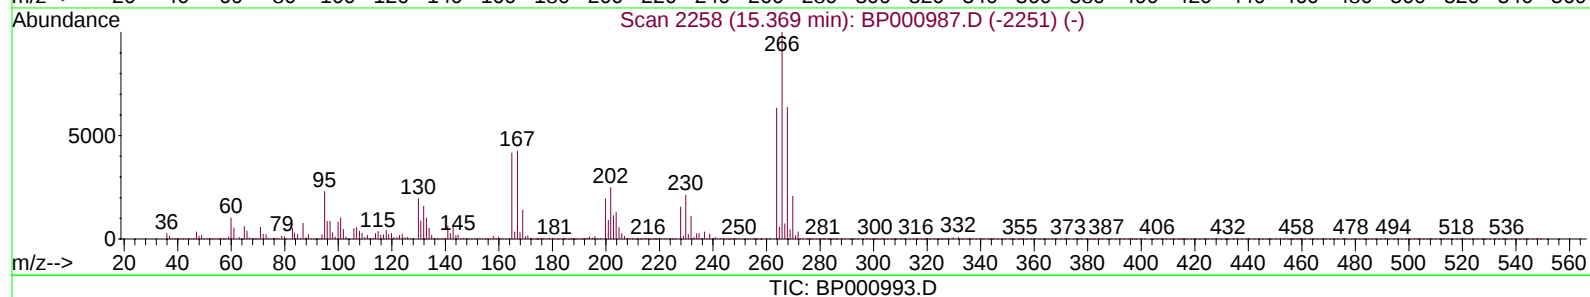
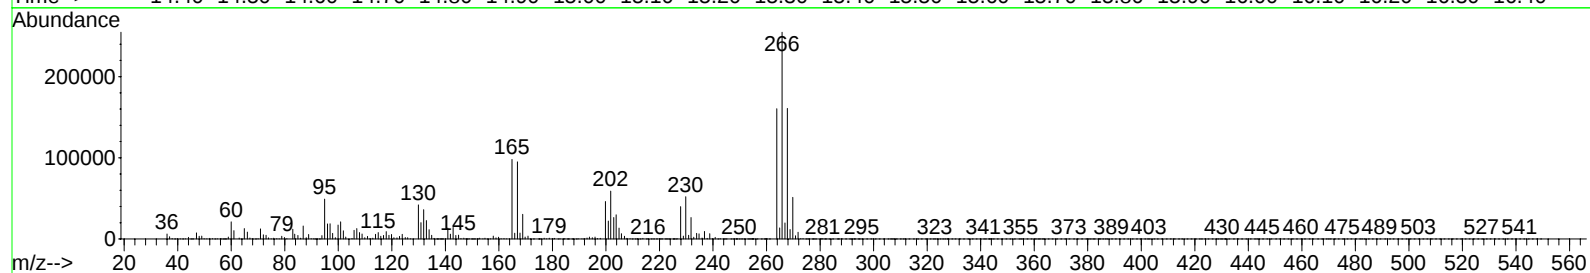


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP110719\
Data File : BP000993.D
Acq On : 07 Nov 2019 09:07
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 07 18:23:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP110619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 06 17:07:13 2019
Response via : Initial Calibration

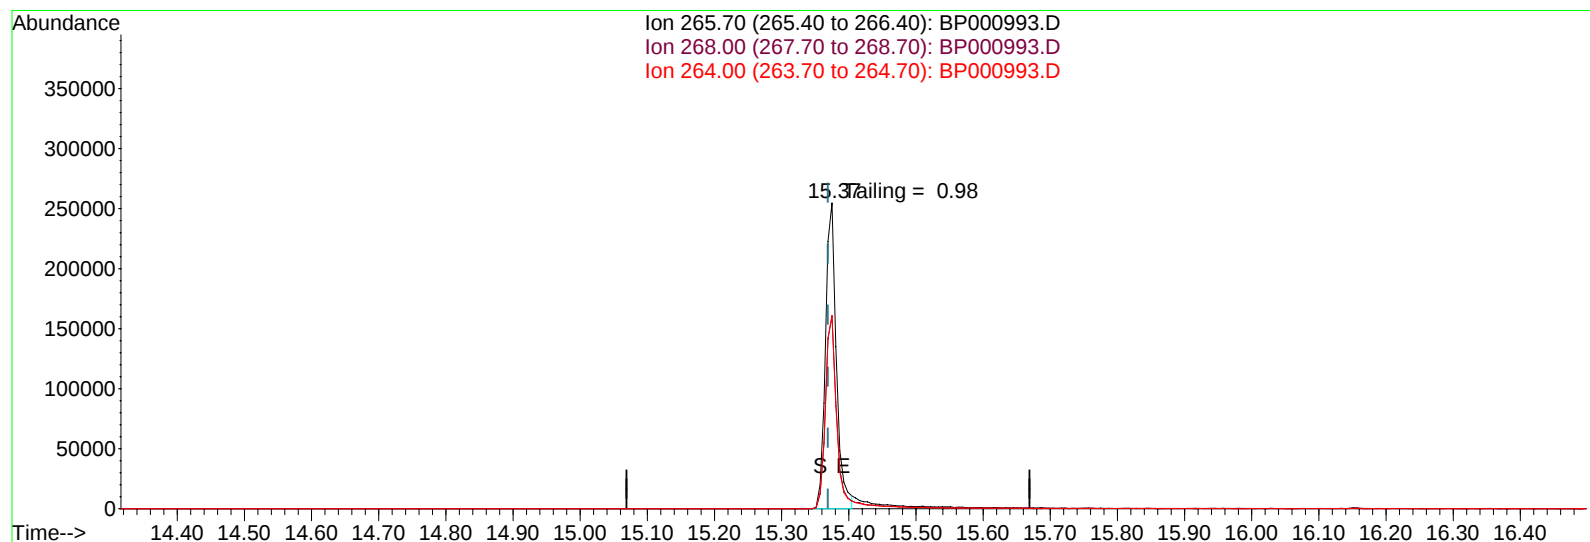

(70) Pentachlorophenol (C)




15.375min (+0.006) 5109115.39ng

response 310256

Ion	Exp%	Act%
265.70	100	100
268.00	63.60	63.17
264.00	63.30	63.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP110719\
Data File : BP000993.D
Acq On : 07 Nov 2019 09:07
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 07 18:23:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP110619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 06 17:07:13 2019
Response via : Initial Calibration

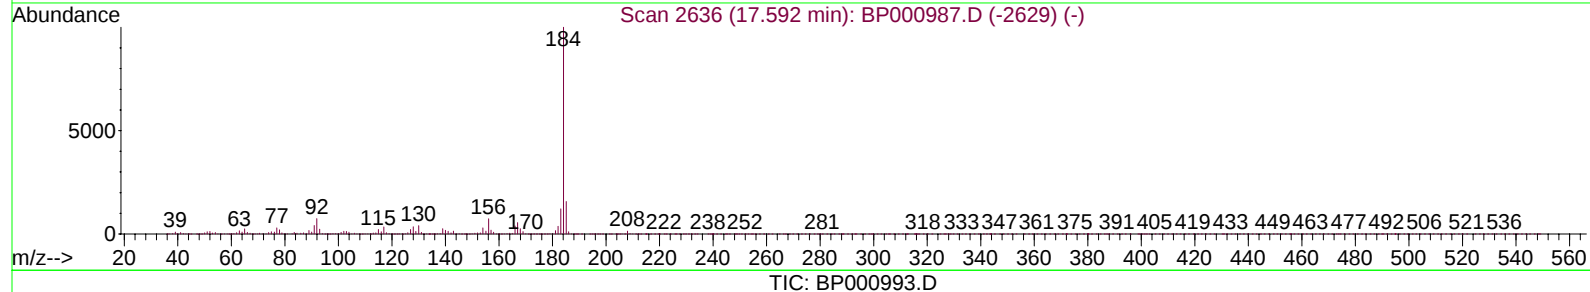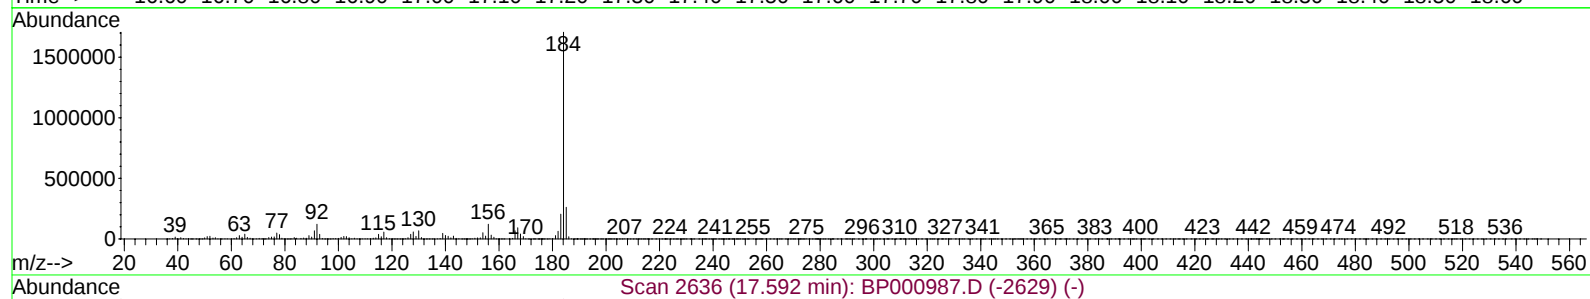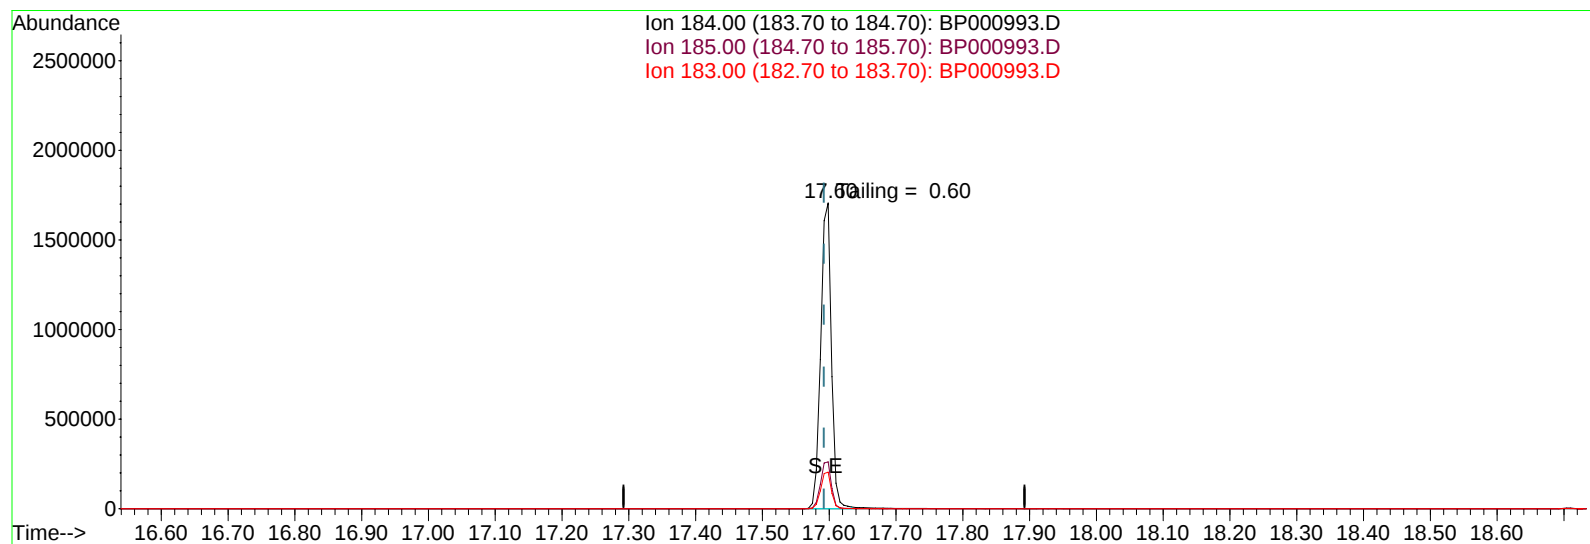

(77) Benzidine

17.598min (+0.006) 2882474.31ng

response 1910696

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.31
183.00	12.20	11.97
0.00	0.00	0.00