


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP110719\
 Data File : BP000993.D
 Acq On : 07 Nov 2019 09:07
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 06 17:07:13 2019

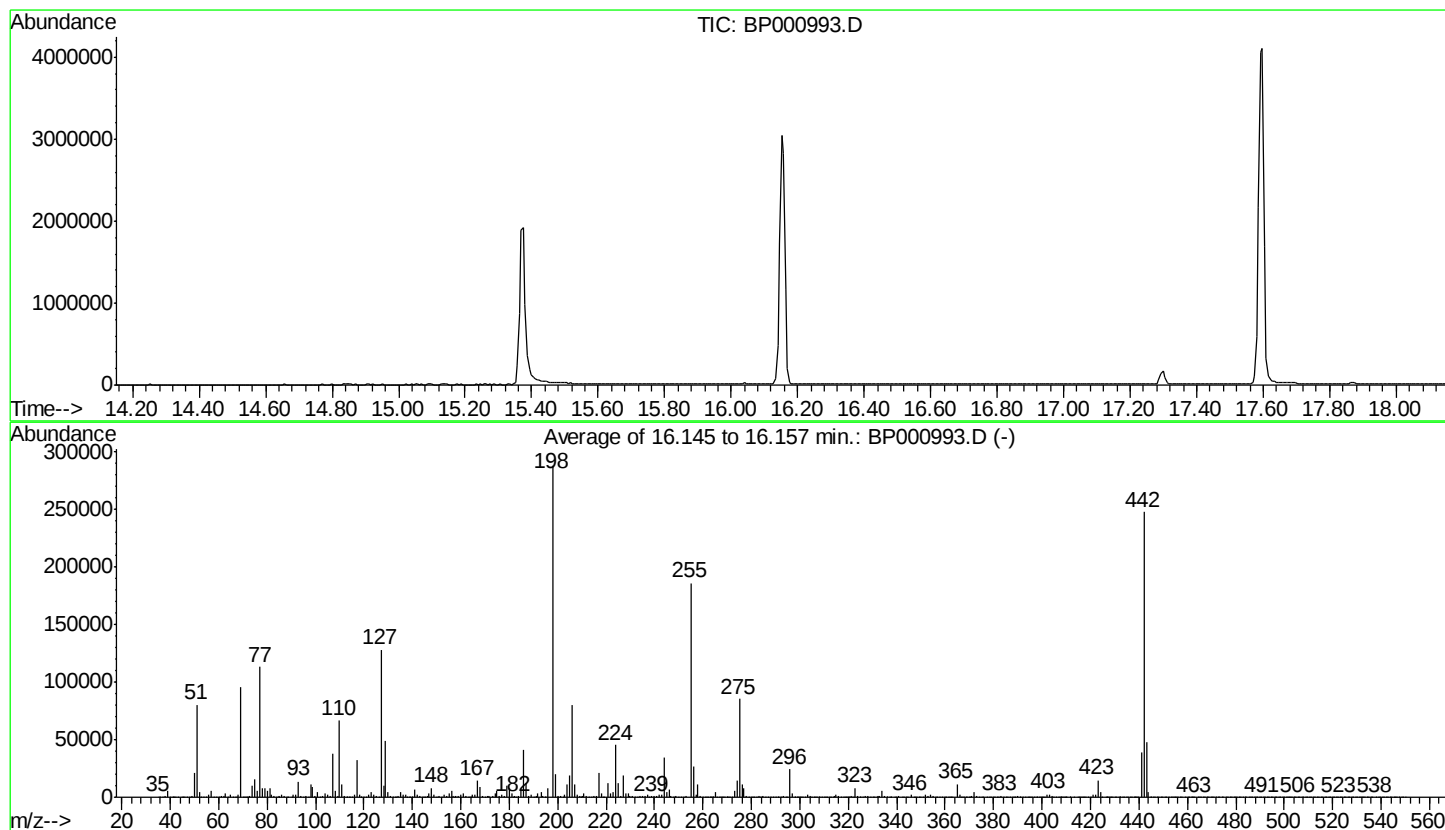

AutoFind: Scans 2390, 2391, 2392; Background Corrected with Scan 2383

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.8	80098	PASS
68	69	0.00	2	1.9	1789	PASS
69	198	0.00	100	33.1	95286	PASS
70	69	0.00	2	0.6	574	PASS
127	198	10	80	44.5	128200	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	287914	PASS
199	198	5	9	7.1	20368	PASS
275	198	10	60	29.7	85530	PASS
365	198	1	100	4.0	11407	PASS
441	198	0.01	100	13.6	39208	PASS
442	198	50	100	86.0	247566	PASS
443	442	15	24	19.2	47576	PASS