




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017930.D
Acq On : 07 Nov 2023 18:17
Operator : MA/JU
Sample : 05026-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH328

Manual IntegrationsAPPROVED

Quant Time: Nov 07 21:49:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 07 03:40:56 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/09/2023
Supervised By :mohammad ahmed 11/11/2023

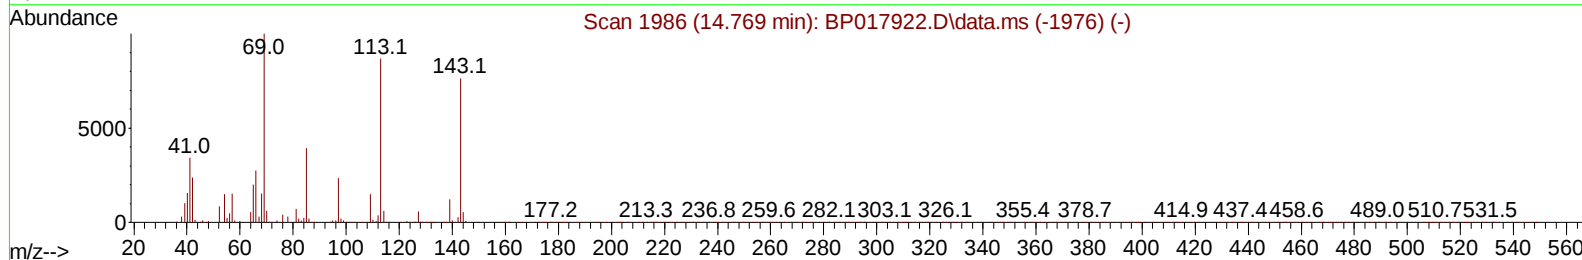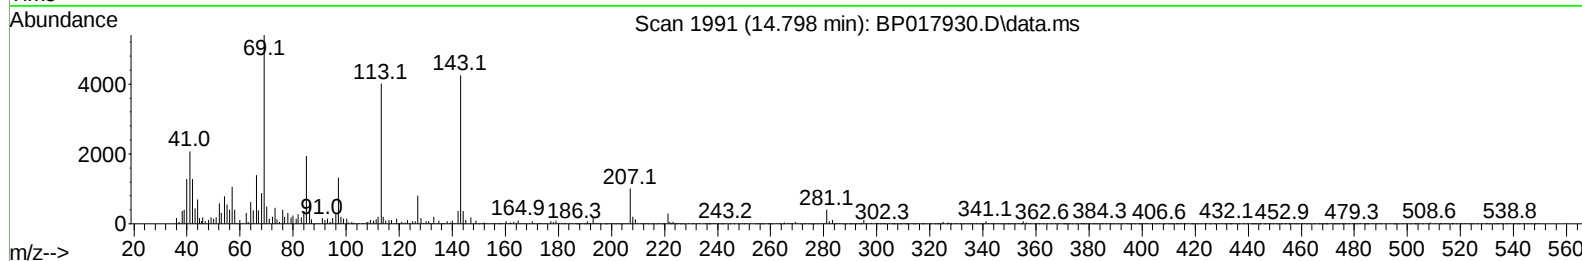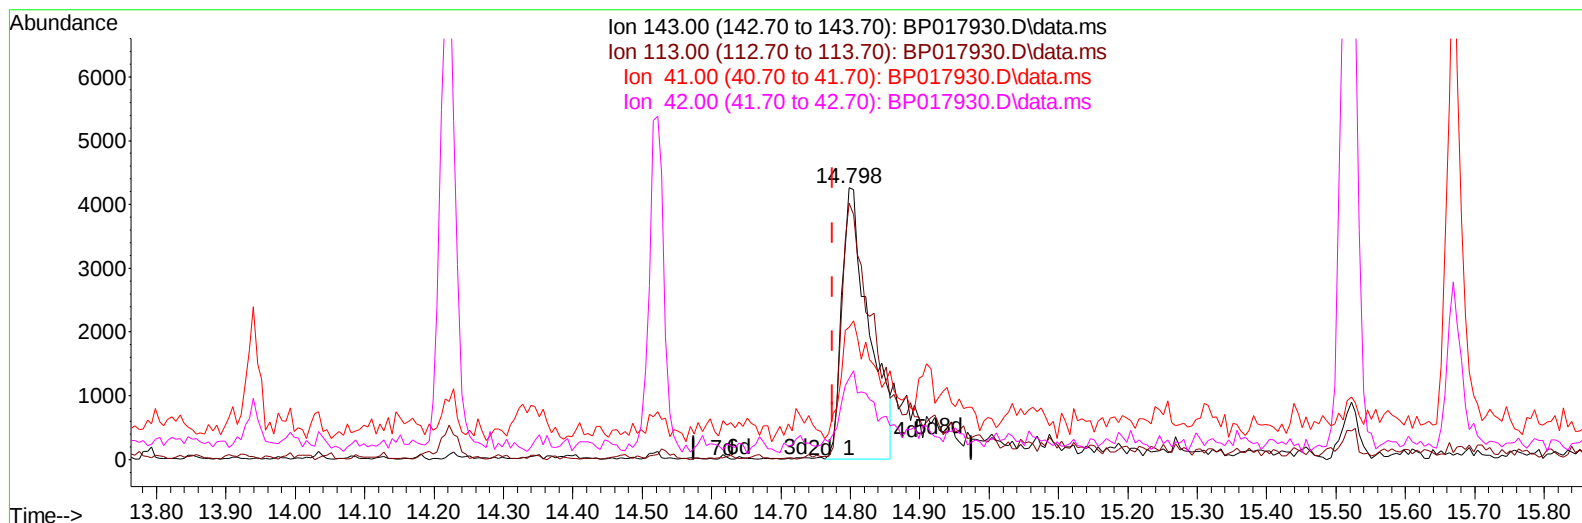

TIC: BP017930.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.798min (+ 0.024) 4.58 ng/u1

response 11488

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	100.40	94.34
41.00	43.00	48.79
42.00	28.20	29.91




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
 Data File : BP017930.D
 Acq On : 07 Nov 2023 18:17
 Operator : MA/JU
 Sample : 05026-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH328

Manual IntegrationsAPPROVED

Quant Time: Nov 07 21:49:40 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 07 03:40:56 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/09/2023
 Supervised By :mohammad ahmed 11/11/2023

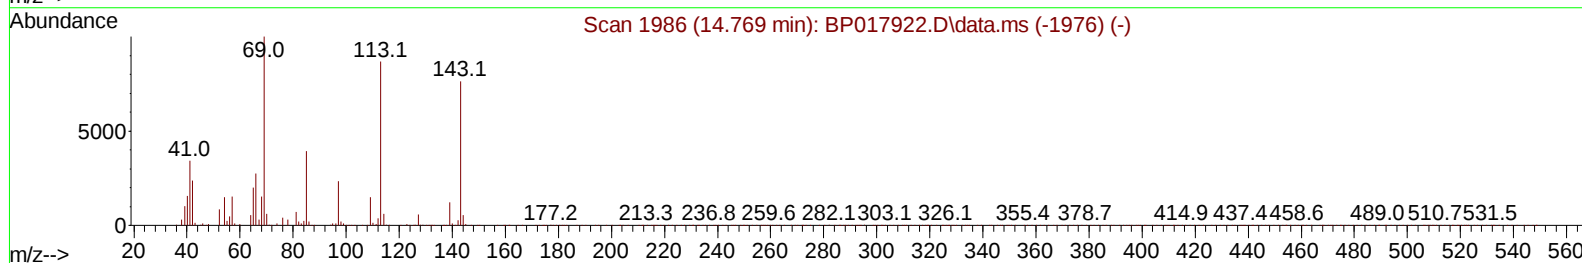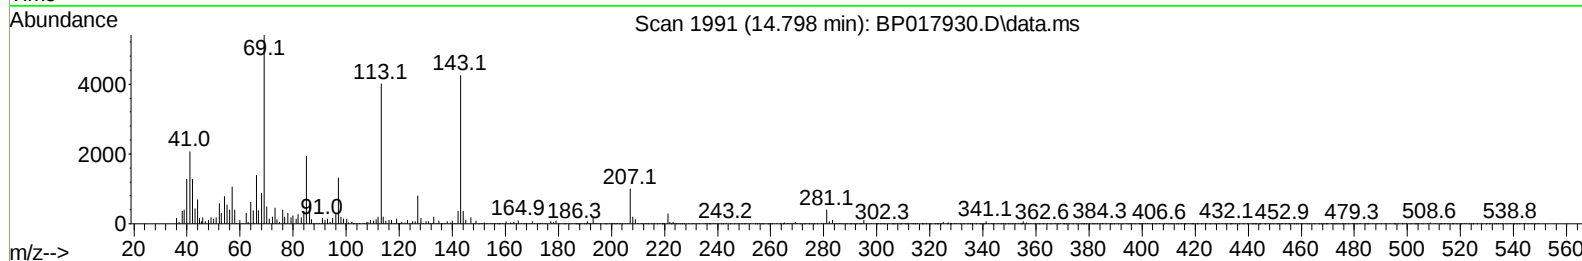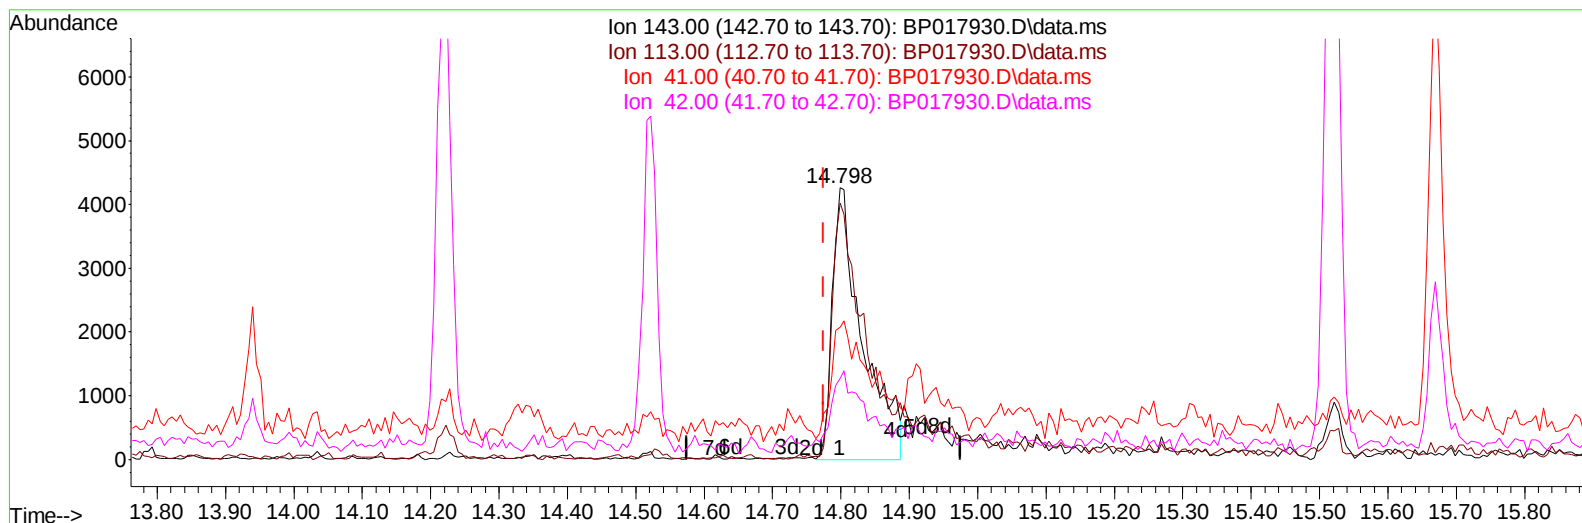

TIC: BP017930.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.798min (+ 0.024) 5.23 ng/ul m

response 13098

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	100.40	94.34
41.00	43.00	48.79
42.00	28.20	29.91

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
 Data File : BP017930.D
 Acq On : 07 Nov 2023 18:17
 Operator : MA/JU
 Sample : 05026-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH328

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/09/2023
 Supervised By :mohammad ahmed 11/11/2023

Quant Time: Nov 07 22:19:11 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 07 03:40:56 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.857	152	67383	20.000	ng/ul	0.00
20) Naphthalene-d8	10.675	136	276940	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.522	164	185866	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.292	188	411785	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.410	240	383966	20.000	ng/ul	0.00
88) Perylene-d12	23.892	264	410798	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.246	96	7768	4.412	ng/uL	0.00
4) Pyridine-d5	3.681	84	61412	12.569	ng/ul	0.00
7) Phenol-d5	7.040	99	54374	8.605	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.210	67	131254	34.434	ng/ul	0.00
11) 2-Chlorophenol-d4	7.387	132	152413	31.390	ng/ul	0.00
15) 4-Methylphenol-d8	8.593	113	104208	19.953	ng/ul	0.01
21) Nitrobenzene-d5	9.063	128	109467	49.462	ng/ul	0.00
24) 2-Nitrophenol-d4	9.775	143	101194	39.698	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.316	165	167356	35.813	ng/ul	0.02
31) 4-Chloroaniline-d4	10.851	131	215661	31.847	ng/ul	0.00
46) Dimethylphthalate-d6	13.940	166	630156	38.665	ng/ul	0.00
49) Acenaphthylene-d8	14.222	160	664001	37.130	ng/ul	0.00
54) 4-Nitrophenol-d4	14.798	143	13098m	5.227	ng/ul	0.02
60) Fluorene-d10	15.522	176	523847	38.402	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.669	200	101830	33.815	ng/ul	0.00
73) Anthracene-d10	17.392	188	861067	40.217	ng/ul	0.00
81) Pyrene-d10	19.645	212	1039976	42.667	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.727	264	967550	42.153	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017930.D
Acq On : 07 Nov 2023 18:17
Operator : MA/JU
Sample : 05026-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH328

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/09/2023
Supervised By :mohammad ahmed 11/11/2023

Quant Time: Nov 07 22:19:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 07 03:40:56 2023
Response via : Initial Calibration

