




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
 Data File : BP017934.D
 Acq On : 07 Nov 2023 20:33
 Operator : MA/JU
 Sample : 05026-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH333

Manual IntegrationsAPPROVED

Quant Time: Nov 07 22:44:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 07 03:40:56 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/09/2023
 Supervised By :mohammad ahmed 11/11/2023

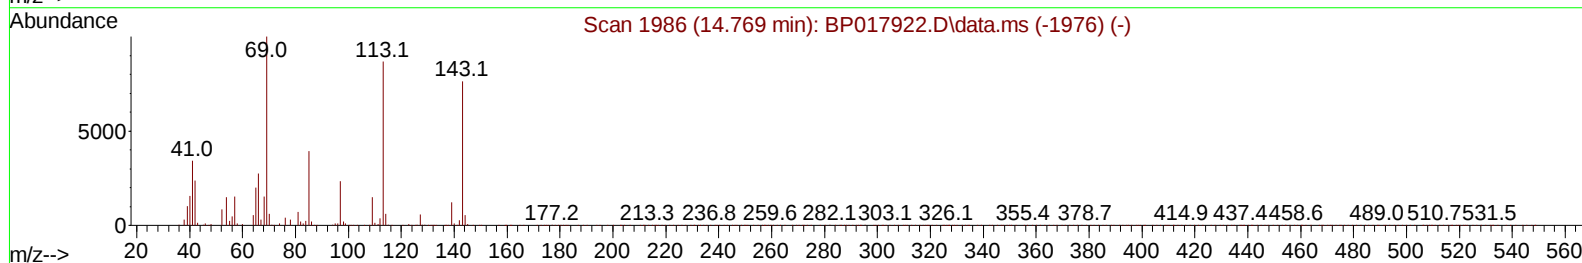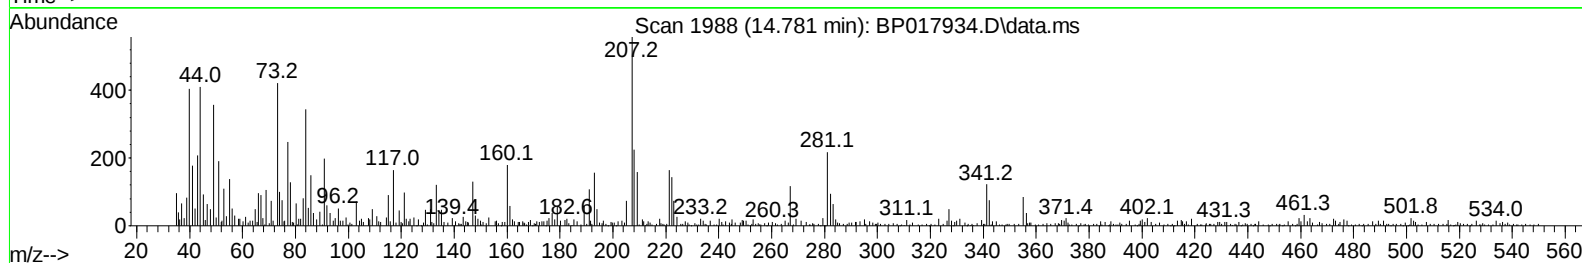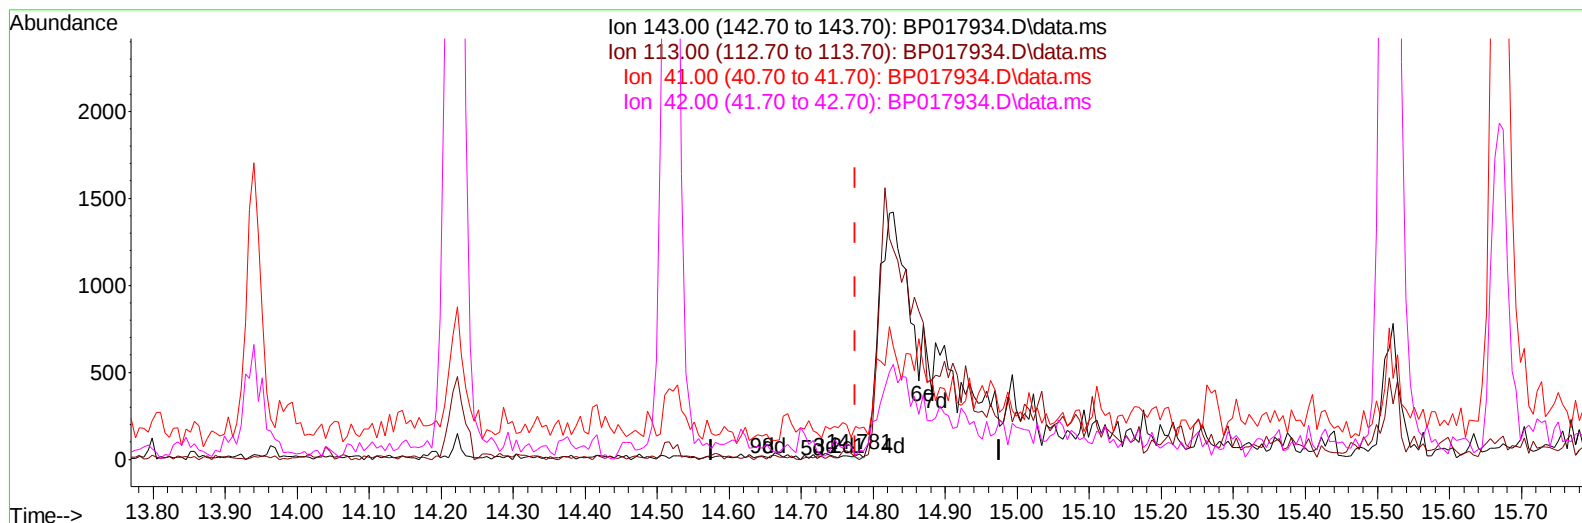

TIC: BP017934.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.781min (+ 0.006) 0.00 ng/u1

response 11

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	100.40	0.00#
41.00	43.00	574.19#
42.00	28.20	164.52#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
 Data File : BP017934.D
 Acq On : 07 Nov 2023 20:33
 Operator : MA/JU
 Sample : 05026-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH333

Manual IntegrationsAPPROVED

Quant Time: Nov 07 22:44:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 07 03:40:56 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/09/2023
 Supervised By :mohammad ahmed 11/11/2023

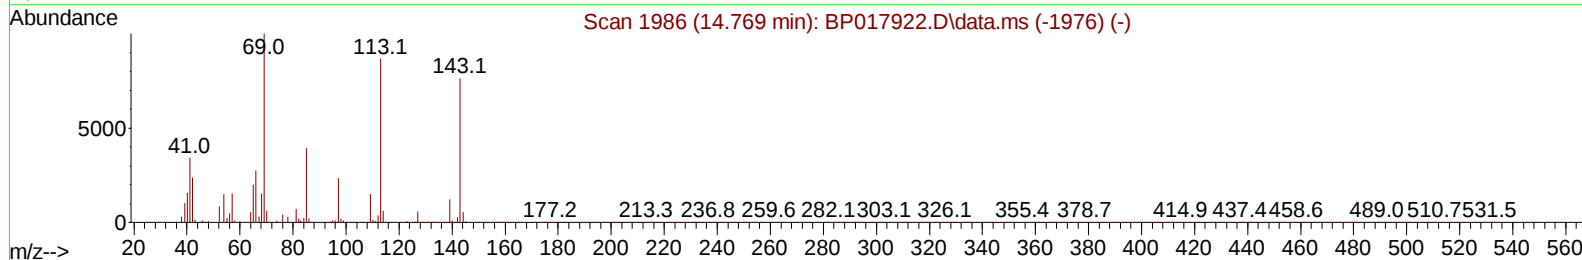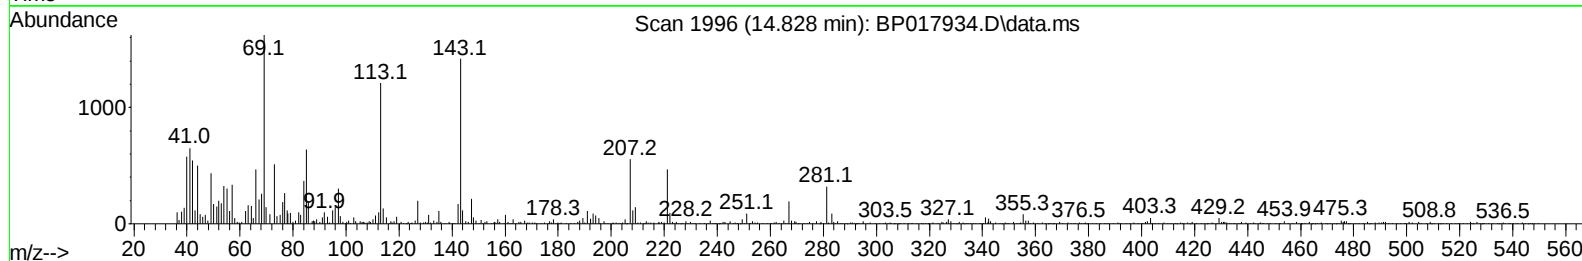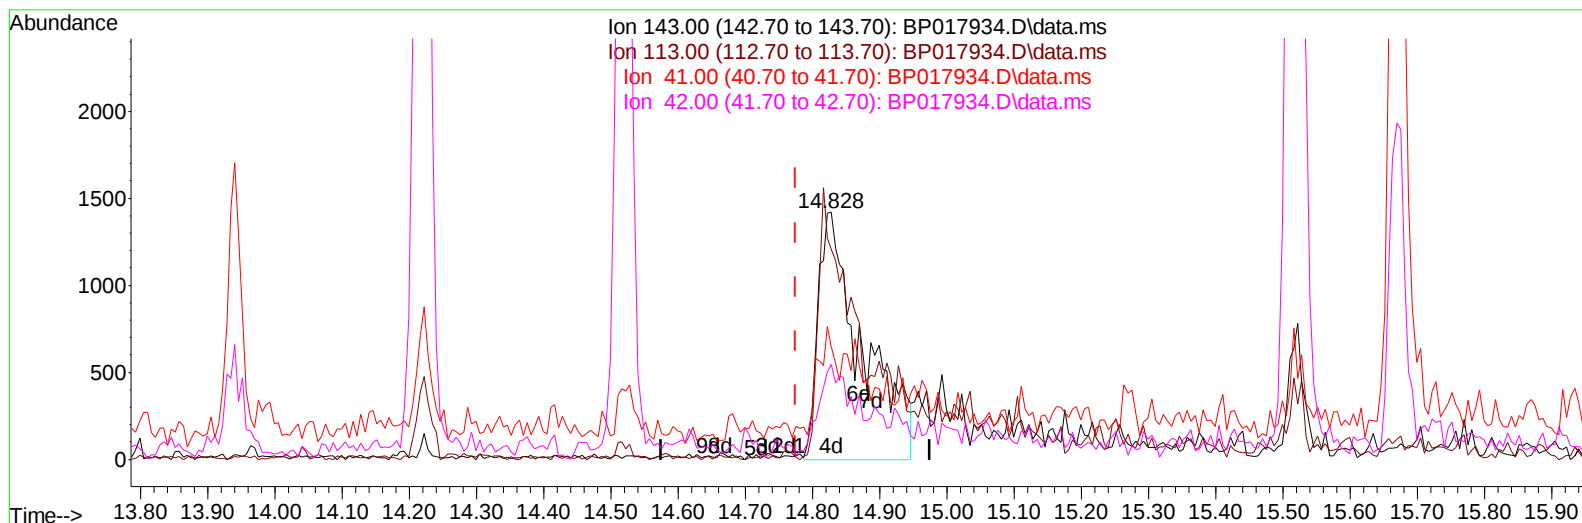

TIC: BP017934.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.828min (+ 0.053) 2.71 ng/ul m

response 6517

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	100.40	85.15
41.00	43.00	45.81
42.00	28.20	38.35#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
 Data File : BP017934.D
 Acq On : 07 Nov 2023 20:33
 Operator : MA/JU
 Sample : 05026-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH333

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/09/2023
 Supervised By :mohammad ahmed 11/11/2023

Quant Time: Nov 07 22:44:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 07 03:40:56 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.858	152	70177	20.000	ng/ul	0.00
20) Naphthalene-d8	10.675	136	284856	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.522	164	178336	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.292	188	392639	20.000	ng/ul	0.00
79) Chrysene-d12	21.410	240	371792	20.000	ng/ul	0.00
88) Perylene-d12	23.892	264	417353	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.240	96	6844	3.733	ng/uL	0.00
4) Pyridine-d5	3.681	84	40319	7.923	ng/ul	0.00
7) Phenol-d5	7.028	99	33706	5.122	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.205	67	134324	33.837	ng/ul	0.00
11) 2-Chlorophenol-d4	7.381	132	122254	24.176	ng/ul	0.00
15) 4-Methylphenol-d8	8.581	113	71065	13.065	ng/ul	0.00
21) Nitrobenzene-d5	9.058	128	85900	37.735	ng/ul	0.00
24) 2-Nitrophenol-d4	9.775	143	91956	35.072	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.299	165	135872	28.267	ng/ul	0.00
31) 4-Chloroaniline-d4	10.852	131	176872	25.393	ng/ul	0.00
46) Dimethylphthalate-d6	13.940	166	580375	37.114	ng/ul	0.00
49) Acenaphthylene-d8	14.222	160	620158	36.142	ng/ul	0.00
54) 4-Nitrophenol-d4	14.828	143	6517m	2.711	ng/ul	0.05
60) Fluorene-d10	15.522	176	476107	36.376	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.669	200	83315	29.016	ng/ul	0.00
73) Anthracene-d10	17.392	188	832708	40.789	ng/ul	0.00
81) Pyrene-d10	19.645	212	988423	41.880	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.727	264	965491	41.402	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017934.D
Acq On : 07 Nov 2023 20:33
Operator : MA/JU
Sample : 05026-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH333

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/09/2023
Supervised By :mohammad ahmed 11/11/2023

Quant Time: Nov 07 22:44:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 07 03:40:56 2023
Response via : Initial Calibration

