

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
 Data File : BP017923.D
 Acq On : 07 Nov 2023 09:20
 Operator : MA/JU
 Sample : PB156841BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK841

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017923.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	23	27	35	rVB	21376	29446	1.84%	0.161%
2	3.517	69	73	77	rBV7	2121	3592	0.22%	0.020%
3	3.681	97	101	122	rBV	198046	342835	21.38%	1.875%
4	3.981	147	152	158	rBV3	8367	13547	0.84%	0.074%
5	4.440	227	230	231	rBV3	2181	2166	0.14%	0.012%
6	4.675	266	270	271	rBV4	1499	1705	0.11%	0.009%
7	5.146	348	350	355	rBV6	1801	3194	0.20%	0.017%
8	5.305	375	377	381	rBV5	1278	1853	0.12%	0.010%
9	5.387	386	391	393	rBV5	1346	2397	0.15%	0.013%
10	6.081	507	509	514	rVB6	1298	1735	0.11%	0.009%
11	6.258	536	539	542	rBV5	1272	2155	0.13%	0.012%
12	7.028	664	670	689	rBV	239039	448004	27.94%	2.451%
13	7.210	694	701	713	rBV	208255	327327	20.41%	1.791%
14	7.381	722	730	743	rBV	277483	467516	29.15%	2.558%
15	7.857	805	811	827	rBV	294115	477901	29.80%	2.614%
16	8.081	845	849	852	rBV6	993	1624	0.10%	0.009%
17	8.581	927	934	949	rBV	289267	541812	33.79%	2.964%
18	8.804	970	972	974	rBV3	1754	1845	0.12%	0.010%
19	9.063	1009	1016	1032	rVV	264042	457135	28.51%	2.501%
20	9.187	1036	1037	1041	rBV4	1696	1781	0.11%	0.010%
21	9.322	1056	1060	1066	rBV8	2213	4444	0.28%	0.024%
22	9.775	1129	1137	1150	rBV	229088	408571	25.48%	2.235%
23	10.304	1220	1227	1249	rBV	272913	559159	34.87%	3.059%
24	10.675	1282	1290	1302	rBV	393625	660270	41.17%	3.612%
25	10.851	1311	1320	1334	rBV	251234	535864	33.41%	2.931%
26	11.116	1363	1365	1369	rVB5	1727	1662	0.10%	0.009%
27	12.287	1560	1564	1571	rBV9	3066	6881	0.43%	0.038%
28	12.593	1611	1616	1621	rBV7	1064	1993	0.12%	0.011%
29	12.845	1654	1659	1661	rBV5	1622	1982	0.12%	0.011%
30	13.004	1683	1686	1692	rVB8	1754	3066	0.19%	0.017%
31	13.163	1709	1713	1716	rBV5	1528	2183	0.14%	0.012%
32	13.369	1742	1748	1752	rBV8	5763	10364	0.65%	0.057%
33	13.728	1806	1809	1815	rVV8	2072	2419	0.15%	0.013%
34	13.816	1819	1824	1826	rBV5	1142	1661	0.10%	0.009%
35	13.940	1838	1845	1861	rBV	632140	947230	59.07%	5.182%
36	14.145	1877	1880	1881	rBV3	1557	1748	0.11%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
 Data File : BP017923.D
 Acq On : 07 Nov 2023 09:20
 Operator : MA/JU
 Sample : PB156841BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK841

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
 Title : SVOA CALIBRATION

37	14.222	1886	1893	1911	rBV	696754	1019425	63.57%	5.577%
38	14.522	1936	1944	1957	rVV	625659	887649	55.35%	4.856%
39	14.634	1961	1963	1966	rVB4	1507	1793	0.11%	0.010%
40	14.781	1980	1988	2006	rBV	108935	313899	19.57%	1.717%
41	15.228	2061	2064	2066	rBV4	2023	2187	0.14%	0.012%
42	15.292	2072	2075	2077	rBV4	1646	1821	0.11%	0.010%
43	15.522	2107	2114	2128	rBV	892090	1268861	79.12%	6.941%
44	15.675	2134	2140	2152	rBV	258016	424999	26.50%	2.325%
45	15.757	2152	2154	2165	rVV10	7877	15522	0.97%	0.085%
46	15.869	2169	2173	2174	rVB4	1499	1775	0.11%	0.010%
47	16.322	2248	2250	2253	rVB4	1857	1903	0.12%	0.010%
48	16.369	2253	2258	2259	rBV4	1984	2458	0.15%	0.013%
49	16.739	2319	2321	2324	rVB4	2089	1892	0.12%	0.010%
50	17.086	2378	2380	2383	rVB4	1449	1621	0.10%	0.009%
51	17.292	2409	2415	2422	rBV	755079	1089400	67.93%	5.960%
52	17.398	2426	2433	2446	rVV	948971	1392974	86.86%	7.620%
53	18.157	2560	2562	2565	rBV4	1866	1821	0.11%	0.010%
54	18.463	2610	2614	2615	rBV4	1810	2663	0.17%	0.015%
55	18.539	2625	2627	2630	rBV4	1575	1733	0.11%	0.009%
56	19.216	2739	2742	2746	rVB4	10204	12981	0.81%	0.071%
57	19.292	2751	2755	2760	rVB3	9832	15309	0.95%	0.084%
58	19.645	2809	2815	2824	rBV	1223155	1603686	100.00%	8.773%
59	21.410	3110	3115	3126	rBV	835338	1173230	73.16%	6.418%
60	23.727	3502	3509	3521	rVB2	788405	1570881	97.95%	8.594%
61	23.892	3531	3537	3553	rVB	577934	1190234	74.22%	6.511%




Sum of corrected areas: 18279784

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017923.D
Acq On : 07 Nov 2023 09:20
Operator : MA/JU
Sample : PB156841BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK841

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

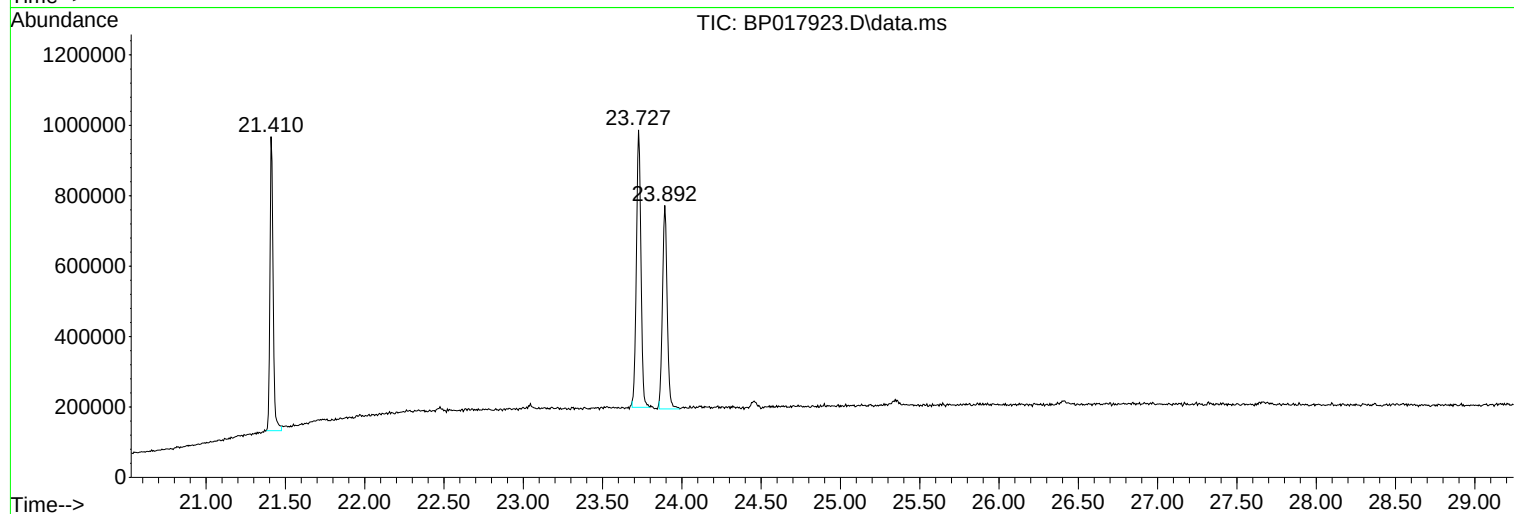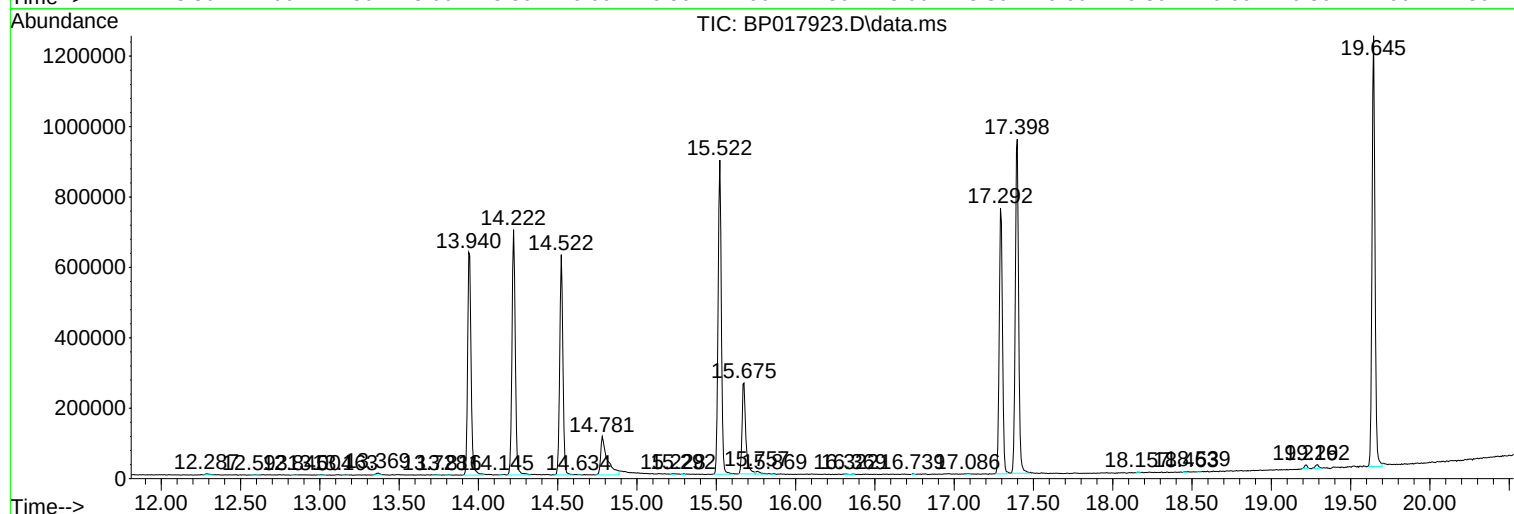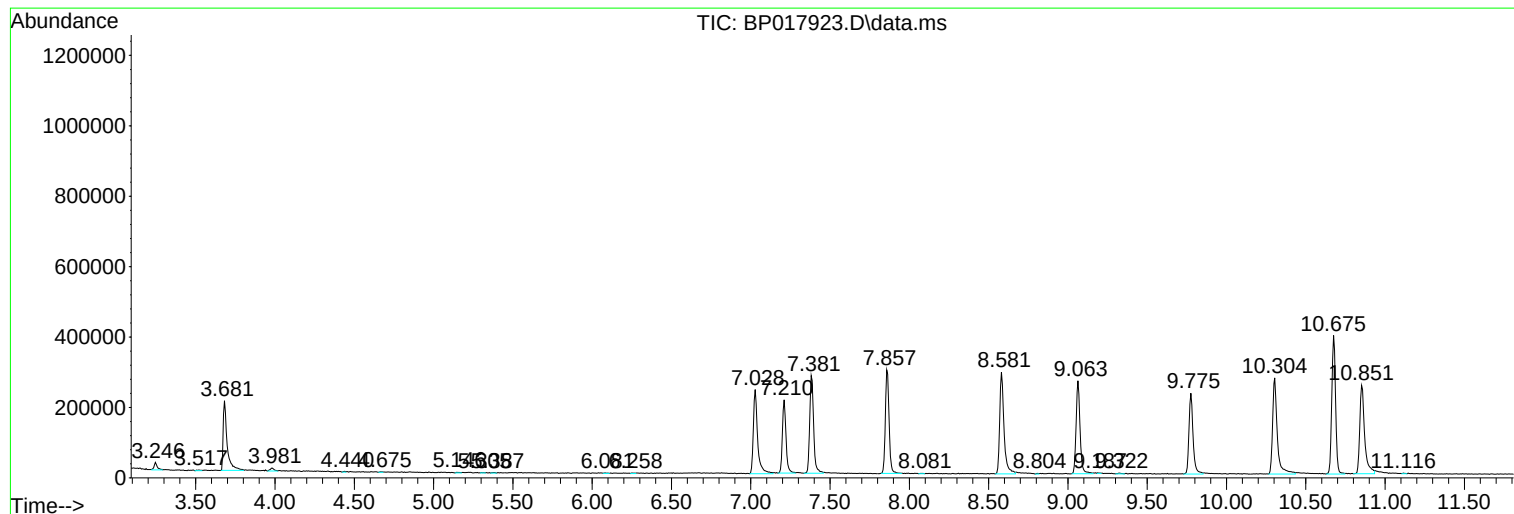

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017923.D
Acq On : 07 Nov 2023 09:20
Operator : MA/JU
Sample : PB156841BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK841

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017923.D
Acq On : 07 Nov 2023 09:20
Operator : MA/JU
Sample : PB156841BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK841

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc