

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
 Data File : BP017927.D
 Acq On : 07 Nov 2023 16:34
 Operator : MA/JU
 Sample : PB156694BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK694

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017927.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	23	26	32	rBV	23703	30680	1.47%	0.140%
2	3.675	96	100	118	rBV	259487	438773	20.97%	2.002%
3	3.975	149	151	154	rBV3	4277	5338	0.26%	0.024%
4	5.793	458	460	464	rVB5	1901	2150	0.10%	0.010%
5	6.822	631	635	641	rVB9	2045	4223	0.20%	0.019%
6	7.022	662	669	690	rBV	320563	587906	28.09%	2.683%
7	7.211	695	701	710	rBV	268723	427245	20.42%	1.949%
8	7.381	723	730	742	rBV	378267	606738	28.99%	2.768%
9	7.858	805	811	822	rBV	281564	454874	21.74%	2.076%
10	8.581	927	934	950	rBV	381540	717495	34.29%	3.274%
11	9.063	1008	1016	1029	rBV	353409	605261	28.92%	2.762%
12	9.775	1129	1137	1149	rBV	299840	542601	25.93%	2.476%
13	10.299	1220	1226	1243	rBV	377595	729318	34.85%	3.328%
14	10.675	1283	1290	1299	rVV	378661	627734	30.00%	2.864%
15	10.852	1312	1320	1338	rBV	358782	718364	34.33%	3.278%
16	12.281	1559	1563	1574	rBV8	4452	10502	0.50%	0.048%
17	13.357	1742	1746	1752	rBV8	5577	8864	0.42%	0.040%
18	13.940	1839	1845	1861	rBV	852672	1215159	58.07%	5.545%
19	14.222	1885	1893	1902	rBV2	890341	1321329	63.14%	6.029%
20	14.522	1937	1944	1956	rBV	589591	855983	40.90%	3.906%
21	14.775	1981	1987	2002	rBV	167133	426078	20.36%	1.944%
22	15.522	2105	2114	2123	rBV	1145998	1628440	77.82%	7.430%
23	15.669	2133	2139	2151	rBV	372032	587088	28.05%	2.679%
24	15.757	2152	2154	2159	rVB5	7146	10777	0.51%	0.049%
25	16.039	2200	2202	2205	rBV3	1425	2168	0.10%	0.010%
26	16.104	2209	2213	2216	rBV5	2122	3860	0.18%	0.018%
27	16.169	2221	2224	2228	rBV6	1599	2382	0.11%	0.011%
28	16.310	2245	2248	2252	rVB6	1622	3069	0.15%	0.014%
29	16.963	2354	2359	2362	rBV7	2457	3553	0.17%	0.016%
30	17.081	2377	2379	2384	rBV6	1545	2867	0.14%	0.013%
31	17.292	2406	2415	2426	rBV	732697	1056074	50.46%	4.819%
32	17.392	2426	2432	2448	rVV	1198386	1788500	85.46%	8.161%
33	18.063	2545	2546	2551	rVB5	1761	2206	0.11%	0.010%
34	18.163	2559	2563	2567	rBV7	2993	6344	0.30%	0.029%
35	18.504	2619	2621	2624	rBV4	2562	3326	0.16%	0.015%
36	18.551	2627	2629	2632	rBV4	2620	2763	0.13%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017927.D
Acq On : 07 Nov 2023 16:34
Operator : MA/JU
Sample : PB156694BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK694

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Title : SVOA CALIBRATION

37	19.216	2738	2742	2747	rBV4	15226	21957	1.05%	0.100%
38	19.286	2750	2754	2760	rVV2	12629	20807	0.99%	0.095%
39	19.645	2809	2815	2825	rBV	1626161	2092707	100.00%	9.549%
40	21.410	3110	3115	3125	rBV	782569	1133915	54.18%	5.174%
41	23.733	3502	3510	3520	rVB2	997562	2077382	99.27%	9.479%
42	23.892	3531	3537	3547	rVB	548936	1129056	53.95%	5.152%




Sum of corrected areas: 21915856

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017927.D
Acq On : 07 Nov 2023 16:34
Operator : MA/JU
Sample : PB156694BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK694

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

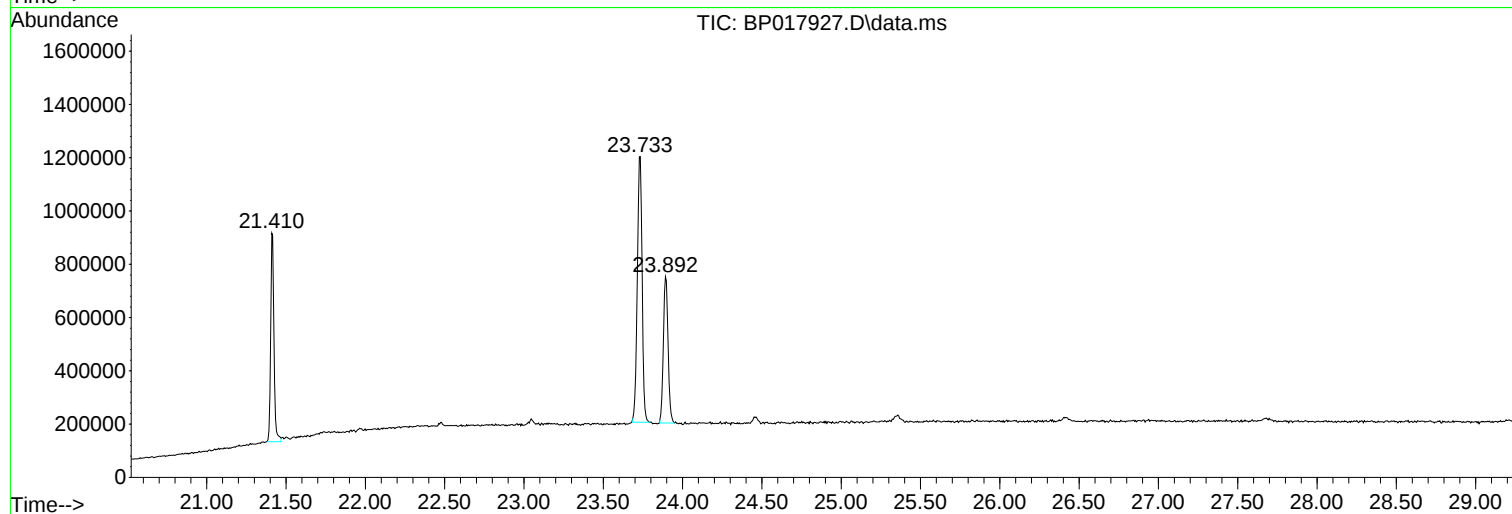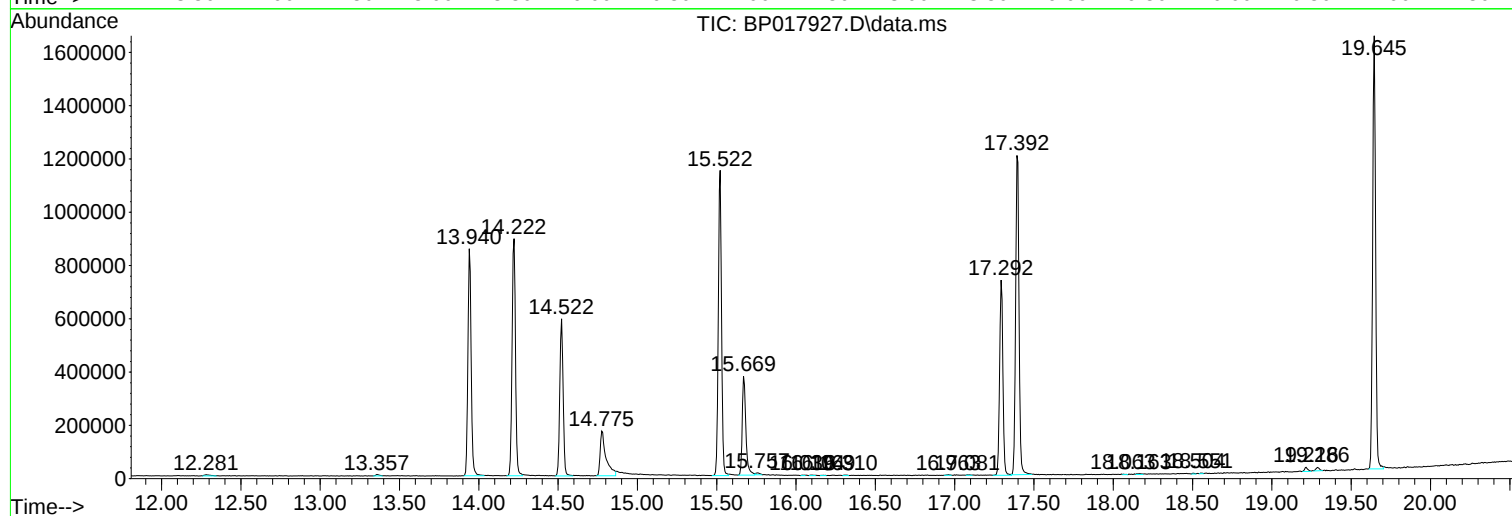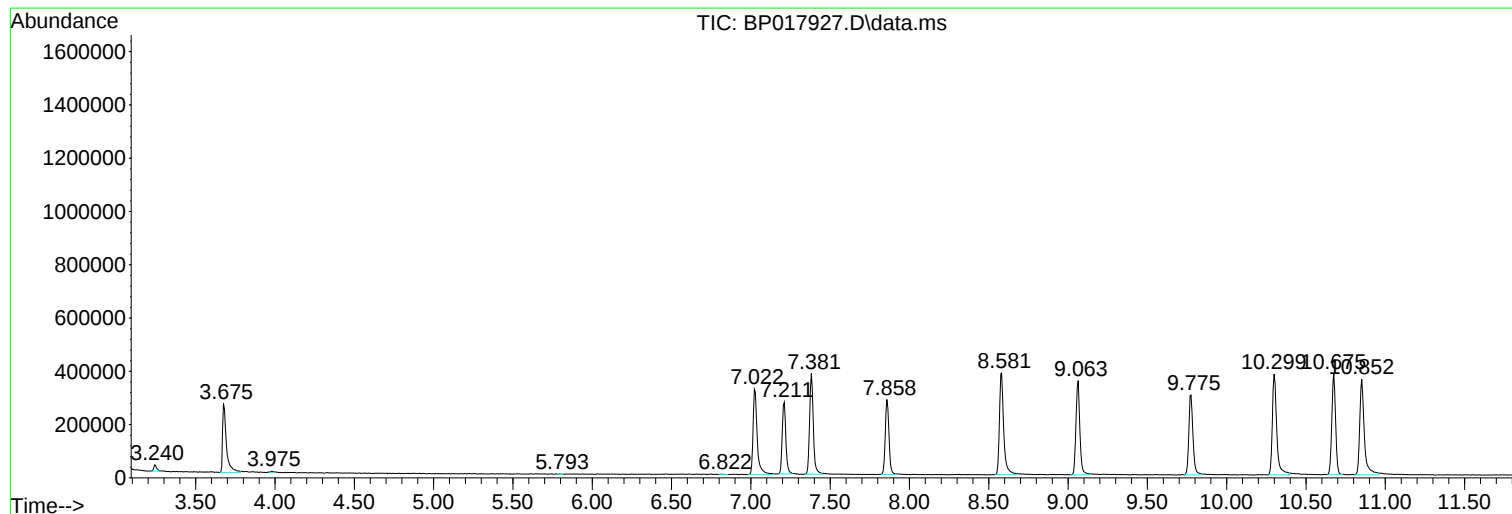

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017927.D
Acq On : 07 Nov 2023 16:34
Operator : MA/JU
Sample : PB156694BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK694

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017927.D
Acq On : 07 Nov 2023 16:34
Operator : MA/JU
Sample : PB156694BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK694

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc