

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
 Data File : BP017941.D
 Acq On : 08 Nov 2023 00:30
 Operator : MA/JU
 Sample : 05026-11
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH361

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017941.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	23	26	35	rVB	15714	24833	0.91%	0.104%
2	3.687	99	102	114	rBV	51158	91452	3.34%	0.385%
3	3.858	128	131	135	rVB2	6128	6944	0.25%	0.029%
4	3.975	149	151	156	rVB5	5266	5594	0.20%	0.024%
5	7.028	661	670	680	rBV	62745	129825	4.75%	0.546%
6	7.205	692	700	712	rBV	297079	494892	18.10%	2.081%
7	7.381	723	730	743	rBV	307566	525395	19.22%	2.209%
8	7.587	761	765	768	rVB6	2442	4073	0.15%	0.017%
9	7.858	804	811	823	rBV	295892	487247	17.82%	2.049%
10	8.169	860	864	865	rBV4	1980	2737	0.10%	0.012%
11	8.581	926	934	950	rBV	206880	412609	15.09%	1.735%
12	9.058	1008	1015	1026	rBV	406097	694830	25.41%	2.922%
13	9.769	1128	1136	1148	rBV2	355404	621036	22.71%	2.612%
14	9.887	1151	1156	1163	rVB2	3035	7645	0.28%	0.032%
15	10.299	1216	1226	1241	rBV	414054	792232	28.97%	3.332%
16	10.669	1282	1289	1304	rBV	405322	685209	25.06%	2.881%
17	10.852	1311	1320	1336	rBV	337798	673258	24.62%	2.831%
18	11.381	1402	1410	1419	rBV	20899	57186	2.09%	0.240%
19	11.593	1442	1446	1449	rBV6	3028	4946	0.18%	0.021%
20	12.269	1558	1561	1569	rBV7	5096	12068	0.44%	0.051%
21	12.834	1654	1657	1661	rBV6	2028	2753	0.10%	0.012%
22	13.081	1697	1699	1705	rVB7	2033	3372	0.12%	0.014%
23	13.357	1742	1746	1756	rVB2	13072	24203	0.89%	0.102%
24	13.940	1838	1845	1850	rBV	777329	1083483	39.63%	4.556%
25	13.987	1850	1853	1862	rVB2	40000	59477	2.18%	0.250%
26	14.081	1867	1869	1875	rVB7	2681	4001	0.15%	0.017%
27	14.222	1884	1893	1909	rBV	1048681	1573671	57.55%	6.618%
28	14.516	1933	1943	1953	rBV	597330	919721	33.64%	3.868%
29	14.751	1976	1983	1988	rBV	28262	45800	1.68%	0.193%
30	14.810	1988	1993	2004	rVV3	16875	53300	1.95%	0.224%
31	15.163	2048	2053	2058	rVB6	8687	12481	0.46%	0.052%
32	15.340	2079	2083	2086	rBV6	3901	5217	0.19%	0.022%
33	15.516	2107	2113	2128	rBV	1411671	2033616	74.38%	8.552%
34	15.669	2133	2139	2150	rBV	512387	747515	27.34%	3.144%
35	15.757	2152	2154	2158	rVB4	7465	9148	0.33%	0.038%
36	16.310	2245	2248	2249	rVV3	2752	2837	0.10%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
 Data File : BP017941.D
 Acq On : 08 Nov 2023 00:30
 Operator : MA/JU
 Sample : 05026-11
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH361

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
 Title : SVOA CALIBRATION

37	16.387	2258	2261	2266	rBV7	4162	6755	0.25%	0.028%
38	16.551	2286	2289	2293	rBV6	2662	3638	0.13%	0.015%
39	16.610	2295	2299	2301	rVV4	2468	3476	0.13%	0.015%
40	16.657	2301	2307	2313	rVB4	3940	7727	0.28%	0.032%
41	16.845	2337	2339	2343	rVB5	2050	2740	0.10%	0.012%
42	16.957	2354	2358	2363	rBV7	3336	5924	0.22%	0.025%
43	17.081	2376	2379	2381	rVB4	2574	2736	0.10%	0.012%
44	17.122	2383	2386	2389	rBV5	1816	3005	0.11%	0.013%
45	17.292	2409	2415	2425	rBV	801480	1109753	40.59%	4.667%
46	17.392	2426	2432	2446	rVV	1742111	2358715	86.27%	9.919%
47	17.657	2474	2477	2480	rBV5	2347	3547	0.13%	0.015%
48	17.922	2517	2522	2527	rBV9	7620	10949	0.40%	0.046%
49	18.134	2554	2558	2564	rBV2	47282	68128	2.49%	0.286%
50	18.233	2572	2575	2577	rVB2	3314	3200	0.12%	0.013%
51	18.951	2694	2697	2703	rVB7	5754	7644	0.28%	0.032%
52	19.045	2710	2713	2716	rBV5	5534	7325	0.27%	0.031%
53	19.210	2737	2741	2745	rBV2	19143	25886	0.95%	0.109%
54	19.286	2750	2754	2758	rVB	20785	28322	1.04%	0.119%
55	19.375	2766	2769	2778	rBV3	39555	64686	2.37%	0.272%
56	19.516	2790	2793	2796	rBV4	9204	9830	0.36%	0.041%
57	19.639	2809	2814	2825	rBV	2099932	2734233	100.00%	11.498%
58	21.410	3110	3115	3125	rBV	874011	1170918	42.82%	4.924%
59	23.727	3501	3509	3519	rVB2	1328141	2656777	97.17%	11.172%
60	23.886	3530	3536	3547	rVB	569160	1169173	42.76%	4.917%




Sum of corrected areas: 23779693

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017941.D
Acq On : 08 Nov 2023 00:30
Operator : MA/JU
Sample : 05026-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH361

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

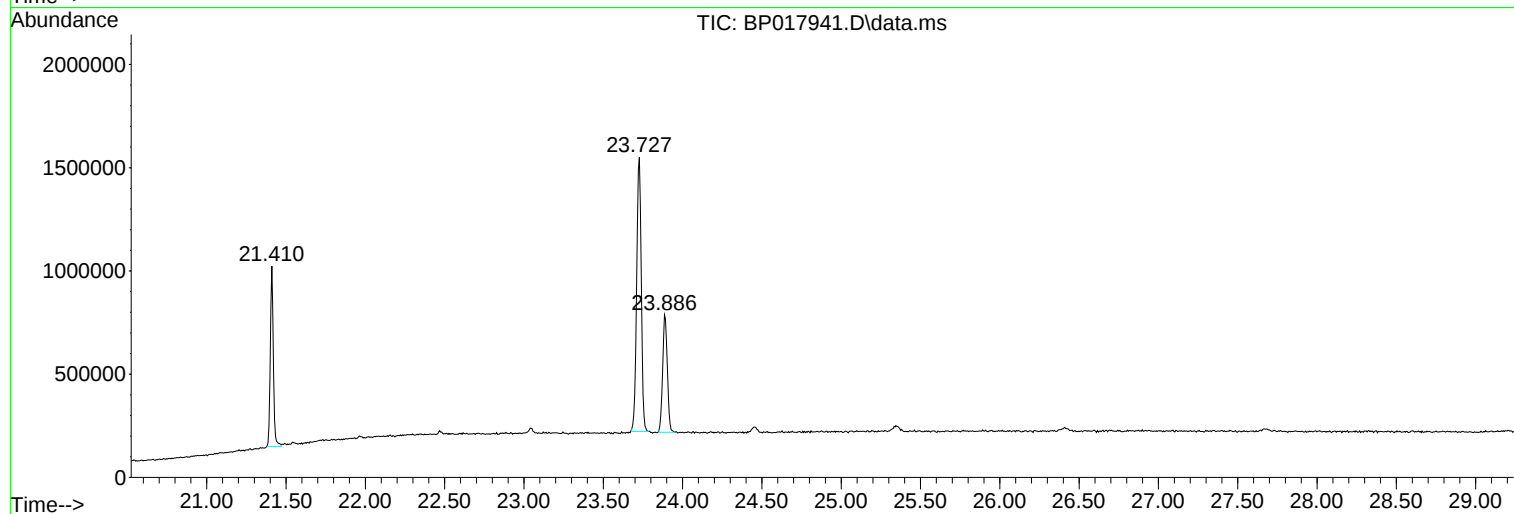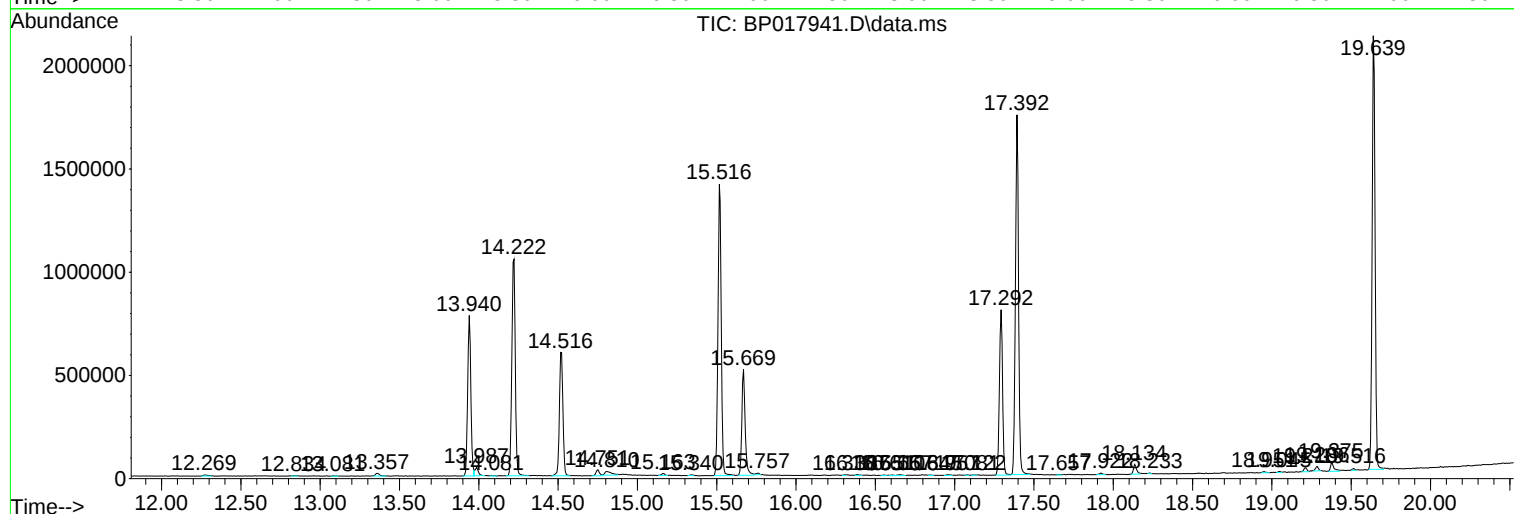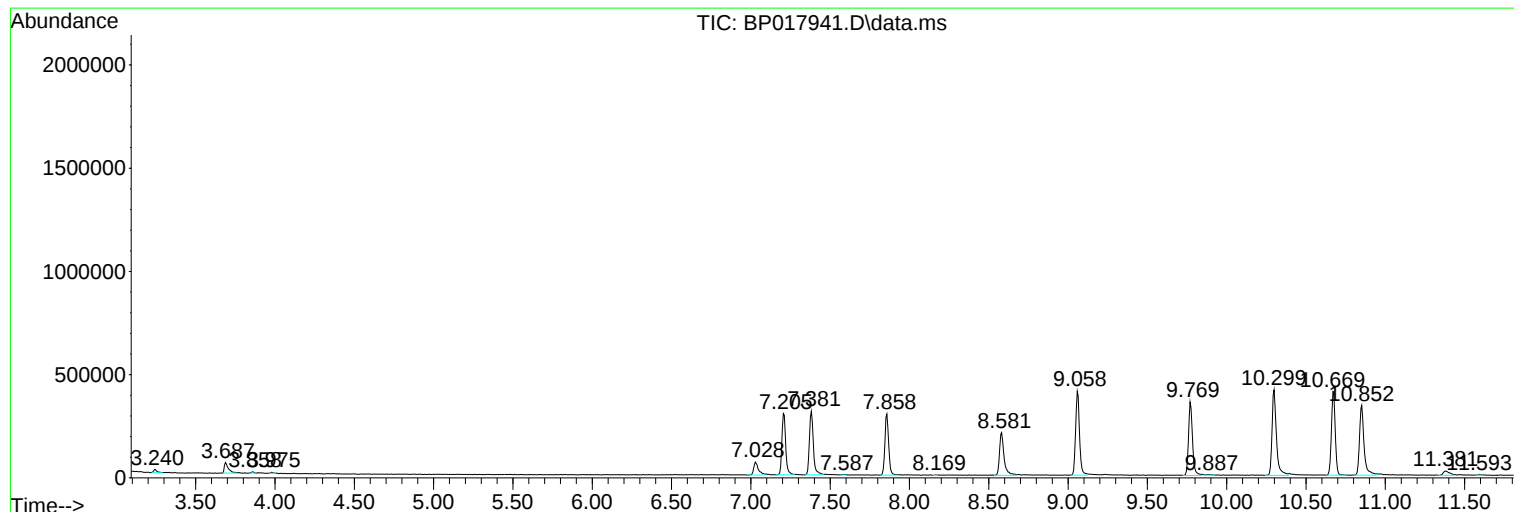

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017941.D
Acq On : 08 Nov 2023 00:30
Operator : MA/JU
Sample : 05026-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH361

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017941.D
Acq On : 08 Nov 2023 00:30
Operator : MA/JU
Sample : 05026-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH361

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc