

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
 Data File : BP017942.D
 Acq On : 08 Nov 2023 01:04
 Operator : MA/JU
 Sample : 05026-12
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH353

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017942.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	23	26	29	rBV	13598	17415	0.66%	0.075%
2	3.275	29	32	41	rVB	38403	55223	2.09%	0.238%
3	3.358	44	46	50	rVB2	8785	10018	0.38%	0.043%
4	3.693	100	103	114	rBV	34142	65223	2.47%	0.282%
5	3.852	126	130	135	rVB3	14411	21125	0.80%	0.091%
6	3.981	148	152	154	rVV4	5407	7219	0.27%	0.031%
7	4.499	236	240	241	rBV4	1907	2639	0.10%	0.011%
8	5.722	444	448	455	rVB	36202	54448	2.07%	0.235%
9	6.051	500	504	513	rVB	9643	16977	0.64%	0.073%
10	7.034	663	671	688	rBV2	54275	147747	5.60%	0.638%
11	7.204	694	700	715	rBV	276108	447302	16.97%	1.932%
12	7.381	723	730	745	rBV	282019	473778	17.97%	2.046%
13	7.675	776	780	784	rBV7	1756	2665	0.10%	0.012%
14	7.857	804	811	822	rBV	293158	478190	18.14%	2.065%
15	8.398	895	903	910	rBV2	13506	25006	0.95%	0.108%
16	8.581	925	934	952	rBV	190629	370592	14.06%	1.600%
17	9.057	1007	1015	1027	rBV	374688	647355	24.55%	2.796%
18	9.463	1081	1084	1088	rBV7	1977	2774	0.11%	0.012%
19	9.769	1128	1136	1151	rBV	316962	557732	21.15%	2.409%
20	10.040	1174	1182	1187	rBV	23565	40279	1.53%	0.174%
21	10.187	1201	1207	1210	rVV8	2933	5098	0.19%	0.022%
22	10.298	1218	1226	1239	rBV	370322	722785	27.41%	3.121%
23	10.669	1282	1289	1303	rVB	387690	669520	25.39%	2.891%
24	10.851	1309	1320	1339	rBV	241626	540287	20.49%	2.333%
25	11.039	1344	1352	1359	rVB6	22409	49358	1.87%	0.213%
26	11.187	1373	1377	1378	rBV4	9466	11027	0.42%	0.048%
27	11.381	1406	1410	1414	rBV7	5412	10558	0.40%	0.046%
28	11.428	1414	1418	1422	rVV2	13083	22815	0.87%	0.099%
29	11.463	1422	1424	1429	rVB3	7122	9580	0.36%	0.041%
30	11.534	1431	1436	1442	rBV9	4525	8829	0.33%	0.038%
31	11.598	1442	1447	1448	rBV5	4222	6511	0.25%	0.028%
32	11.704	1458	1465	1477	rVB	58147	104673	3.97%	0.452%
33	12.269	1555	1561	1567	rVB6	6362	12164	0.46%	0.053%
34	12.357	1567	1576	1589	rBV4	8217	31535	1.20%	0.136%
35	13.075	1697	1698	1705	rVB6	1896	2831	0.11%	0.012%
36	13.363	1741	1747	1754	rBV3	12772	21858	0.83%	0.094%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
 Data File : BP017942.D
 Acq On : 08 Nov 2023 01:04
 Operator : MA/JU
 Sample : 05026-12
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH353

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
 Title : SVOA CALIBRATION

37	13.828	1824	1826	1832	rVB7	2389	3312	0.13%	0.014%
38	13.939	1839	1845	1851	rBV	869916	1176060	44.61%	5.079%
39	14.216	1885	1892	1905	rBV	989396	1455348	55.20%	6.285%
40	14.310	1907	1908	1913	rVB5	2631	3734	0.14%	0.016%
41	14.516	1936	1943	1952	rBV	602378	884117	33.53%	3.818%
42	14.810	1988	1993	2003	rVV5	18327	56282	2.13%	0.243%
43	14.916	2007	2011	2015	rVB6	3031	6543	0.25%	0.028%
44	15.075	2035	2038	2041	rBV5	2652	2919	0.11%	0.013%
45	15.163	2048	2053	2056	rBV7	4833	7519	0.29%	0.032%
46	15.263	2066	2070	2074	rVV	13254	15932	0.60%	0.069%
47	15.516	2106	2113	2127	rBV	1332883	1875065	71.12%	8.097%
48	15.669	2133	2139	2151	rBV	496027	709184	26.90%	3.063%
49	15.757	2151	2154	2160	rVB7	8266	13323	0.51%	0.058%
50	16.239	2231	2236	2240	rBV8	4065	8104	0.31%	0.035%
51	16.327	2246	2251	2256	rBV	8078	14188	0.54%	0.061%
52	16.380	2256	2260	2268	rVV7	8419	18622	0.71%	0.080%
53	16.445	2268	2271	2275	rVV5	7815	10820	0.41%	0.047%
54	16.492	2276	2279	2282	rVV5	4298	4358	0.17%	0.019%
55	16.551	2285	2289	2291	rBV5	3399	4277	0.16%	0.018%
56	16.592	2293	2296	2301	rVB7	3030	4528	0.17%	0.020%
57	16.651	2301	2306	2311	rVB6	7067	13789	0.52%	0.060%
58	16.727	2311	2319	2322	rBV4	5582	11198	0.42%	0.048%
59	16.774	2322	2327	2335	rVV2	19776	41382	1.57%	0.179%
60	16.851	2337	2340	2344	rVB5	7481	8883	0.34%	0.038%
61	16.963	2357	2359	2365	rVB7	3656	3396	0.13%	0.015%
62	17.204	2398	2400	2406	rVB7	1919	2765	0.10%	0.012%
63	17.292	2409	2415	2425	rVV	808422	1098537	41.67%	4.744%
64	17.392	2425	2432	2445	rVV	1627701	2246430	85.20%	9.701%
65	17.921	2519	2522	2526	rBV6	6392	7031	0.27%	0.030%
66	18.133	2554	2558	2568	rBV4	26801	47063	1.79%	0.203%
67	18.345	2592	2594	2599	rBV6	2073	3030	0.11%	0.013%
68	19.210	2737	2741	2745	rBV3	21041	26057	0.99%	0.113%
69	19.280	2750	2753	2757	rVB2	20895	27733	1.05%	0.120%
70	19.374	2766	2769	2776	rBV5	23263	33831	1.28%	0.146%
71	19.515	2789	2793	2800	rBV3	16962	19742	0.75%	0.085%
72	19.639	2808	2814	2823	rBV	1930296	2636562	100.00%	11.386%
73	21.410	3110	3115	3126	rBV	887380	1176690	44.63%	5.081%
74	23.727	3501	3509	3521	rVB2	1297450	2608210	98.92%	11.263%
75	23.892	3530	3537	3550	rVB	588379	1196937	45.40%	5.169%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017942.D
Acq On : 08 Nov 2023 01:04
Operator : MA/JU
Sample : 05026-12
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH353

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 23156637

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017942.D
Acq On : 08 Nov 2023 01:04
Operator : MA/JU
Sample : 05026-12
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH353

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

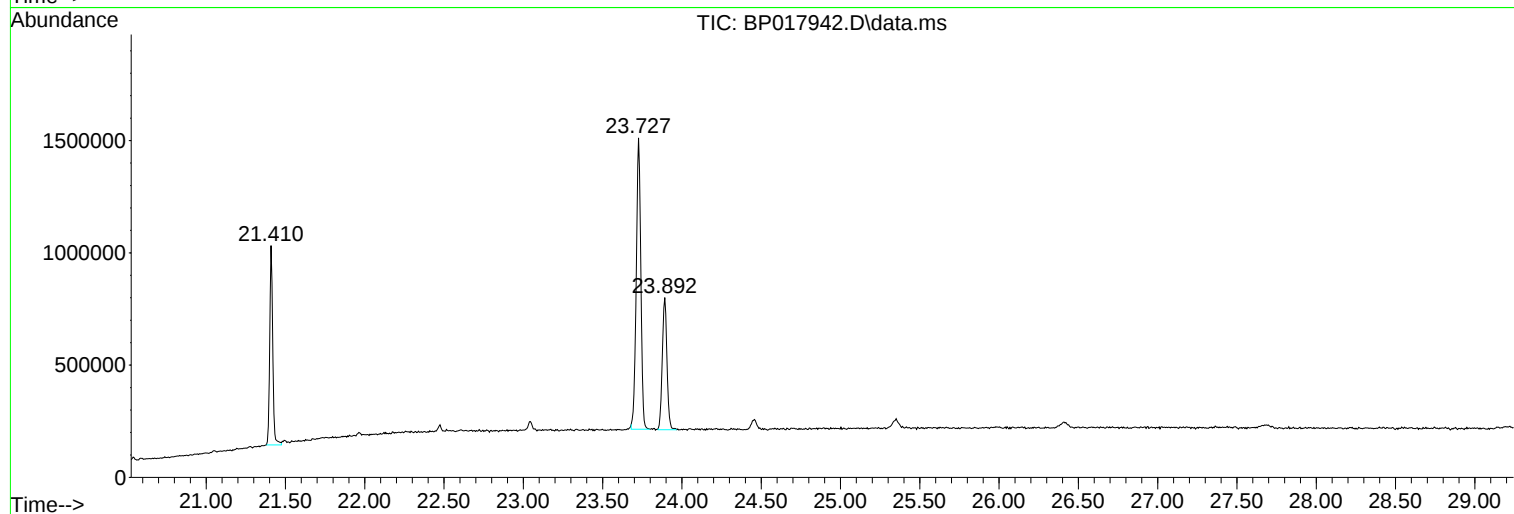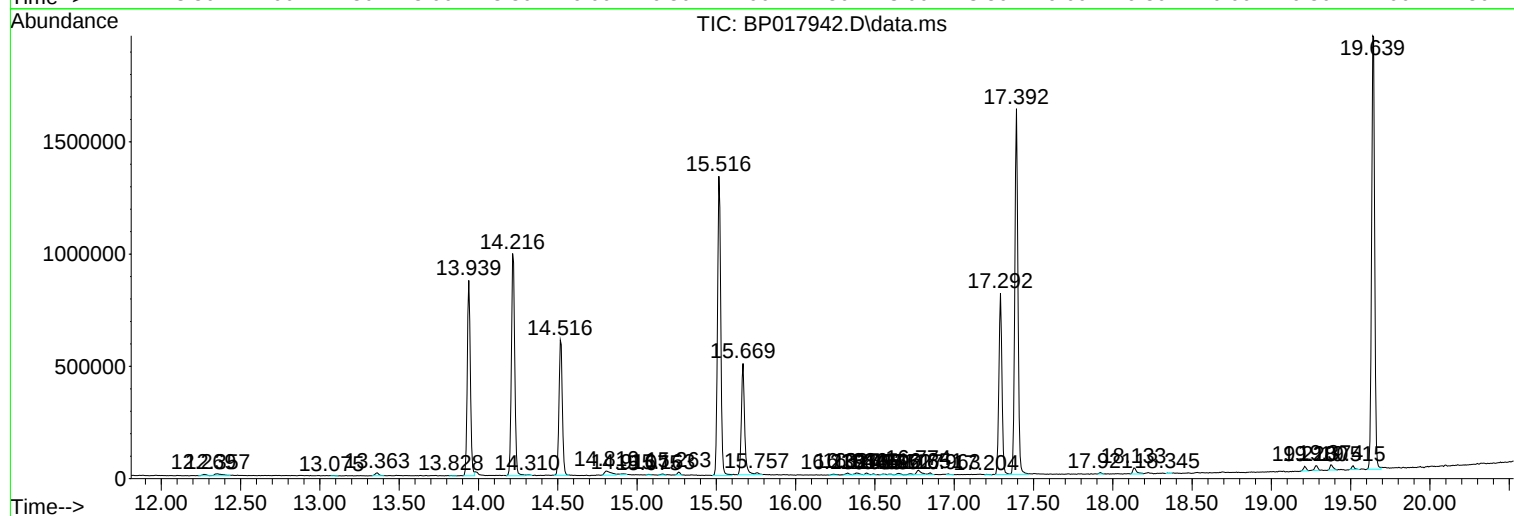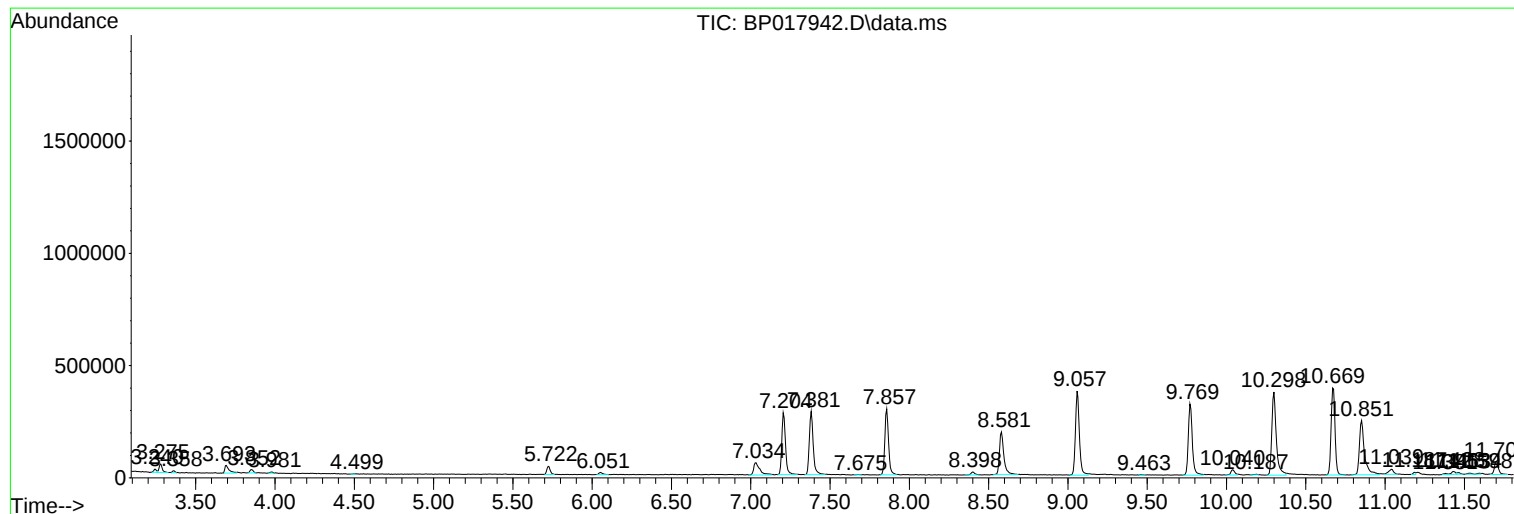

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017942.D
Acq On : 08 Nov 2023 01:04
Operator : MA/JU
Sample : 05026-12
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH353










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1-Butanol, 3-methoxy- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.722	2.28 ng/ul	54448	1,4-Dichlorobenzene-d4	7.857

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Butanol, 3-methoxy-			104	C5H12O2	002517-43-3	64
2	2-Hexanol, methyl ether			116	C7H16O	1000333-92-0	53
3	2-Decanol, methyl ether			172	C11H24O	1000333-83-9	53
4	1-Butanol, 3-methoxy-			104	C5H12O2	002517-43-3	50
5	3-Pentanol, 2-methyl-			102	C6H14O	000565-67-3	50

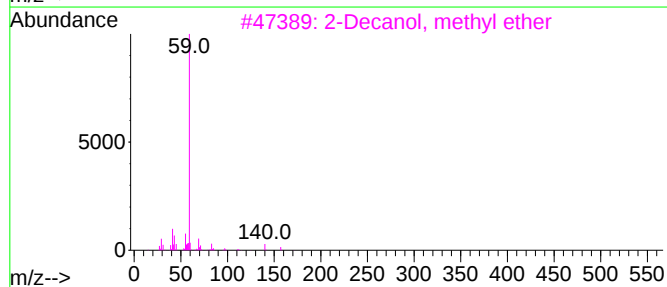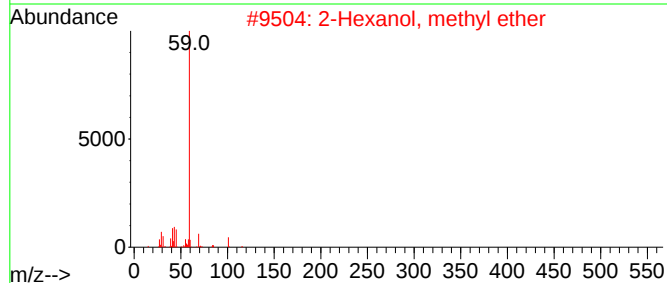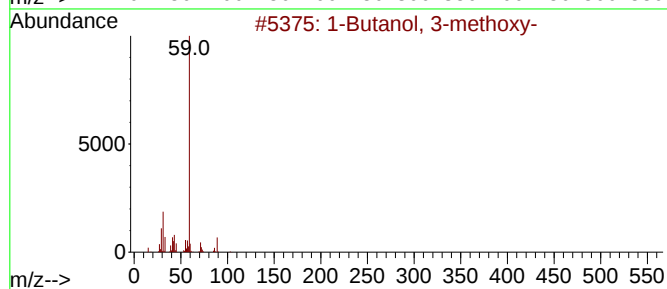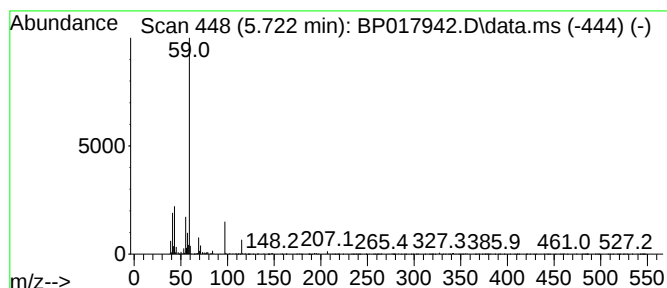

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017942.D
Acq On : 08 Nov 2023 01:04
Operator : MA/JU
Sample : 05026-12
Misc :
ALS Vial : 21 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
BH353

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 3,5,9-Undecatrien-2-one, 6,... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
11.704	3.13 ng/ul	104673	Naphthalene-d8	10.669	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	3,5,9-Undecatrien-2-one, 6,10-di...	192	C13H20O	000141-10-6	50
2	3-Methylpentyl acetate	144	C8H16O2	035897-13-3	38
3	1H-Pyrazole, 4,5-dihydro-5-methyl-	84	C4H8N2	001568-20-3	38
4	Ethanone, 1-cyclopropyl-	84	C5H8O	000765-43-5	35
5	2-Octen-4-one	126	C8H14O	004643-27-0	35

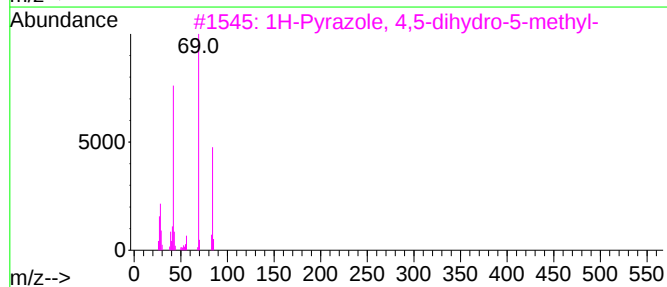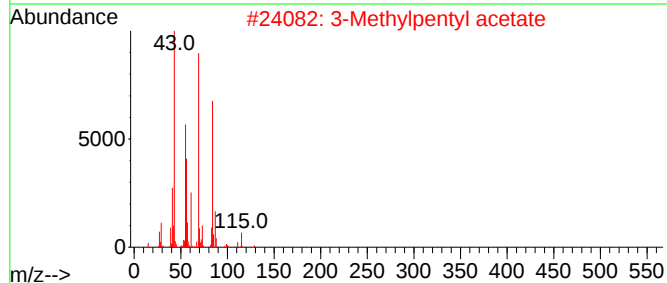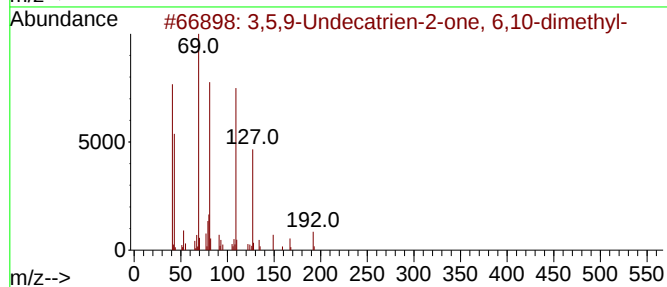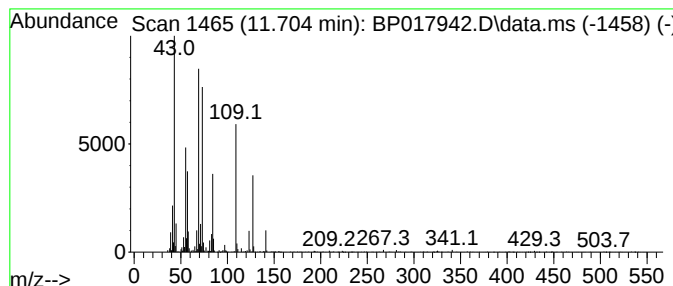

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017942.D
Acq On : 08 Nov 2023 01:04
Operator : MA/JU
Sample : 05026-12
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH353

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Butanol, 3-me...	5.722	2.3	ng/ul	54448	1	7.857	478190	20.0
3,5,9-Undecatri...	11.704	3.1	ng/ul	104673	2	10.669	669520	20.0