

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
 Data File : BP017946.D
 Acq On : 08 Nov 2023 03:54
 Operator : MA/JU
 Sample : PB156696BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK696

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017946.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	21	26	33	rBV	34320	46339	1.60%	0.151%
2	3.675	96	100	121	rBV	377057	624017	21.52%	2.039%
3	3.975	148	151	155	rVB2	5961	6703	0.23%	0.022%
4	7.022	663	669	686	rBV	485080	840166	28.98%	2.745%
5	7.205	694	700	710	rBV	407343	628555	21.68%	2.054%
6	7.375	722	729	743	rBV	526555	880376	30.37%	2.876%
7	7.858	803	811	821	rBV	369319	603177	20.80%	1.971%
8	8.575	926	933	952	rBV	601854	1067979	36.84%	3.489%
9	9.057	1008	1015	1032	rBV	524629	882267	30.43%	2.883%
10	9.769	1129	1136	1148	rBV	474269	797961	27.52%	2.607%
11	10.293	1219	1225	1247	rBV	568506	1090409	37.61%	3.563%
12	10.669	1281	1289	1298	rBV	505508	843274	29.09%	2.755%
13	10.846	1312	1319	1339	rBV	533139	1046794	36.11%	3.420%
14	12.275	1558	1562	1567	rBV7	5748	12085	0.42%	0.039%
15	13.357	1741	1746	1756	rVB5	12940	25133	0.87%	0.082%
16	13.940	1837	1845	1865	rBV	1210135	1702875	58.73%	5.564%
17	14.216	1885	1892	1905	rBV	1300622	1911845	65.94%	6.246%
18	14.516	1936	1943	1951	rBV	753054	1118625	38.58%	3.655%
19	14.769	1980	1986	2009	rBV	254838	694721	23.96%	2.270%
20	14.969	2018	2020	2028	rVV9	3554	5416	0.19%	0.018%
21	15.516	2105	2113	2130	rBV	1624131	2337417	80.62%	7.637%
22	15.669	2133	2139	2150	rVV	531510	799222	27.57%	2.611%
23	15.757	2150	2154	2160	rVB7	10322	18968	0.65%	0.062%
24	16.963	2352	2359	2364	rVB7	2137	4737	0.16%	0.015%
25	17.292	2408	2415	2424	rBV	973604	1351458	46.61%	4.416%
26	17.392	2426	2432	2445	rVV	1753810	2517615	86.84%	8.226%
27	18.316	2583	2589	2593	rVB9	3051	6030	0.21%	0.020%
28	19.210	2737	2741	2745	rBV3	22852	32132	1.11%	0.105%
29	19.280	2748	2753	2759	rVV2	56937	74815	2.58%	0.244%
30	19.380	2767	2770	2771	rBV3	4604	4933	0.17%	0.016%
31	19.516	2788	2793	2797	rBV	134436	155910	5.38%	0.509%
32	19.639	2808	2814	2825	rBV	2252565	2899278	100.00%	9.473%
33	20.333	2929	2932	2937	rBV4	20481	22705	0.78%	0.074%
34	20.539	2963	2967	2972	rBV2	109283	120734	4.16%	0.394%
35	21.410	3110	3115	3125	rBV	996583	1368814	47.21%	4.472%
36	23.727	3501	3509	3523	rVB2	1304242	2742200	94.58%	8.959%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017946.D
Acq On : 08 Nov 2023 03:54
Operator : MA/JU
Sample : PB156696BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK696

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Title : SVOA CALIBRATION

37	23.886	3530	3536	3545	rVB	637502	1321128	45.57%	4.316%
----	--------	------	------	------	-----	--------	---------	--------	--------




Sum of corrected areas: 30606813

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017946.D
Acq On : 08 Nov 2023 03:54
Operator : MA/JU
Sample : PB156696BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK696

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

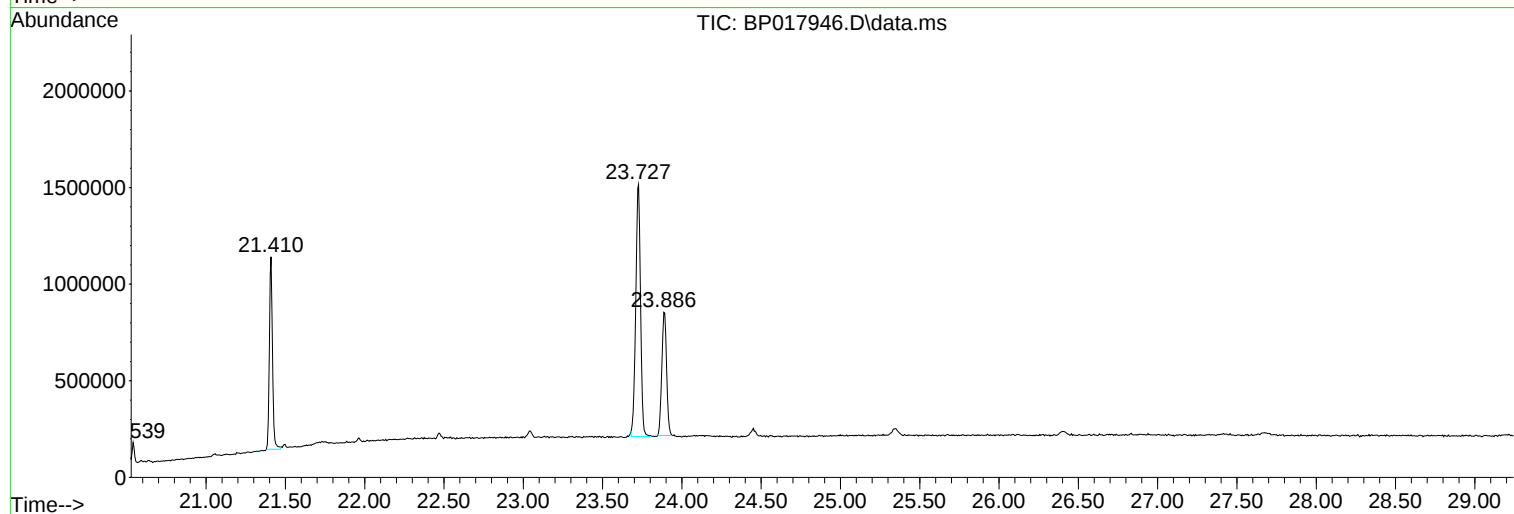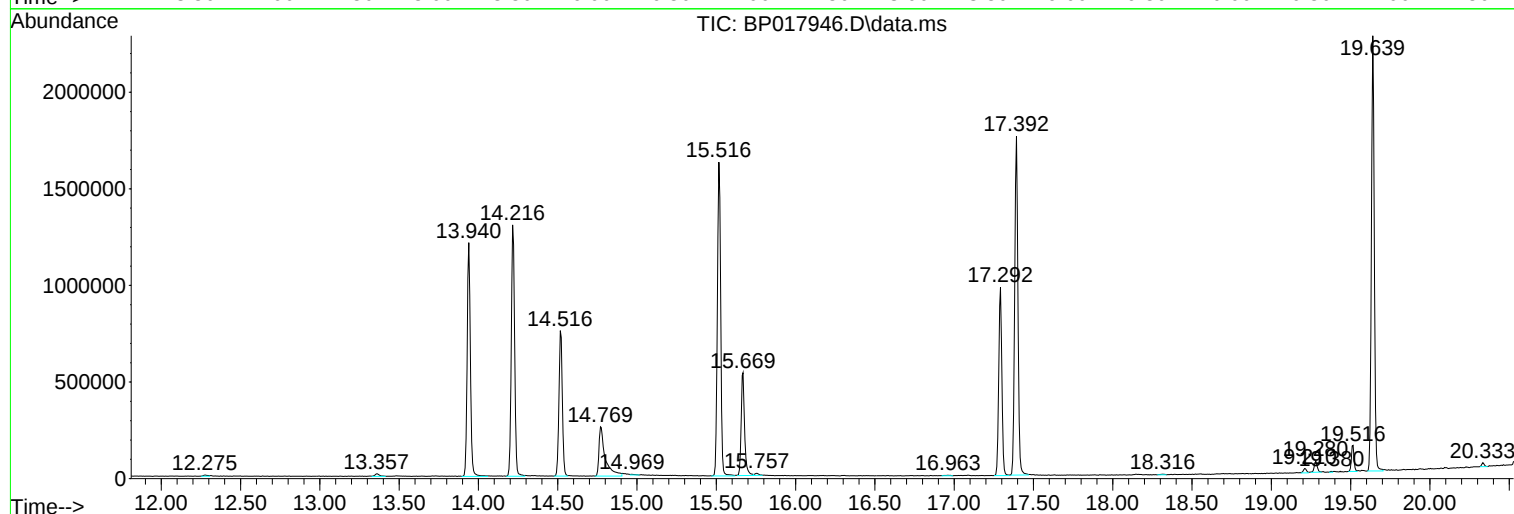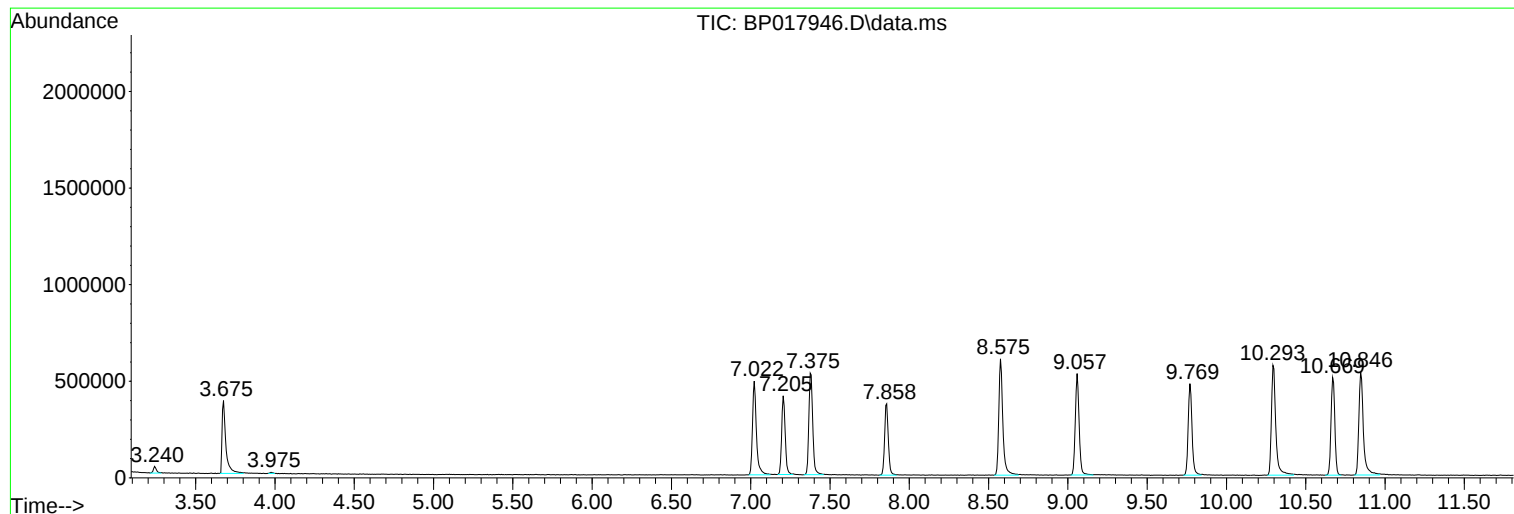

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017946.D
Acq On : 08 Nov 2023 03:54
Operator : MA/JU
Sample : PB156696BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK696










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Hexadecanoic acid, 2-methyl... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
19.516	2.28 ng/ul	155910	Chrysene-d12	21.410

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Hexadecanoic acid, 2-methylpropy...	312	C20H40O2	000110-34-9	93
2			Hexadecanoic acid, butyl ester	312	C20H40O2	000111-06-8	91
3			Hexadecanoic acid, butyl ester	312	C20H40O2	000111-06-8	90
4			Hexadecanoic acid, 2-methylpropy...	312	C20H40O2	000110-34-9	86
5			Hexadecanoic acid, 1,1-dimethyle...	312	C20H40O2	031158-91-5	60

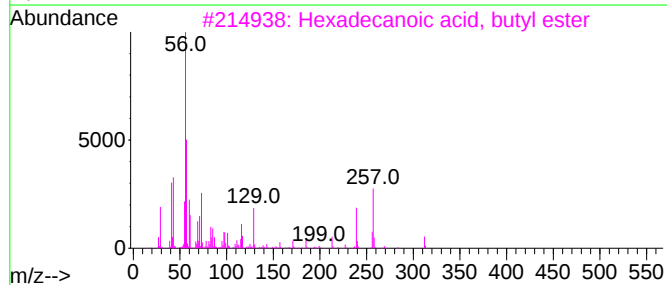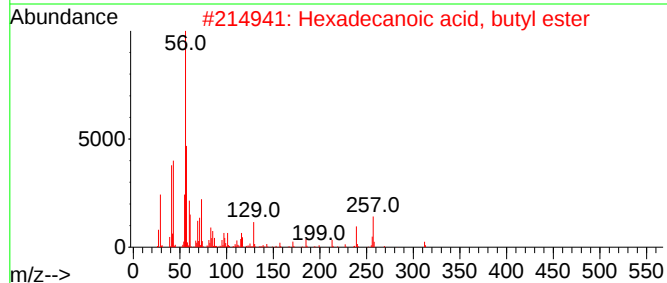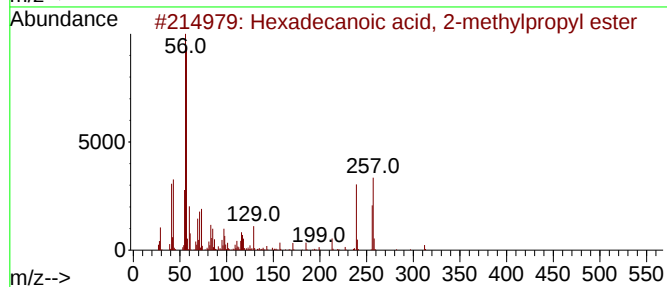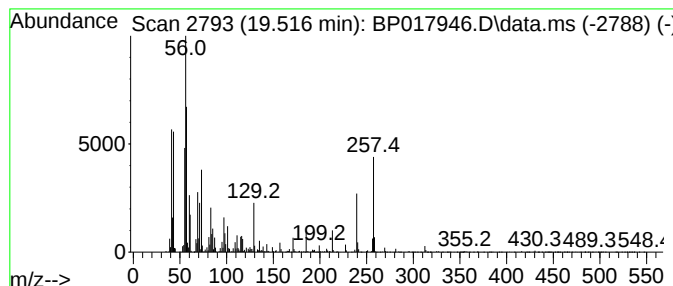

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017946.D
Acq On : 08 Nov 2023 03:54
Operator : MA/JU
Sample : PB156696BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK696

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Hexadecanoic ac...	19.516	2.3	ng/ul	155910	5	21.410	1368810	20.0