

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
 Data File : BP017947.D
 Acq On : 08 Nov 2023 04:28
 Operator : MA/JU
 Sample : PB156698BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK698

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017947.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	23	26	34	rVB	30651	41589	1.61%	0.157%
2	3.675	96	100	124	rBV	340582	567659	21.93%	2.146%
3	3.981	149	152	157	rVB6	5590	7928	0.31%	0.030%
4	4.940	311	315	318	rBV6	1594	2709	0.10%	0.010%
5	6.405	559	564	568	rVV8	1570	2993	0.12%	0.011%
6	6.464	570	574	577	rVB6	1869	2654	0.10%	0.010%
7	7.022	662	669	682	rBV	419813	731857	28.28%	2.767%
8	7.205	694	700	714	rBV	348289	543250	20.99%	2.054%
9	7.381	722	730	744	rBV	459742	773848	29.90%	2.926%
10	7.858	803	811	823	rBV	314564	508754	19.66%	1.923%
11	8.575	926	933	954	rBV2	525243	924080	35.70%	3.494%
12	8.828	974	976	980	rVB4	2474	2761	0.11%	0.010%
13	9.058	1008	1015	1030	rBV	457377	772932	29.86%	2.922%
14	9.769	1127	1136	1148	rBV	412355	705909	27.27%	2.669%
15	10.299	1219	1226	1247	rBV	496577	960842	37.12%	3.633%
16	10.669	1281	1289	1301	rVB	429793	715550	27.65%	2.705%
17	10.846	1312	1319	1338	rBV	466642	918515	35.49%	3.473%
18	12.287	1558	1564	1575	rVB10	5512	14923	0.58%	0.056%
19	13.357	1741	1746	1751	rBV5	6549	11428	0.44%	0.043%
20	13.940	1838	1845	1856	rBV	1039474	1469585	56.78%	5.556%
21	14.010	1856	1857	1862	rVV4	4441	5408	0.21%	0.020%
22	14.057	1862	1865	1869	rVB6	1589	2710	0.10%	0.010%
23	14.216	1884	1892	1908	rBV2	1122391	1652365	63.84%	6.247%
24	14.393	1919	1922	1928	rVB8	1812	3067	0.12%	0.012%
25	14.516	1936	1943	1953	rBV	612867	932904	36.04%	3.527%
26	14.775	1981	1987	2005	rBV	217530	568533	21.97%	2.149%
27	15.516	2103	2113	2121	rBV	1402827	2012599	77.76%	7.609%
28	15.669	2133	2139	2151	rBV	464830	686248	26.51%	2.594%
29	15.751	2151	2153	2159	rVB6	7620	10653	0.41%	0.040%
30	16.098	2210	2212	2218	rVB7	2123	2943	0.11%	0.011%
31	16.304	2243	2247	2251	rVB7	2439	4625	0.18%	0.017%
32	16.957	2355	2358	2364	rVB7	2879	4471	0.17%	0.017%
33	17.081	2376	2379	2383	rBV6	2377	3480	0.13%	0.013%
34	17.292	2404	2415	2424	rBV	818334	1161091	44.86%	4.390%
35	17.392	2425	2432	2449	rVV	1546146	2223617	85.91%	8.407%
36	17.504	2449	2451	2454	rVB4	3212	3611	0.14%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017947.D
Acq On : 08 Nov 2023 04:28
Operator : MA/JU
Sample : PB156698BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK698

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Title : SVOA CALIBRATION

37	18.157	2558	2562	2564	rBV5	2877	3826	0.15%	0.014%
38	18.733	2658	2660	2664	rBV5	2230	2916	0.11%	0.011%
39	19.210	2737	2741	2746	rBV	20403	27780	1.07%	0.105%
40	19.286	2750	2754	2757	rVV	15410	19408	0.75%	0.073%
41	19.639	2808	2814	2823	rBV	1941677	2507579	96.89%	9.480%
42	21.410	3110	3115	3126	rBV	844768	1176174	45.44%	4.447%
43	23.727	3500	3509	3527	rVB2	1211088	2588179	100.00%	9.785%
44	23.892	3530	3537	3545	rVB	551480	1166360	45.06%	4.410%




Sum of corrected areas: 26450313

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017947.D
Acq On : 08 Nov 2023 04:28
Operator : MA/JU
Sample : PB156698BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK698

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

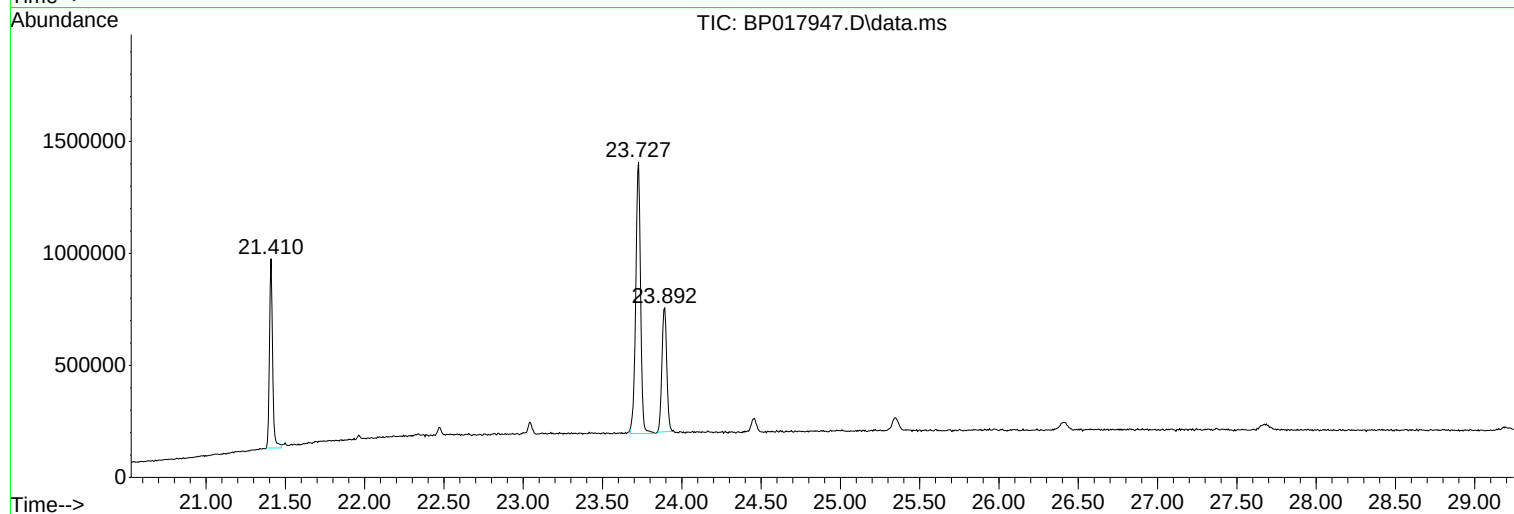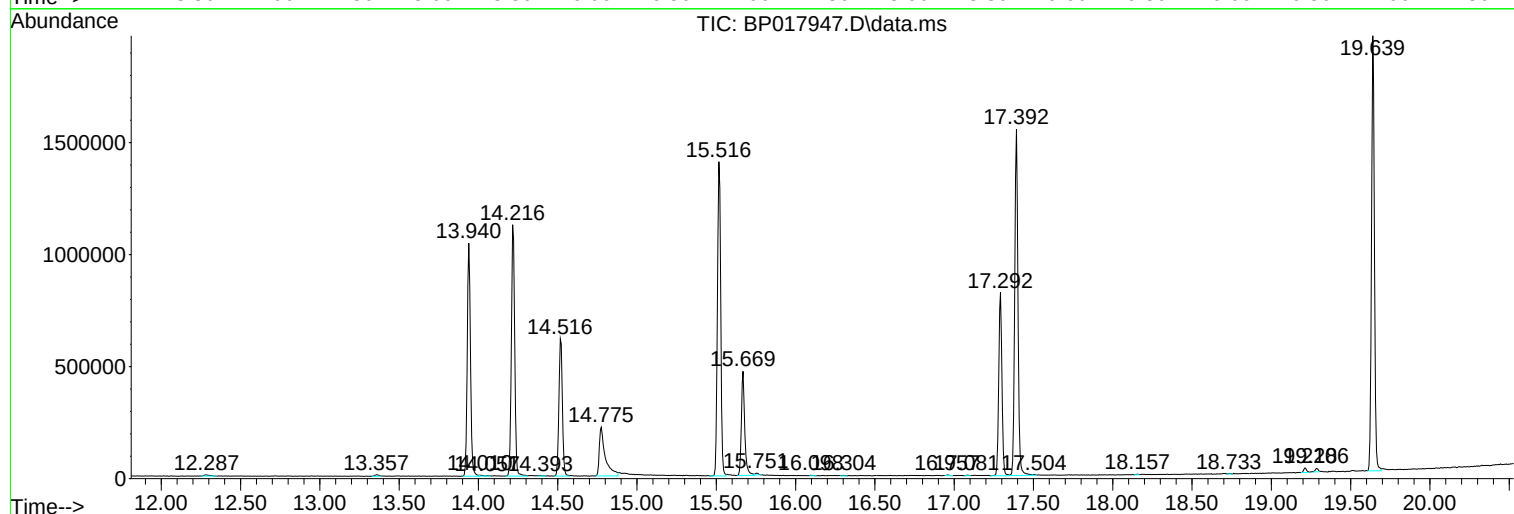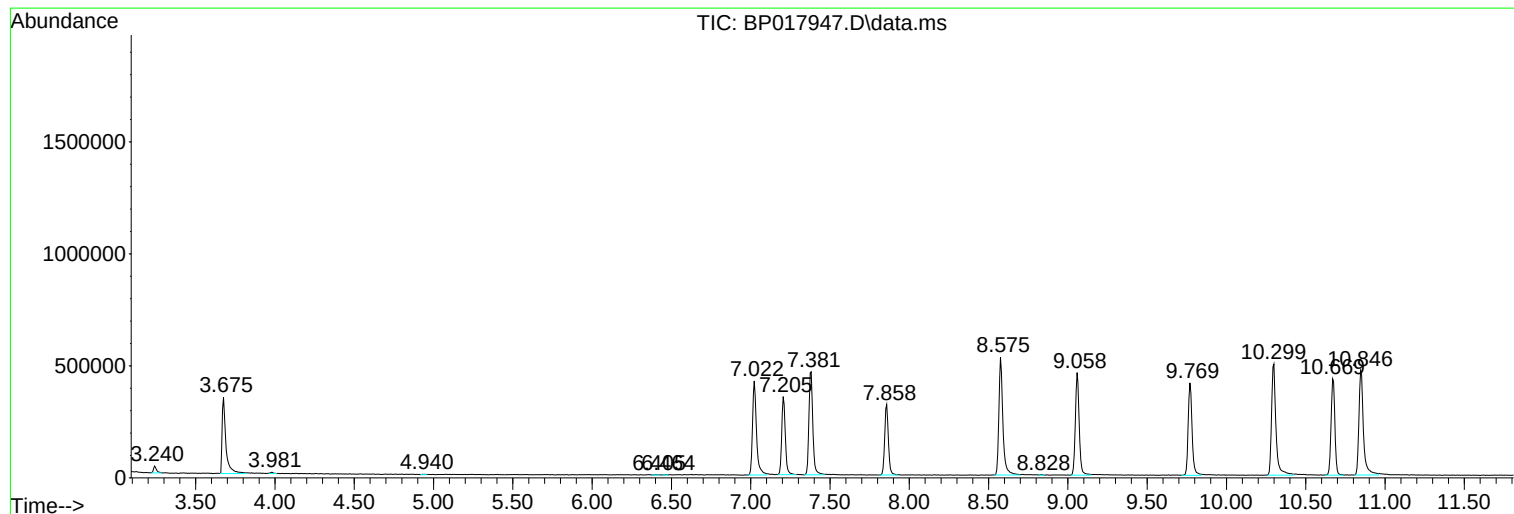

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017947.D
Acq On : 08 Nov 2023 04:28
Operator : MA/JU
Sample : PB156698BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK698

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017947.D
Acq On : 08 Nov 2023 04:28
Operator : MA/JU
Sample : PB156698BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK698

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc