

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
 Data File : BP017953.D
 Acq On : 08 Nov 2023 07:51
 Operator : MA/JU
 Sample : 05026-19
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH346

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017953.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	23	26	30	rBV	15096	21660	0.66%	0.078%
2	3.281	31	33	37	rVB3	7024	6981	0.21%	0.025%
3	3.499	68	70	77	rBV8	2002	3606	0.11%	0.013%
4	3.687	99	102	113	rBV	44166	82924	2.51%	0.297%
5	3.858	127	131	134	rBV3	6838	8607	0.26%	0.031%
6	3.975	148	151	155	rVB3	6630	7125	0.22%	0.026%
7	4.534	244	246	251	rBV5	2150	3379	0.10%	0.012%
8	5.705	441	445	448	rBV5	2407	3363	0.10%	0.012%
9	7.028	664	670	683	rBV	77437	157035	4.76%	0.563%
10	7.205	694	700	716	rBV	344036	545960	16.55%	1.956%
11	7.381	721	730	743	rBV	350703	602130	18.25%	2.157%
12	7.858	804	811	822	rBV	325342	536010	16.25%	1.920%
13	8.575	925	933	948	rBV	253947	483721	14.66%	1.733%
14	9.057	1008	1015	1031	rBV	464988	795747	24.12%	2.851%
15	9.769	1129	1136	1152	rBV	399289	697384	21.14%	2.499%
16	10.299	1219	1226	1247	rBV	464400	916584	27.78%	3.284%
17	10.669	1282	1289	1301	rBV	459935	760837	23.06%	2.726%
18	10.851	1311	1320	1337	rBV	326889	678839	20.58%	2.432%
19	11.946	1503	1506	1512	rBV8	1963	4913	0.15%	0.018%
20	12.275	1557	1562	1568	rBV6	6675	15375	0.47%	0.055%
21	12.375	1573	1579	1581	rBV7	2542	4202	0.13%	0.015%
22	13.357	1740	1746	1753	rBV2	8853	15517	0.47%	0.056%
23	13.498	1763	1770	1774	rVB9	2241	4771	0.14%	0.017%
24	13.940	1838	1845	1862	rBV	1207745	1671770	50.67%	5.990%
25	14.216	1885	1892	1902	rBV	1254758	1815092	55.02%	6.503%
26	14.363	1912	1917	1921	rVB8	1750	4164	0.13%	0.015%
27	14.516	1937	1943	1951	rBV	681003	1018479	30.87%	3.649%
28	14.604	1954	1958	1959	rBV4	6653	8129	0.25%	0.029%
29	14.798	1985	1991	2002	rBV5	30743	96957	2.94%	0.347%
30	15.263	2064	2070	2075	rBV4	7228	13167	0.40%	0.047%
31	15.339	2079	2083	2088	rVB	8554	11435	0.35%	0.041%
32	15.516	2106	2113	2122	rBV	1641989	2338214	70.87%	8.377%
33	15.669	2133	2139	2150	rBV	615800	920718	27.91%	3.299%
34	15.757	2151	2154	2163	rVB8	9558	17847	0.54%	0.064%
35	15.898	2170	2178	2184	rBV5	7183	14941	0.45%	0.054%
36	16.304	2242	2247	2250	rBV7	3198	5157	0.16%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
 Data File : BP017953.D
 Acq On : 08 Nov 2023 07:51
 Operator : MA/JU
 Sample : 05026-19
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH346

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
 Title : SVOA CALIBRATION

37	16.786	2325	2329	2335	rBV6	2805	6691	0.20%	0.024%
38	16.957	2353	2358	2359	rBV5	4039	4672	0.14%	0.017%
39	17.028	2367	2370	2375	rVB6	4539	6147	0.19%	0.022%
40	17.086	2376	2380	2384	rVB6	2469	4459	0.14%	0.016%
41	17.292	2408	2415	2425	rBV	900331	1265357	38.35%	4.534%
42	17.392	2425	2432	2451	rVB2	2060779	2857141	86.60%	10.237%
43	17.922	2518	2522	2527	rBV7	3476	5916	0.18%	0.021%
44	18.133	2551	2558	2568	rBV2	53353	87965	2.67%	0.315%
45	19.210	2737	2741	2746	rBV2	26155	35713	1.08%	0.128%
46	19.286	2750	2754	2758	rVB	27959	37718	1.14%	0.135%
47	19.380	2766	2770	2781	rBV3	33318	55738	1.69%	0.200%
48	19.516	2789	2793	2798	rBV3	24969	27678	0.84%	0.099%
49	19.645	2808	2815	2828	rBV	2451746	3299154	100.00%	11.820%
50	20.539	2965	2967	2970	rBV3	20541	20383	0.62%	0.073%
51	21.410	3110	3115	3125	rBV	1009554	1330143	40.32%	4.766%
52	23.727	3501	3509	3517	rVB	1654195	3250950	98.54%	11.648%
53	23.892	3530	3537	3546	rVB	652052	1322372	40.08%	4.738%




Sum of corrected areas: 27910937

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017953.D
Acq On : 08 Nov 2023 07:51
Operator : MA/JU
Sample : 05026-19
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH346

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

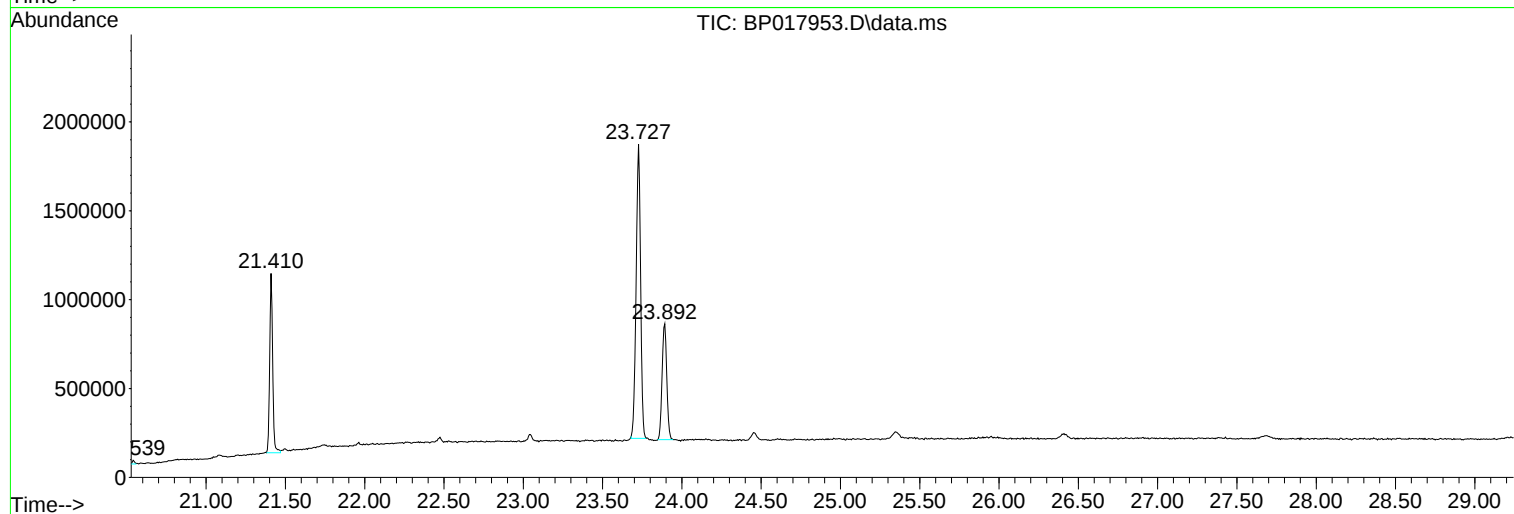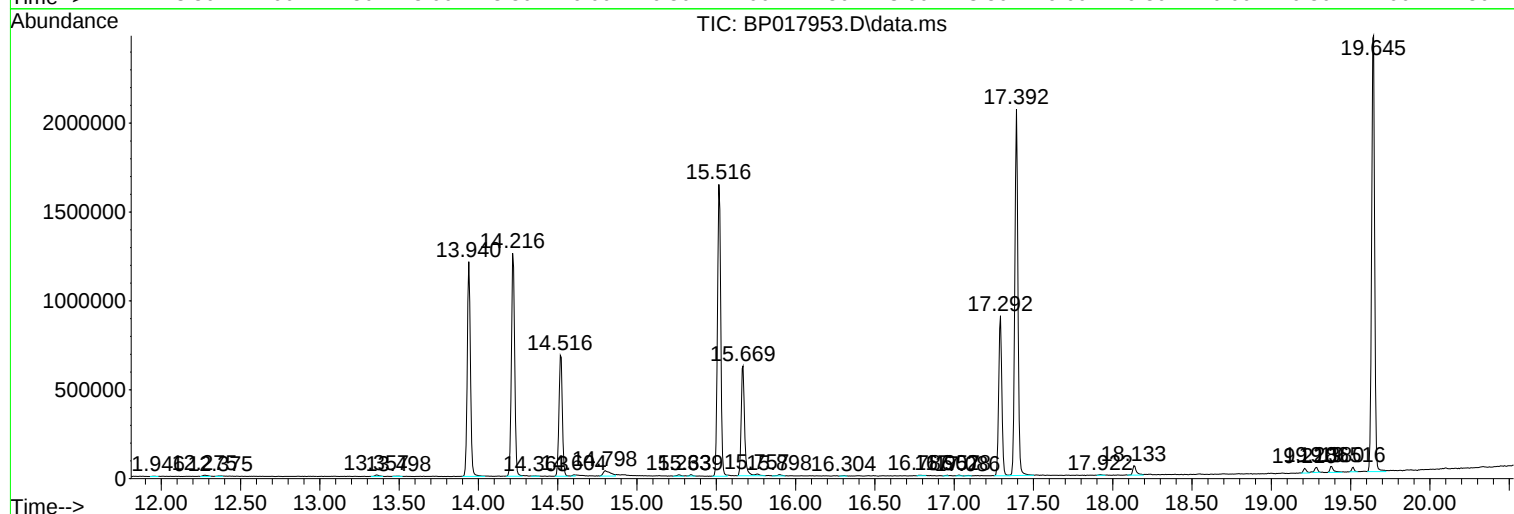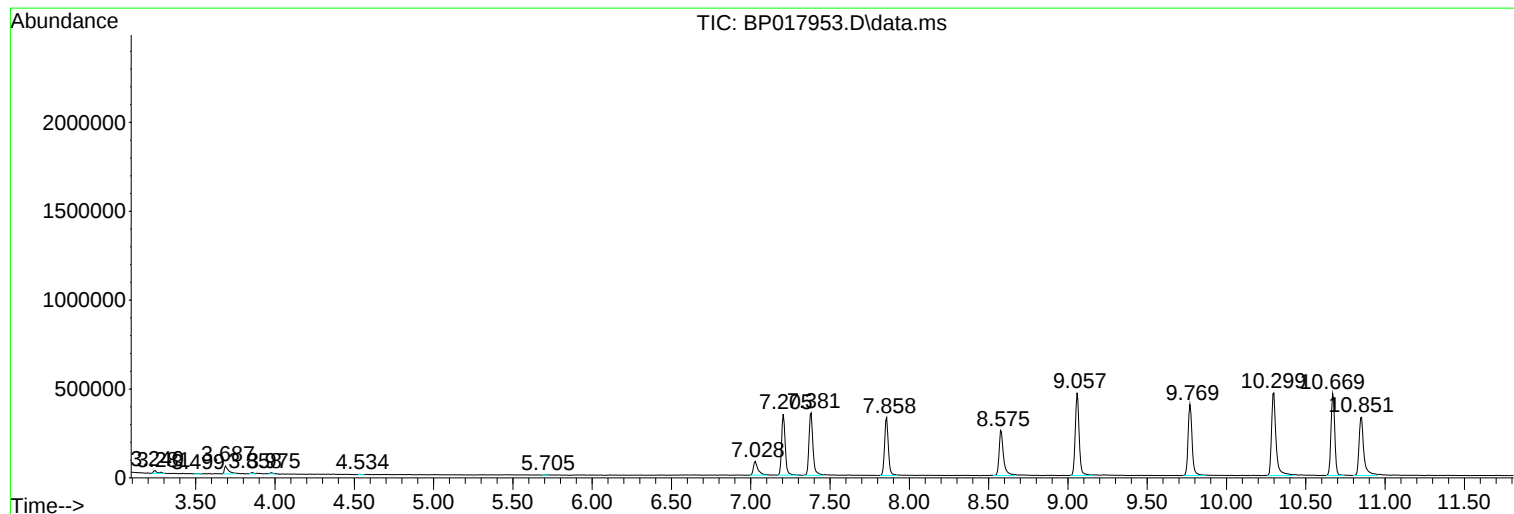

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017953.D
Acq On : 08 Nov 2023 07:51
Operator : MA/JU
Sample : 05026-19
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH346

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017953.D
Acq On : 08 Nov 2023 07:51
Operator : MA/JU
Sample : 05026-19
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH346

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------