

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
 Data File : BP017957.D
 Acq On : 08 Nov 2023 10:07
 Operator : MA/JU
 Sample : 05168-04
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 XA015

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017957.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	13	15	21	rVB	15191	19218	0.20%	0.019%
2	3.240	23	26	33	rVB	27133	37534	0.39%	0.038%
3	3.628	87	92	97	rBV	578831	742614	7.67%	0.748%
4	3.675	97	100	114	rVV	301095	489486	5.05%	0.493%
5	3.775	114	117	122	rVB3	10527	14076	0.15%	0.014%
6	3.975	147	151	159	rVB	16937	27350	0.28%	0.028%
7	4.181	183	186	188	rBV3	7987	10537	0.11%	0.011%
8	4.846	296	299	306	rVB	13123	21580	0.22%	0.022%
9	5.240	360	366	373	rBV	35487	49399	0.51%	0.050%
10	5.463	396	404	409	rBV6	7409	16642	0.17%	0.017%
11	7.022	662	669	686	rBV	417487	719389	7.43%	0.724%
12	7.205	693	700	707	rBV	340077	510656	5.27%	0.514%
13	7.299	709	716	724	rBV	1110215	1589788	16.41%	1.600%
14	7.381	724	730	739	rVB	440337	705232	7.28%	0.710%
15	7.852	803	810	813	rBV	324759	533063	5.50%	0.537%
16	7.893	813	817	827	rVB	1042708	1607289	16.59%	1.618%
17	8.199	862	869	878	rBV	520876	846837	8.74%	0.852%
18	8.369	890	898	899	rBV	963948	1396672	14.42%	1.406%
19	8.387	899	901	906	rVV	1004252	1289360	13.31%	1.298%
20	8.434	906	909	922	rVB	39460	64424	0.67%	0.065%
21	8.575	926	933	958	rBV	500455	905266	9.34%	0.911%
22	9.057	1008	1015	1019	rBV	441723	731234	7.55%	0.736%
23	9.099	1019	1022	1034	rVB	304205	512891	5.29%	0.516%
24	9.604	1101	1108	1122	rBV	472196	762357	7.87%	0.767%
25	9.769	1129	1136	1150	rBV	391936	667792	6.89%	0.672%
26	9.940	1159	1165	1169	rVB	9623	15519	0.16%	0.016%
27	10.098	1185	1192	1204	rBV	1113327	1669961	17.24%	1.681%
28	10.293	1217	1225	1245	rBV	494489	953164	9.84%	0.959%
29	10.669	1282	1289	1301	rVB	430269	717496	7.41%	0.722%
30	10.846	1312	1319	1346	rBV	455364	920691	9.50%	0.927%
31	12.257	1550	1559	1565	rBV3	11751	28692	0.30%	0.029%
32	12.334	1565	1572	1584	rBV	1599021	2457933	25.37%	2.474%
33	12.463	1590	1594	1601	rVB5	6806	16183	0.17%	0.016%
34	12.557	1601	1610	1617	rBV	18362	35605	0.37%	0.036%
35	13.357	1740	1746	1750	rBV3	9189	13718	0.14%	0.014%
36	13.939	1838	1845	1849	rBV	1086797	1526877	15.76%	1.537%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
 Data File : BP017957.D
 Acq On : 08 Nov 2023 10:07
 Operator : MA/JU
 Sample : 05168-04
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 XA015

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
 Title : SVOA CALIBRATION

37	13.992	1849	1854	1871	rVB	4928742	6519158	67.29%	6.562%
38	14.216	1885	1892	1895	rBV	1113932	1705589	17.61%	1.717%
39	14.245	1895	1897	1906	rVB	648831	817623	8.44%	0.823%
40	14.516	1936	1943	1949	rBV	650311	964730	9.96%	0.971%
41	14.581	1949	1954	1965	rVB	1519567	2201736	22.73%	2.216%
42	14.775	1981	1987	2003	rBV	267739	651746	6.73%	0.656%
43	14.934	2010	2014	2018	rVB2	11420	18953	0.20%	0.019%
44	14.975	2018	2021	2033	rVB10	9191	20994	0.22%	0.021%
45	15.516	2106	2113	2118	rBV	1480554	2081281	21.48%	2.095%
46	15.575	2118	2123	2131	rVV	1758954	2455095	25.34%	2.471%
47	15.669	2133	2139	2151	rVV	508524	768949	7.94%	0.774%
48	15.757	2151	2154	2160	rVV6	12069	18342	0.19%	0.018%
49	15.822	2160	2165	2169	rVB2	25424	34760	0.36%	0.035%
50	16.169	2218	2224	2230	rBV8	9230	14637	0.15%	0.015%
51	16.469	2268	2275	2282	rBV	665463	903088	9.32%	0.909%
52	16.551	2282	2289	2297	rVB	1456265	2029341	20.95%	2.043%
53	17.110	2381	2384	2390	rVB3	8958	16059	0.17%	0.016%
54	17.292	2409	2415	2418	rBV	848712	1187649	12.26%	1.195%
55	17.333	2418	2422	2427	rVV	1754152	2406417	24.84%	2.422%
56	17.392	2427	2432	2435	rVV	1769978	2461032	25.40%	2.477%
57	17.428	2435	2438	2449	rVB	1867033	2426685	25.05%	2.443%
58	18.227	2569	2574	2579	rBV	5238154	5999726	61.93%	6.039%
59	19.210	2737	2741	2746	rBV3	23518	34006	0.35%	0.034%
60	19.280	2751	2753	2758	rVB2	18129	23154	0.24%	0.023%
61	19.551	2796	2799	2805	rVB	17354	23530	0.24%	0.024%
62	19.639	2808	2814	2817	rBV	2174393	2979477	30.76%	2.999%
63	19.669	2817	2819	2828	rVB	1369144	1639525	16.92%	1.650%
64	20.533	2962	2966	2971	rBV	4690112	5348340	55.21%	5.384%
65	21.274	3087	3092	3096	rBV	6728068	6767766	69.86%	6.812%
66	21.398	3107	3113	3124	rBV2	1316956	2778985	28.69%	2.797%
67	22.227	3248	3254	3264	rVB	7656938	9687574	100.00%	9.751%
68	23.121	3399	3406	3410	rBV	1076690	1910680	19.72%	1.923%
69	23.174	3410	3415	3422	rVB	1228587	2140122	22.09%	2.154%
70	23.727	3502	3509	3514	rBV2	1384400	2761849	28.51%	2.780%
71	23.780	3514	3518	3526	rVB	423099	807181	8.33%	0.813%
72	23.892	3530	3537	3548	rVB	613304	1284508	13.26%	1.293%
73	26.545	3978	3988	4005	rVB	879543	2828120	29.19%	2.847%




Sum of corrected areas: 99344932

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017957.D
Acq On : 08 Nov 2023 10:07
Operator : MA/JU
Sample : 05168-04
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
XA015

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

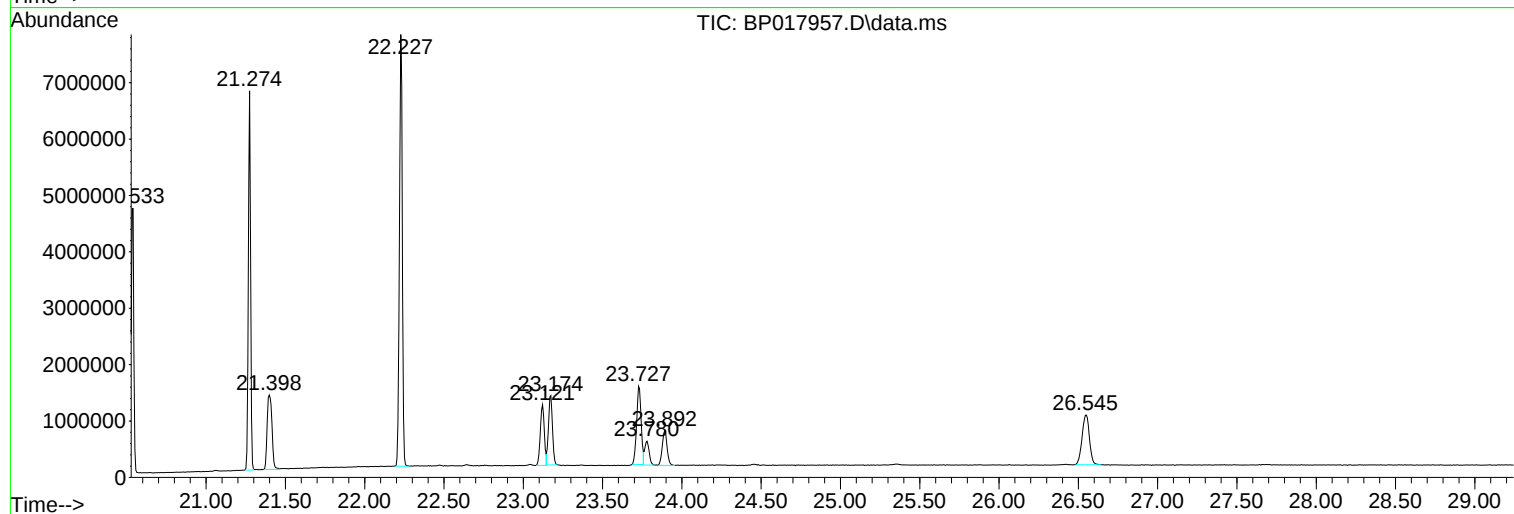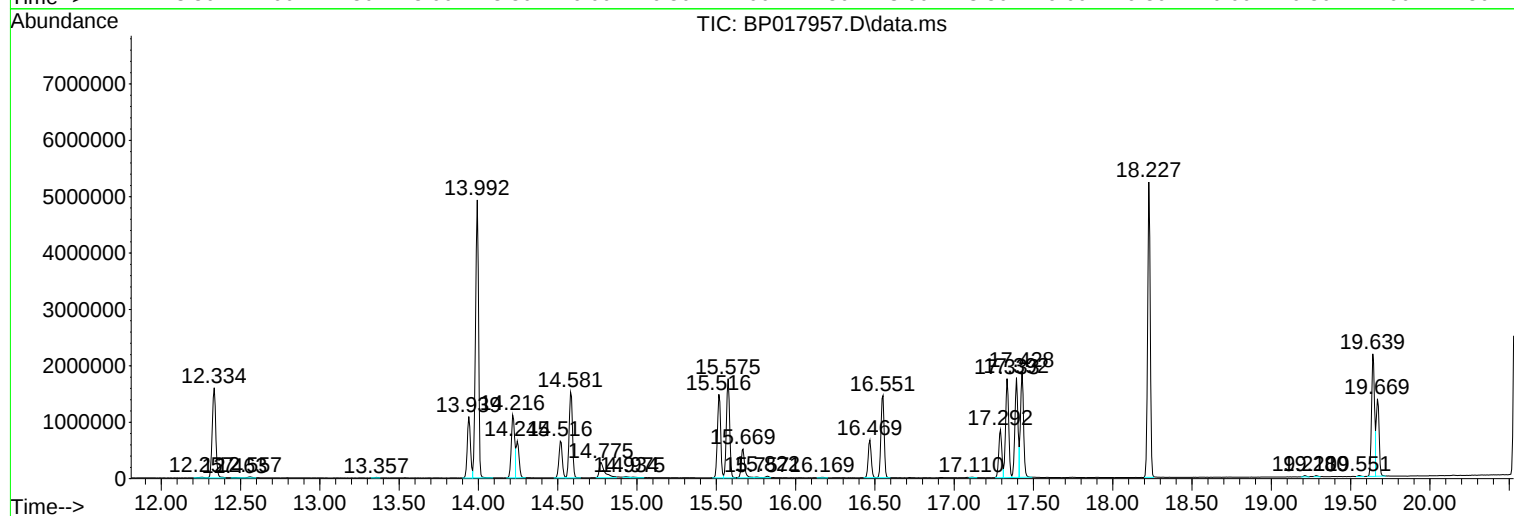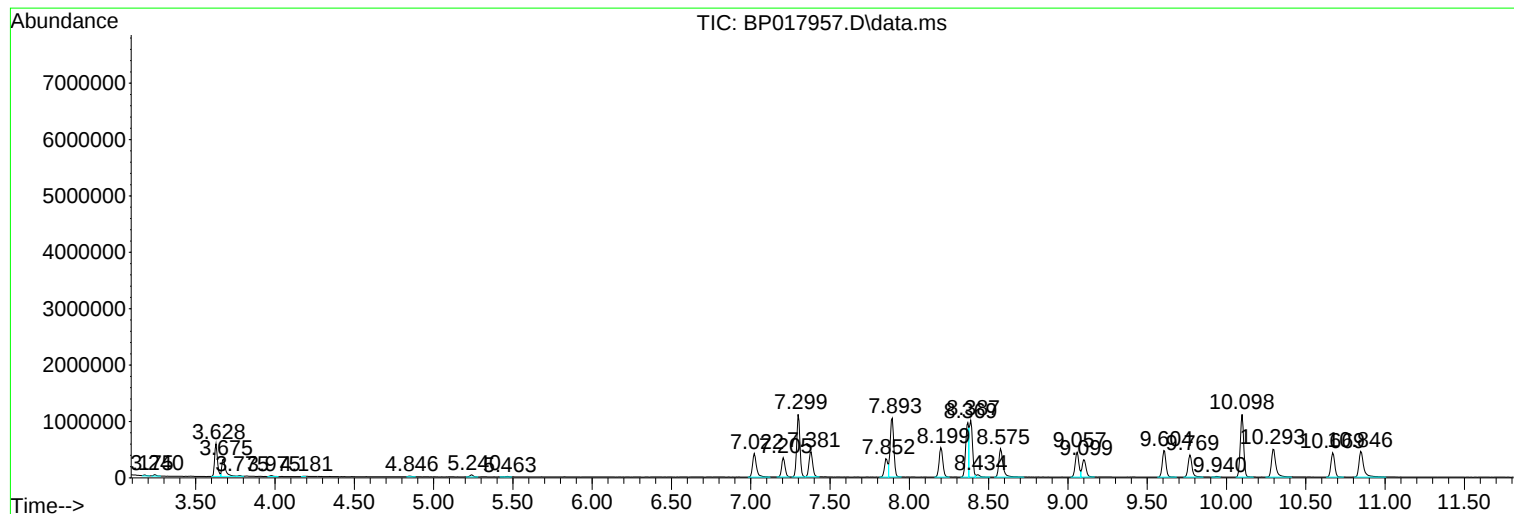

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017957.D
Acq On : 08 Nov 2023 10:07
Operator : MA/JU
Sample : 05168-04
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
XA015










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzene, 1,3-dichloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.199	31.77 ng/ul	846837	1,4-Dichlorobenzene-d4	7.852

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1,3-dichloro-	146	C6H4Cl2	000541-73-1	98
2			Benzene, 1,4-dichloro-	146	C6H4Cl2	000106-46-7	97
3			Benzene, 1,2-dichloro-	146	C6H4Cl2	000095-50-1	97
4			Benzene, 1,4-dichloro-	146	C6H4Cl2	000106-46-7	96
5			Benzene, 1,4-dichloro-	146	C6H4Cl2	000106-46-7	96

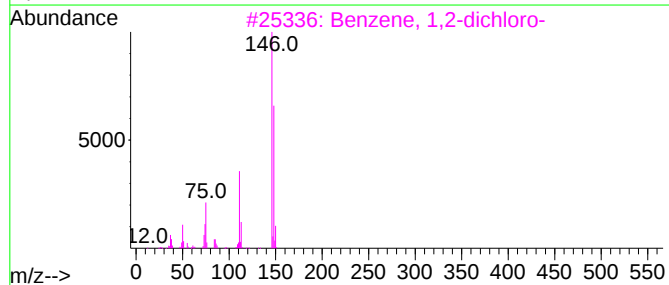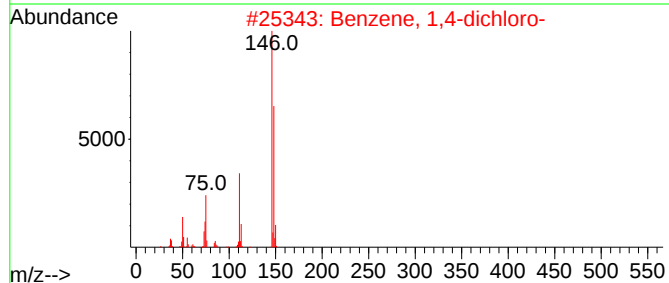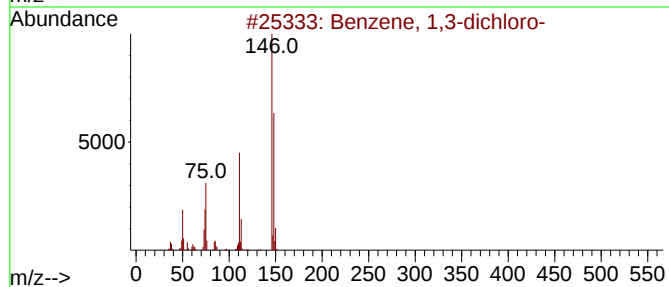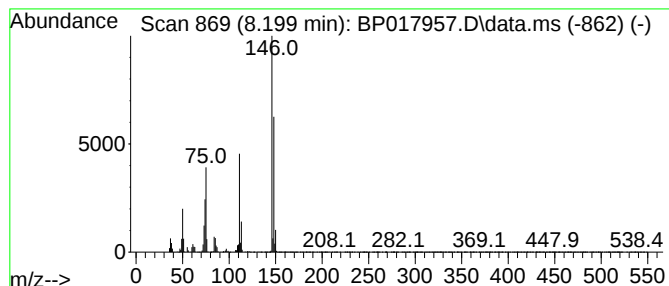

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017957.D
Acq On : 08 Nov 2023 10:07
Operator : MA/JU
Sample : 05168-04
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
XA015

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzene, 1,3-di...	8.199	31.8	ng/ul	846837	1	7.852	533063	20.0