

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
 Data File : BP017962.D
 Acq On : 08 Nov 2023 14:15
 Operator : MA/JU
 Sample : PB156829BL
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK829

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017962.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	23	26	33	rBV	23959	31981	1.51%	0.137%
2	3.676	97	100	119	rBV	265245	451866	21.28%	1.940%
3	3.976	147	151	158	rVB5	6184	10319	0.49%	0.044%
4	4.458	230	233	238	rBV7	2139	3569	0.17%	0.015%
5	4.564	246	251	252	rBV5	2298	3117	0.15%	0.013%
6	6.105	508	513	517	rVB8	1385	2414	0.11%	0.010%
7	7.022	661	669	684	rBV	305083	565214	26.62%	2.427%
8	7.205	694	700	713	rVB	264926	411417	19.37%	1.766%
9	7.375	723	729	742	rBV	355575	580967	27.36%	2.494%
10	7.852	803	810	825	rBV	355002	579346	27.28%	2.487%
11	8.575	926	933	953	rBV	378230	701650	33.04%	3.012%
12	9.058	1008	1015	1028	rBV	335901	585294	27.56%	2.513%
13	9.769	1129	1136	1147	rBV	299884	520462	24.51%	2.234%
14	10.293	1219	1225	1249	rBV	351642	730048	34.38%	3.134%
15	10.669	1281	1289	1304	rBV	495277	813617	38.32%	3.493%
16	10.846	1312	1319	1334	rBV	344622	707623	33.32%	3.038%
17	12.281	1558	1563	1570	rBV8	4090	10055	0.47%	0.043%
18	13.357	1738	1746	1753	rBV7	6245	12046	0.57%	0.052%
19	13.899	1833	1838	1839	rBV5	1589	2521	0.12%	0.011%
20	13.940	1839	1845	1855	rVV	811673	1174806	55.33%	5.044%
21	14.216	1884	1892	1906	rBV2	874703	1289307	60.72%	5.535%
22	14.516	1936	1943	1954	rBV	768292	1108027	52.18%	4.757%
23	14.775	1981	1987	2005	rBV	148212	429313	20.22%	1.843%
24	15.516	2105	2113	2124	rBV	1117062	1613223	75.97%	6.926%
25	15.669	2133	2139	2151	rBV	342774	531233	25.02%	2.281%
26	15.751	2151	2153	2160	rVB6	7586	12201	0.57%	0.052%
27	16.310	2244	2248	2252	rVB6	1814	2794	0.13%	0.012%
28	16.863	2339	2342	2344	rBV4	1690	2428	0.11%	0.010%
29	16.951	2355	2357	2361	rVB5	2568	2831	0.13%	0.012%
30	17.087	2376	2380	2384	rVB7	3467	4589	0.22%	0.020%
31	17.292	2408	2415	2425	rBV	988360	1371413	64.58%	5.888%
32	17.392	2425	2432	2445	rVV	1270188	1792876	84.43%	7.697%
33	17.922	2521	2522	2528	rVB6	1924	2504	0.12%	0.011%
34	18.151	2559	2561	2565	rBV5	1655	2185	0.10%	0.009%
35	18.281	2580	2583	2585	rBV4	2414	2720	0.13%	0.012%
36	18.834	2675	2677	2679	rBV3	2704	2252	0.11%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017962.D
Acq On : 08 Nov 2023 14:15
Operator : MA/JU
Sample : PB156829BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK829

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Title : SVOA CALIBRATION

37	19.216	2737	2742	2747	rBV2	16747	28204	1.33%	0.121%
38	19.286	2751	2754	2758	rVB2	13809	19441	0.92%	0.083%
39	19.381	2768	2770	2771	rBV2	3209	2468	0.12%	0.011%
40	19.639	2808	2814	2826	rBV	1631080	2123449	100.00%	9.116%
41	21.410	3110	3115	3128	rBV	1090760	1466753	69.07%	6.297%
42	23.727	3501	3509	3522	rVB2	1030578	2075780	97.76%	8.911%
43	23.892	3530	3537	3552	rVB	696310	1509058	71.07%	6.478%




Sum of corrected areas: 23293381

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017962.D
Acq On : 08 Nov 2023 14:15
Operator : MA/JU
Sample : PB156829BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK829

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

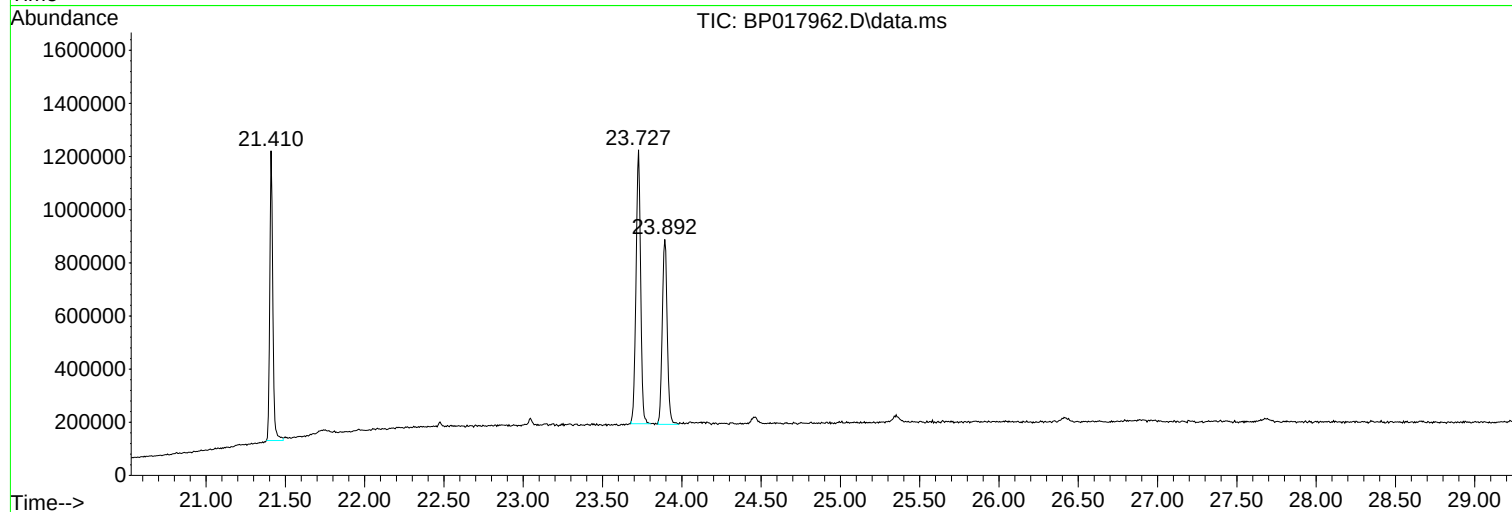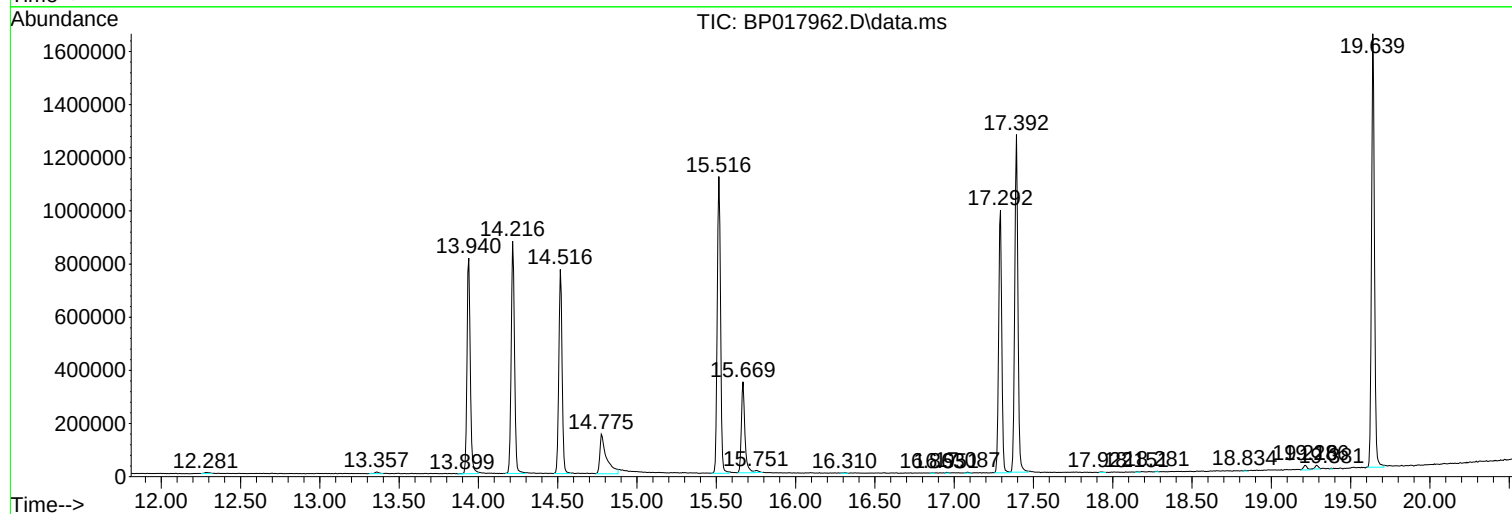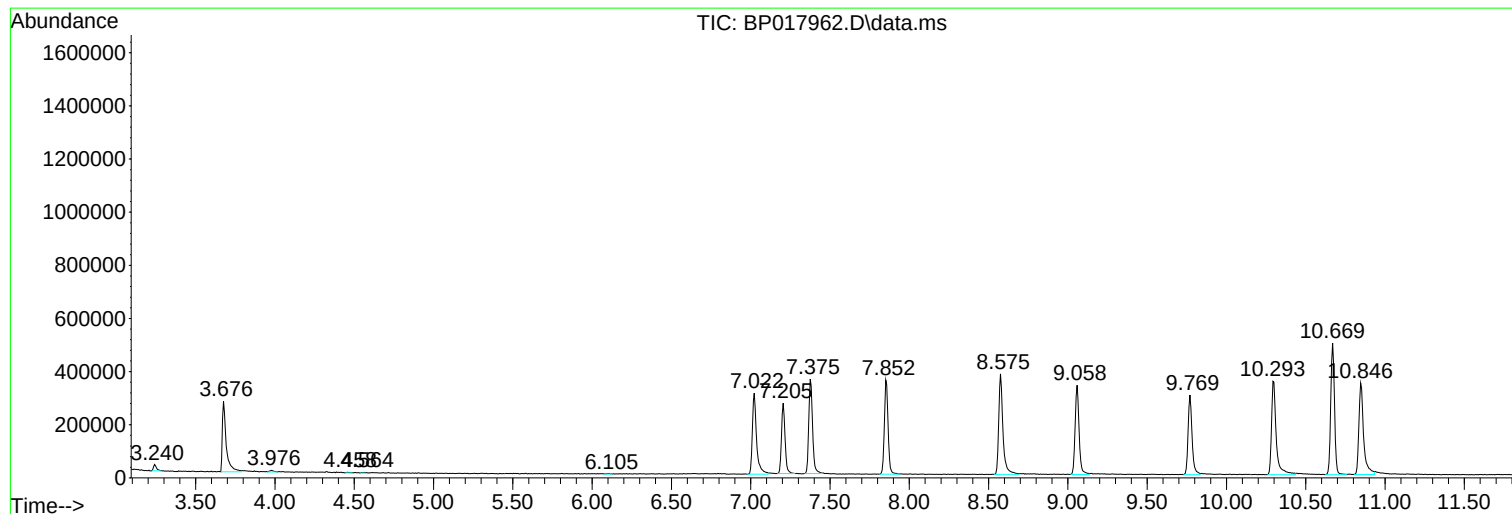

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017962.D
Acq On : 08 Nov 2023 14:15
Operator : MA/JU
Sample : PB156829BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK829

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017962.D
Acq On : 08 Nov 2023 14:15
Operator : MA/JU
Sample : PB156829BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK829

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------