

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
 Data File : BP017969.D
 Acq On : 08 Nov 2023 19:07
 Operator : MA/JU
 Sample : 05158-17
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH375

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017969.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	23	26	30	rBV	17587	21791	0.81%	0.095%
2	3.276	30	32	43	rVB3	14960	25062	0.93%	0.110%
3	3.681	98	101	117	rBV	106604	190511	7.06%	0.833%
4	3.858	127	131	135	rBV4	6513	9050	0.34%	0.040%
5	3.976	149	151	155	rVB4	4640	5263	0.20%	0.023%
6	5.923	475	482	488	rBV4	3477	7455	0.28%	0.033%
7	6.805	629	632	639	rBV9	1574	3471	0.13%	0.015%
8	7.028	664	670	683	rBV	66768	140699	5.22%	0.615%
9	7.205	693	700	711	rBV	296843	478150	17.73%	2.091%
10	7.375	723	729	744	rBV	304517	524491	19.45%	2.294%
11	7.852	802	810	823	rBV	276140	457397	16.96%	2.001%
12	8.375	897	899	903	rVB5	2311	3397	0.13%	0.015%
13	8.575	927	933	946	rBV	210372	407236	15.10%	1.781%
14	9.058	1008	1015	1024	rBV	379596	666421	24.71%	2.915%
15	9.234	1039	1045	1050	rVB2	14353	23242	0.86%	0.102%
16	9.769	1128	1136	1153	rBV	334960	590145	21.88%	2.581%
17	10.199	1203	1209	1211	rVB7	1759	2827	0.10%	0.012%
18	10.293	1218	1225	1245	rBV	380812	759152	28.15%	3.320%
19	10.669	1282	1289	1299	rBV	372361	615929	22.84%	2.694%
20	10.846	1311	1319	1338	rBV	360860	724718	26.87%	3.170%
21	12.275	1559	1562	1570	rBV9	4095	8827	0.33%	0.039%
22	13.357	1742	1746	1754	rBV5	8891	15370	0.57%	0.067%
23	13.481	1763	1767	1769	rBV4	2260	2767	0.10%	0.012%
24	13.940	1838	1845	1858	rBV	926025	1318588	48.89%	5.767%
25	14.216	1885	1892	1907	rBV	1008268	1455992	53.99%	6.368%
26	14.516	1935	1943	1953	rBV	568125	821153	30.45%	3.592%
27	14.804	1987	1992	1996	rBV4	17319	37990	1.41%	0.166%
28	15.516	2106	2113	2132	rBV	1295900	1863101	69.08%	8.149%
29	15.663	2132	2138	2150	rBV	430547	676141	25.07%	2.957%
30	15.757	2152	2154	2159	rVB6	8718	11435	0.42%	0.050%
31	16.304	2242	2247	2250	rBV7	3339	5229	0.19%	0.023%
32	16.851	2337	2340	2344	rVB6	2101	3652	0.14%	0.016%
33	17.287	2408	2414	2425	rBV	715694	1011818	37.52%	4.426%
34	17.392	2425	2432	2446	rVV	1512819	2218045	82.24%	9.702%
35	18.134	2553	2558	2568	rBV4	29964	55661	2.06%	0.243%
36	19.210	2737	2741	2745	rBV2	19167	25193	0.93%	0.110%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017969.D
Acq On : 08 Nov 2023 19:07
Operator : MA/JU
Sample : 05158-17
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH375

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Title : SVOA CALIBRATION

37	19.287	2750	2754	2758	rVB	17246	23496	0.87%	0.103%
38	19.381	2766	2770	2779	rBV	16560	31686	1.17%	0.139%
39	19.510	2790	2792	2798	rBV6	6658	7688	0.29%	0.034%
40	19.639	2808	2814	2823	rBV	2065022	2637739	97.80%	11.537%
41	21.410	3110	3115	3125	rBV	826835	1122175	41.61%	4.908%
42	23.727	3501	3509	3519	rVB2	1337617	2696950	100.00%	11.796%
43	23.886	3530	3536	3546	rVB	561909	1155672	42.85%	5.055%




Sum of corrected areas: 22862775

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017969.D
Acq On : 08 Nov 2023 19:07
Operator : MA/JU
Sample : 05158-17
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH375

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

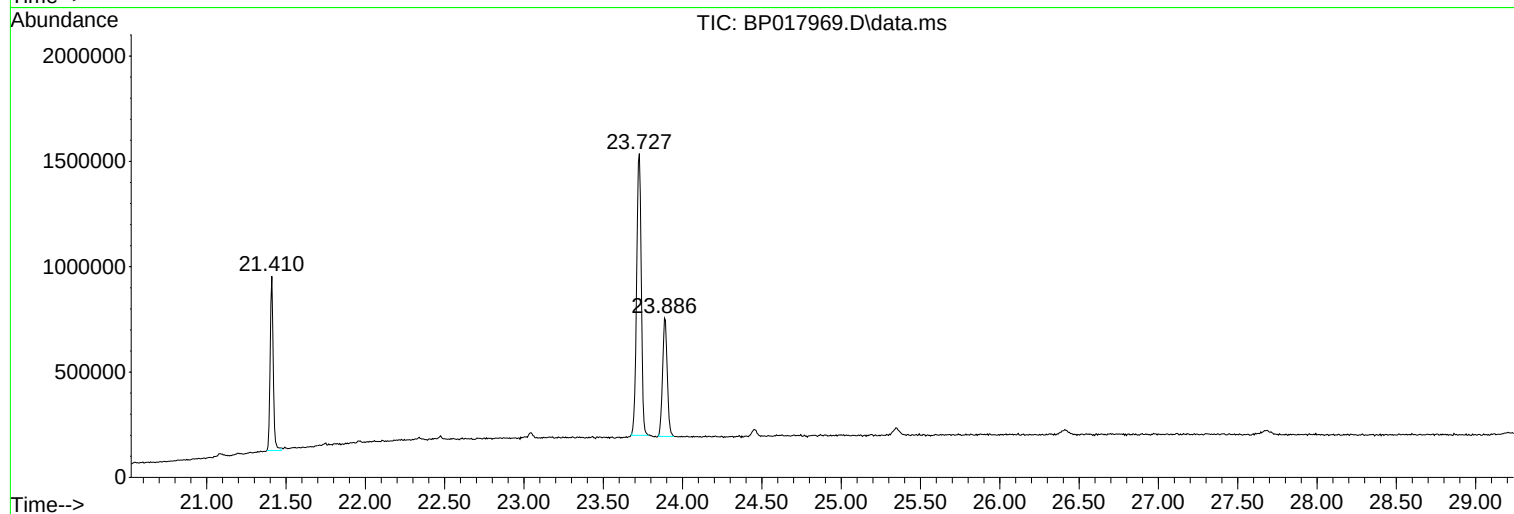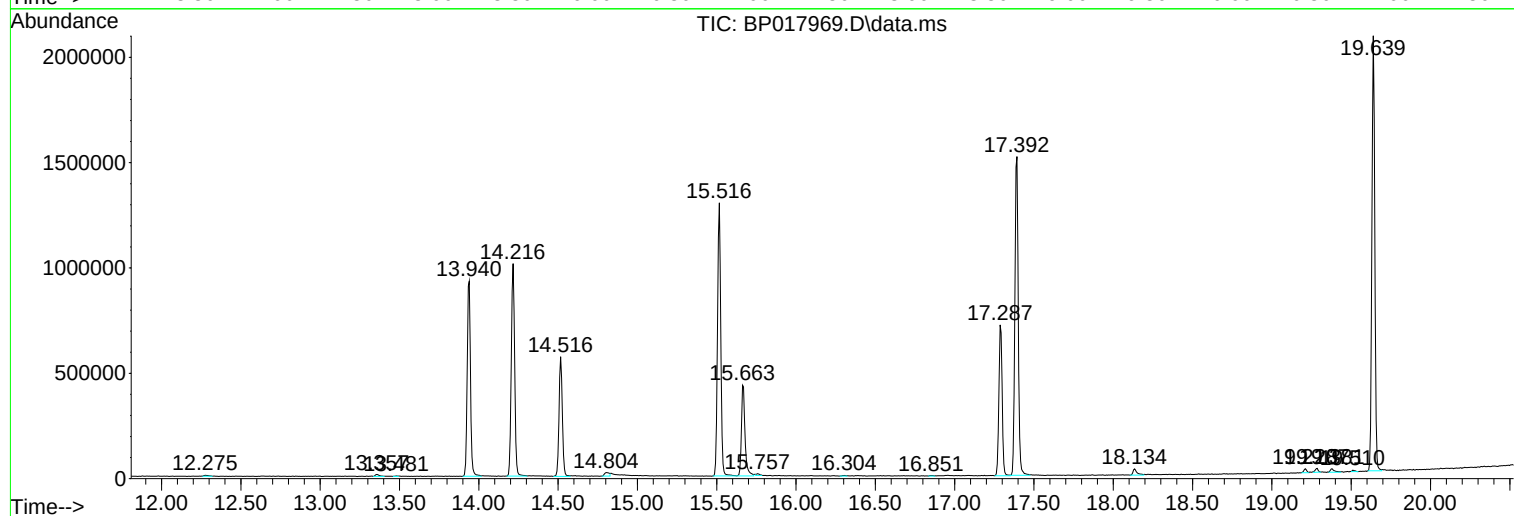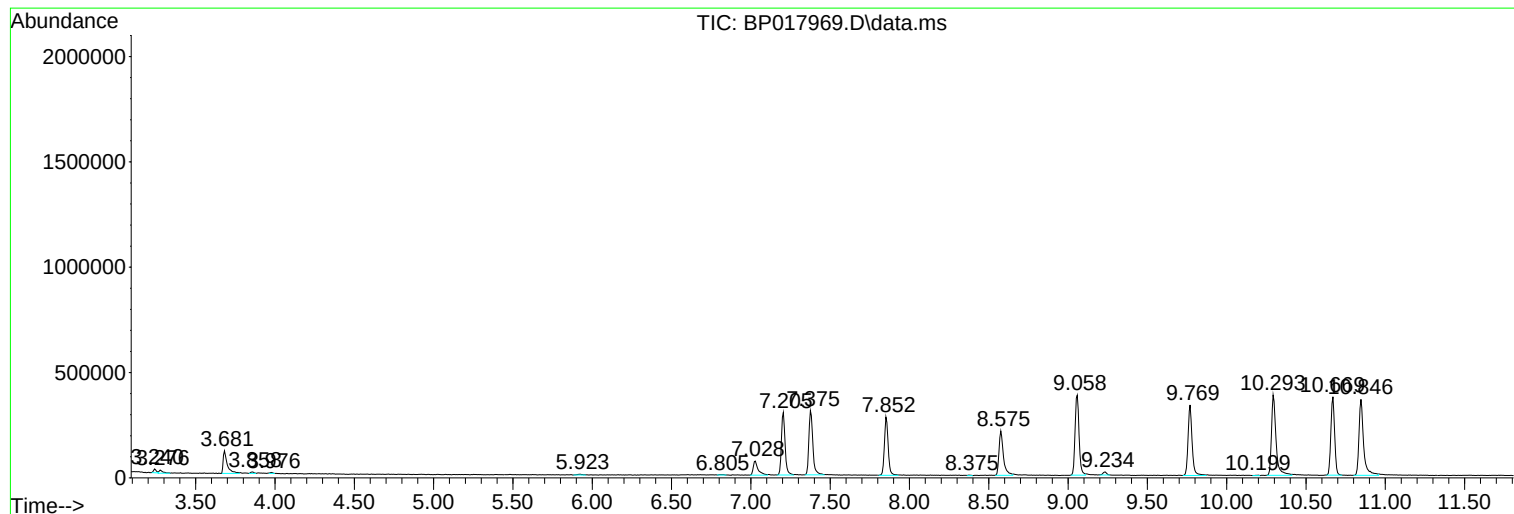

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017969.D
Acq On : 08 Nov 2023 19:07
Operator : MA/JU
Sample : 05158-17
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH375

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017969.D
Acq On : 08 Nov 2023 19:07
Operator : MA/JU
Sample : 05158-17
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH375

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------