

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
 Data File : BP017973.D
 Acq On : 08 Nov 2023 21:57
 Operator : MA/JU
 Sample : PB156653BL
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK653

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017973.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	23	26	31	rVB	24922	29750	1.32%	0.127%
2	3.675	96	100	115	rBV	269018	449275	20.00%	1.924%
3	3.975	147	151	157	rVB	15925	21916	0.98%	0.094%
4	6.675	609	610	615	rVB5	2477	2437	0.11%	0.010%
5	7.016	662	668	687	rBV	328058	611294	27.21%	2.617%
6	7.205	694	700	714	rVB	281052	447103	19.90%	1.914%
7	7.375	721	729	741	rBV	380751	637521	28.38%	2.730%
8	7.852	803	810	823	rBV	316996	513846	22.88%	2.200%
9	8.575	926	933	953	rBV	406726	762313	33.94%	3.264%
10	8.887	982	986	993	rVB9	1883	4159	0.19%	0.018%
11	9.058	1008	1015	1028	rBV	356311	623655	27.76%	2.670%
12	9.487	1084	1088	1090	rBV4	1432	2447	0.11%	0.010%
13	9.716	1124	1127	1129	rBV4	2178	2569	0.11%	0.011%
14	9.769	1129	1136	1149	rBV	308209	560617	24.96%	2.400%
15	10.293	1219	1225	1245	rBV	388027	769672	34.26%	3.296%
16	10.669	1280	1289	1298	rBV	423997	710053	31.61%	3.040%
17	10.846	1311	1319	1341	rBV	368900	760847	33.87%	3.258%
18	11.187	1375	1377	1383	rVB6	1726	2520	0.11%	0.011%
19	11.734	1467	1470	1474	rVB6	1630	2477	0.11%	0.011%
20	11.775	1474	1477	1480	rBV4	2269	2718	0.12%	0.012%
21	12.281	1558	1563	1572	rBV8	3856	9900	0.44%	0.042%
22	13.363	1742	1747	1751	rBV6	6006	10077	0.45%	0.043%
23	13.728	1806	1809	1814	rVB6	1712	3132	0.14%	0.013%
24	13.940	1837	1845	1861	rBV	848181	1246425	55.49%	5.337%
25	14.216	1883	1892	1906	rBV	926605	1360242	60.56%	5.824%
26	14.516	1936	1943	1952	rBV	653994	949012	42.25%	4.063%
27	14.775	1981	1987	2007	rBV	168790	479618	21.35%	2.054%
28	15.516	2104	2113	2121	rBV	1204683	1701925	75.77%	7.287%
29	15.663	2132	2138	2151	rBV	368295	579584	25.80%	2.482%
30	15.757	2151	2154	2161	rVB6	7910	12914	0.57%	0.055%
31	16.698	2310	2314	2319	rVB8	1632	2983	0.13%	0.013%
32	16.963	2355	2359	2363	rVB6	2125	2960	0.13%	0.013%
33	17.286	2408	2414	2425	rBV	846477	1185154	52.76%	5.075%
34	17.392	2425	2432	2449	rVB	1299197	1931779	86.00%	8.272%
35	17.634	2469	2473	2476	rVB5	2411	3040	0.14%	0.013%
36	17.728	2487	2489	2495	rVB7	2173	3748	0.17%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017973.D
Acq On : 08 Nov 2023 21:57
Operator : MA/JU
Sample : PB156653BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK653

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Title : SVOA CALIBRATION

37	17.922	2517	2522	2526	rBV8	2859	5243	0.23%	0.022%
38	18.157	2557	2562	2567	rBV8	2571	6612	0.29%	0.028%
39	18.322	2589	2590	2595	rVB4	2026	2767	0.12%	0.012%
40	18.933	2691	2694	2697	rBV5	2422	3669	0.16%	0.016%
41	19.210	2737	2741	2746	rBV2	16384	22413	1.00%	0.096%
42	19.281	2750	2753	2758	rVB2	12340	17608	0.78%	0.075%
43	19.639	2808	2814	2822	rBV	1793548	2246257	100.00%	9.618%
44	21.410	3110	3115	3127	rBV	886630	1254533	55.85%	5.372%
45	23.721	3501	3508	3517	rVB2	1093128	2130116	94.83%	9.121%
46	23.886	3529	3536	3550	rBV	591856	1265674	56.35%	5.419%




Sum of corrected areas: 23354574

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017973.D
Acq On : 08 Nov 2023 21:57
Operator : MA/JU
Sample : PB156653BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK653

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

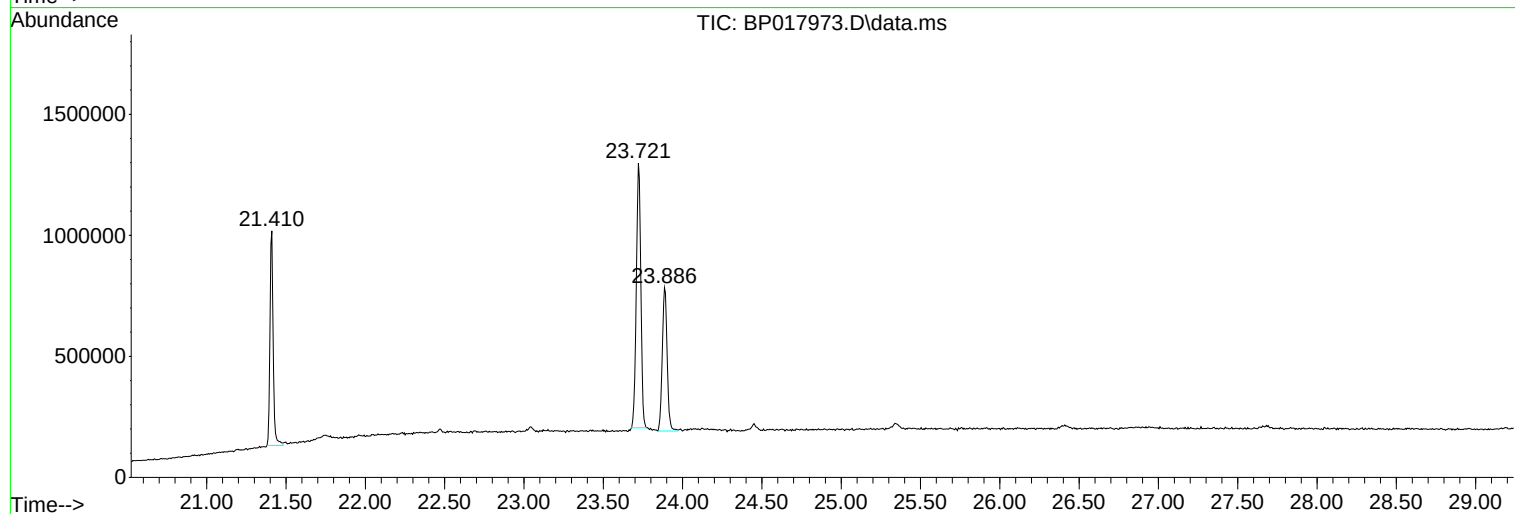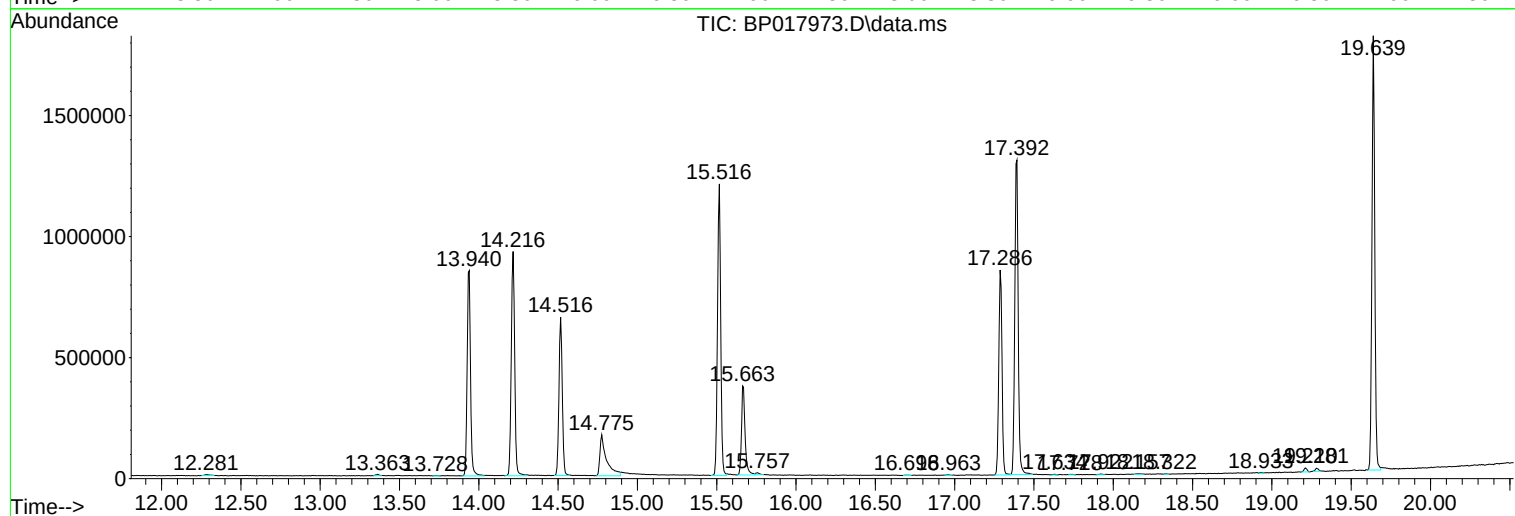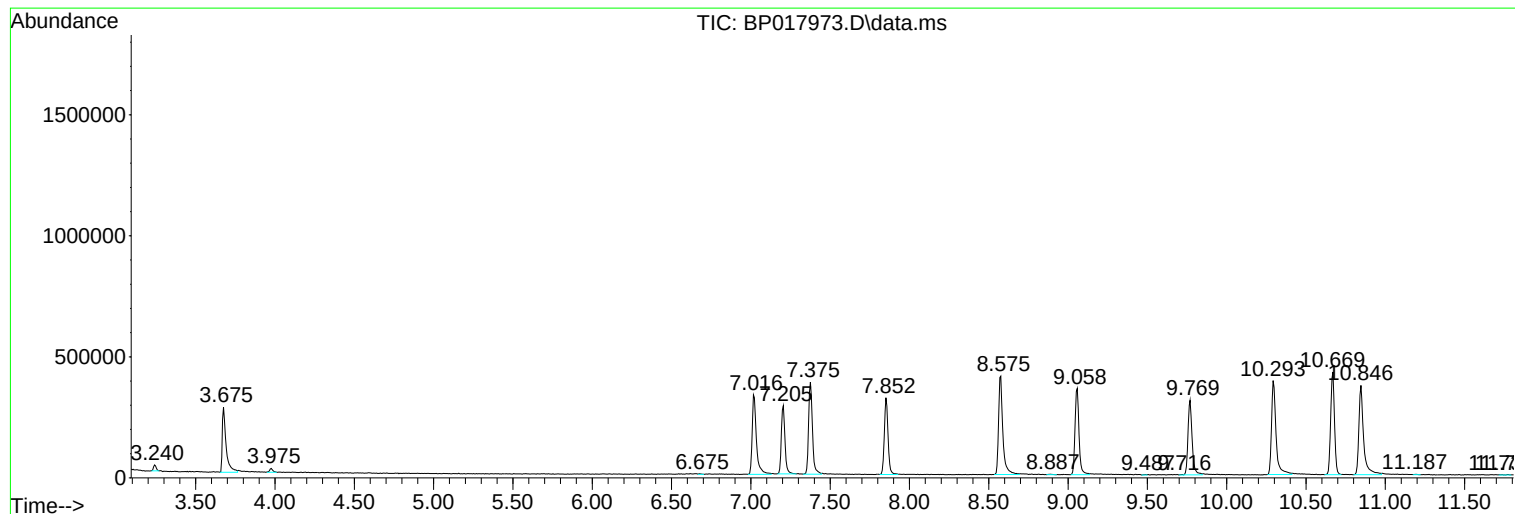

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017973.D
Acq On : 08 Nov 2023 21:57
Operator : MA/JU
Sample : PB156653BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK653

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017973.D
Acq On : 08 Nov 2023 21:57
Operator : MA/JU
Sample : PB156653BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK653

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc