

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
 Data File : BP017974.D
 Acq On : 08 Nov 2023 22:31
 Operator : MA/JU
 Sample : PB156654BL
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK654

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017974.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	22	27	34	rVB	24231	37241	1.75%	0.179%
2	3.675	97	100	117	rBV	255901	429580	20.13%	2.067%
3	3.975	147	151	158	rVB	12800	18880	0.88%	0.091%
4	7.016	661	668	684	rBV	309380	581775	27.26%	2.799%
5	7.205	694	700	711	rBV	256858	409488	19.19%	1.970%
6	7.375	723	729	741	rBV	367014	596794	27.96%	2.872%
7	7.728	786	789	791	rBV3	2067	2326	0.11%	0.011%
8	7.852	803	810	820	rBV	214899	352303	16.51%	1.695%
9	8.575	927	933	955	rBV	378094	719813	33.73%	3.464%
10	9.058	1006	1015	1028	rBV	335338	594708	27.87%	2.862%
11	9.769	1128	1136	1152	rBV	295445	538398	25.23%	2.591%
12	10.116	1192	1195	1198	rBV5	1571	2586	0.12%	0.012%
13	10.293	1217	1225	1247	rBV	370597	750509	35.17%	3.611%
14	10.669	1279	1289	1298	rBV	289169	487985	22.87%	2.348%
15	10.846	1310	1319	1339	rBV	357400	722101	33.84%	3.475%
16	12.163	1541	1543	1547	rBV5	1545	2251	0.11%	0.011%
17	12.275	1558	1562	1564	rBV5	3710	5253	0.25%	0.025%
18	12.675	1626	1630	1632	rBV5	1406	2194	0.10%	0.011%
19	13.363	1741	1747	1751	rBV6	4166	7654	0.36%	0.037%
20	13.934	1838	1844	1858	rBV	790575	1188864	55.71%	5.721%
21	14.216	1885	1892	1907	rBV	880700	1281335	60.04%	6.166%
22	14.516	1934	1943	1951	rBV	440757	651595	30.53%	3.135%
23	14.775	1981	1987	2018	rBV	156276	502179	23.53%	2.416%
24	15.516	2106	2113	2123	rBV	1119966	1606779	75.29%	7.732%
25	15.663	2133	2138	2150	rBV	364131	555451	26.03%	2.673%
26	15.757	2152	2154	2158	rVB5	6933	8310	0.39%	0.040%
27	16.098	2207	2212	2215	rVV7	1266	2263	0.11%	0.011%
28	16.392	2258	2262	2268	rBV8	1731	2388	0.11%	0.011%
29	16.951	2355	2357	2360	rVB4	2425	2368	0.11%	0.011%
30	17.075	2373	2378	2382	rBV8	3291	4708	0.22%	0.023%
31	17.287	2408	2414	2424	rBV	579471	816506	38.26%	3.929%
32	17.387	2425	2431	2450	rVB	1245612	1831643	85.83%	8.814%
33	17.922	2519	2522	2526	rVB5	2750	3568	0.17%	0.017%
34	18.157	2558	2562	2569	rBV10	3277	8458	0.40%	0.041%
35	19.210	2737	2741	2746	rBV5	17712	25771	1.21%	0.124%
36	19.281	2749	2753	2759	rBV2	13846	24573	1.15%	0.118%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017974.D
Acq On : 08 Nov 2023 22:31
Operator : MA/JU
Sample : PB156654BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK654

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Title : SVOA CALIBRATION

37	19.639	2808	2814	2823	rBV	1623628	2121435	99.41%	10.208%
38	21.410	3110	3115	3127	rBV	616732	865022	40.53%	4.162%
39	23.721	3501	3508	3525	rVB2	1012452	2134093	100.00%	10.269%
40	23.886	3530	3536	3550	rVB	420045	882513	41.35%	4.247%




Sum of corrected areas: 20781661

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017974.D
Acq On : 08 Nov 2023 22:31
Operator : MA/JU
Sample : PB156654BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK654

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

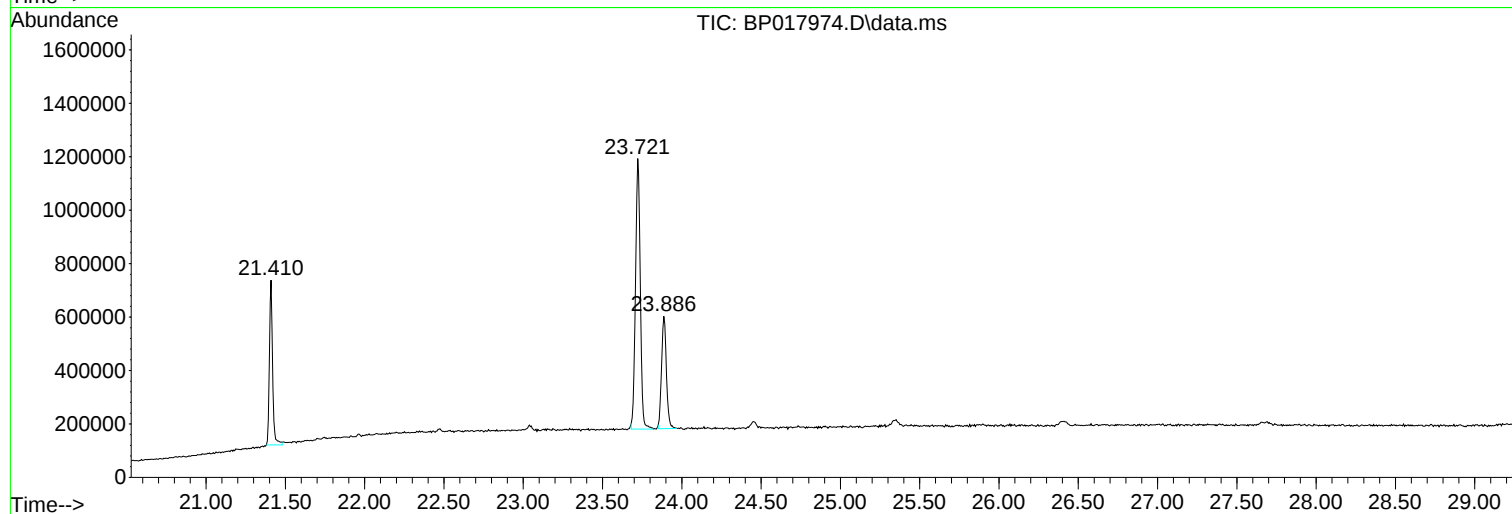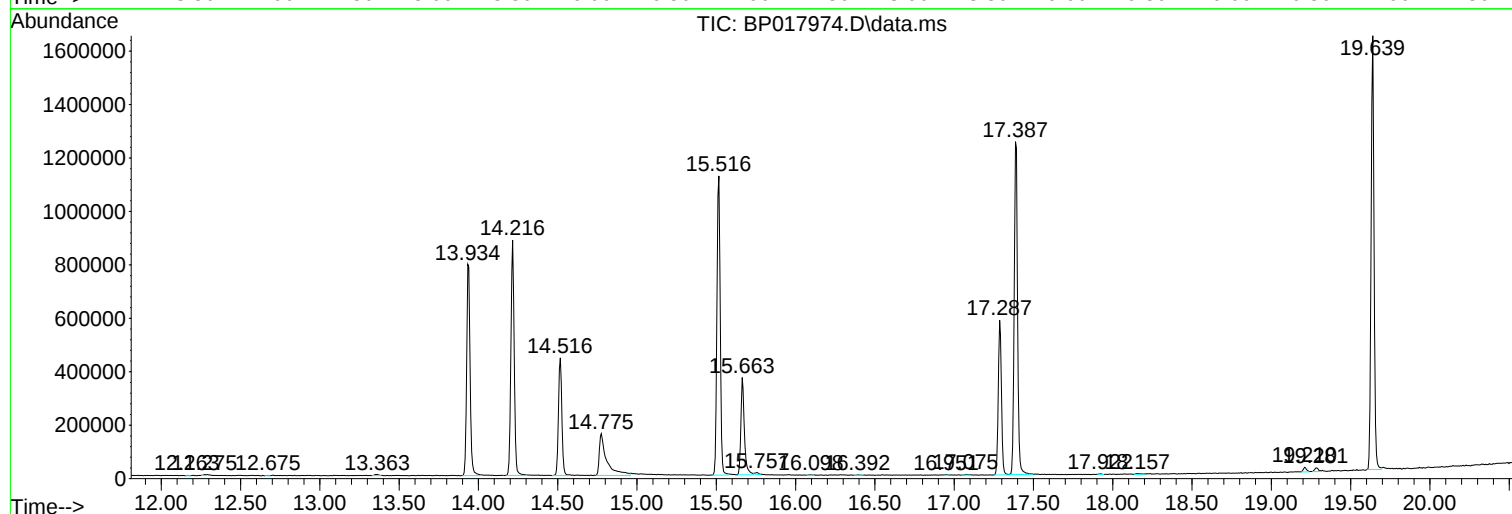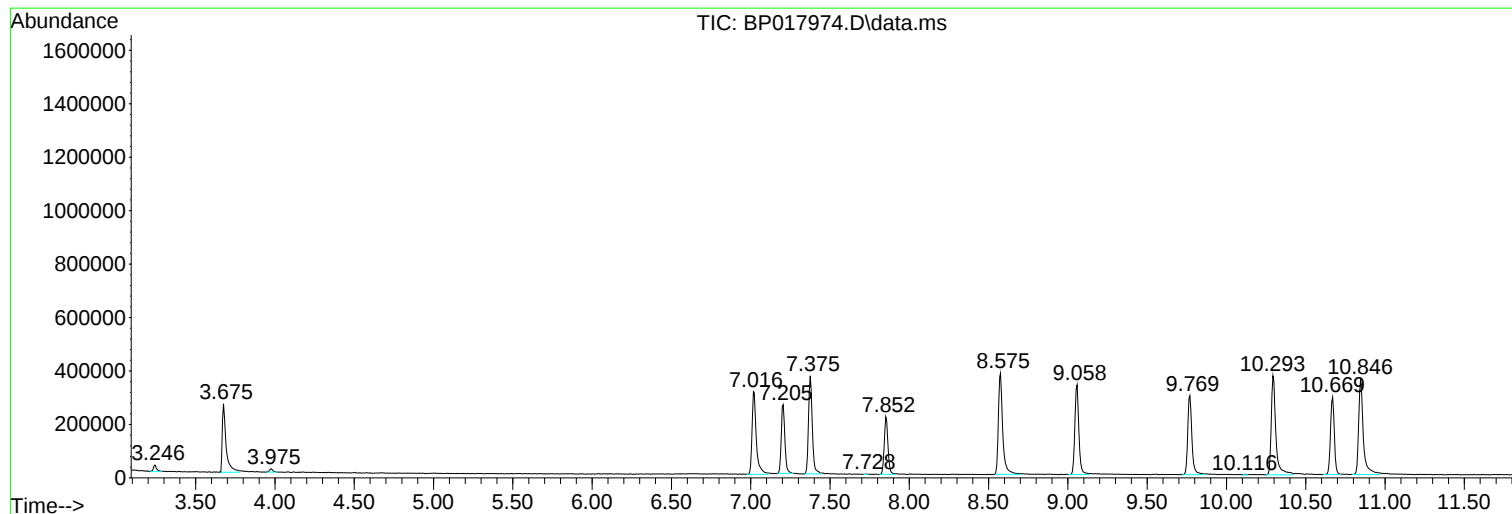

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017974.D
Acq On : 08 Nov 2023 22:31
Operator : MA/JU
Sample : PB156654BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK654

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110723\
Data File : BP017974.D
Acq On : 08 Nov 2023 22:31
Operator : MA/JU
Sample : PB156654BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK654

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------