
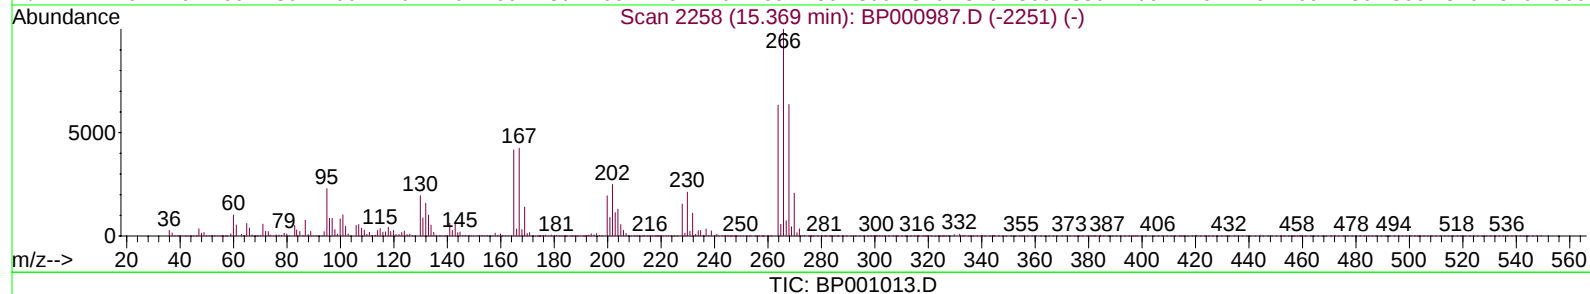
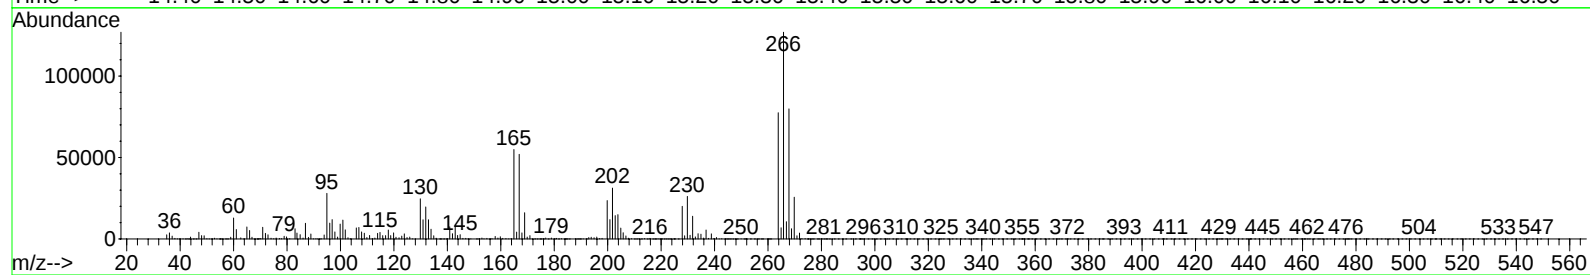


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP110819\
Data File : BP001013.D
Acq On : 08 Nov 2019 13:34
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 08 18:11:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP110619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 06 17:07:13 2019
Response via : Initial Calibration

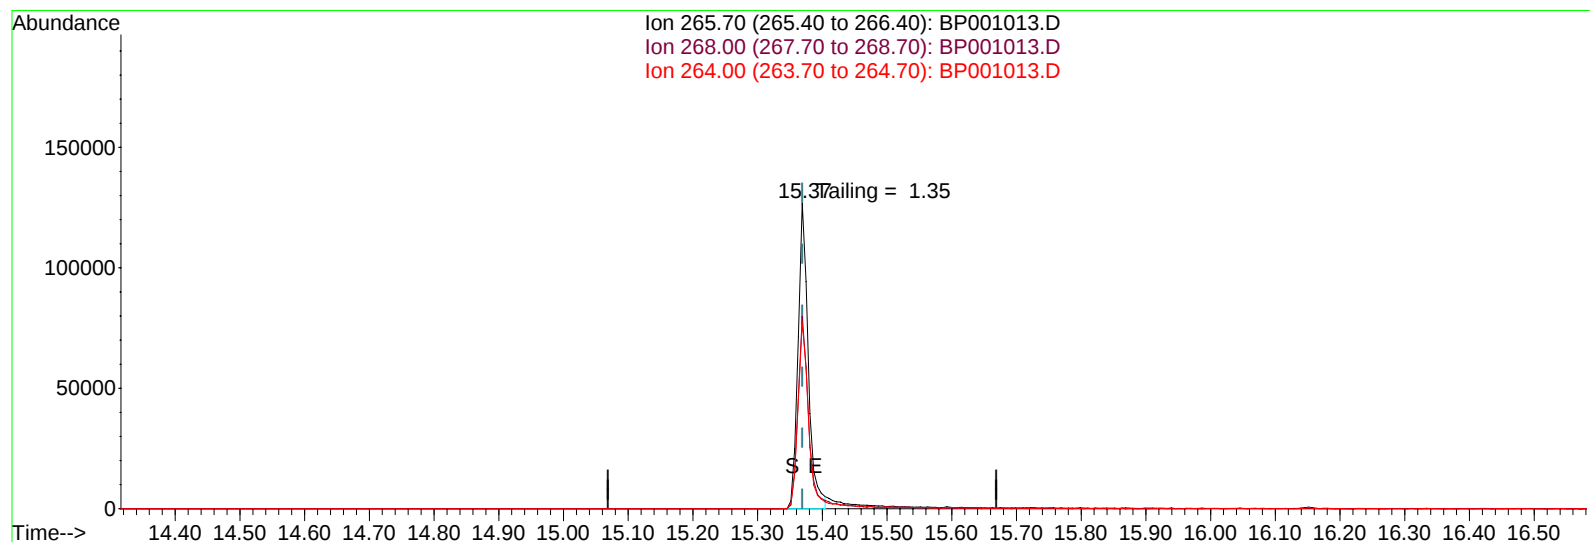

(70) Pentachlorophenol (C)




15.369min (-0.000) 1591709.79ng

response 154653

Ion	Exp%	Act%
265.70	100	100
268.00	63.60	62.96
264.00	63.30	61.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP110819\
Data File : BP001013.D
Acq On : 08 Nov 2019 13:34
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 08 18:11:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP110619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 06 17:07:13 2019
Response via : Initial Calibration

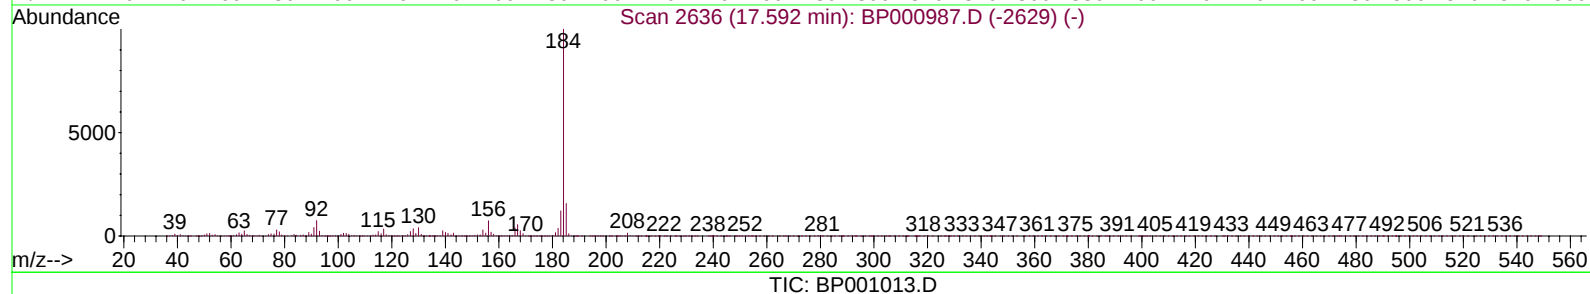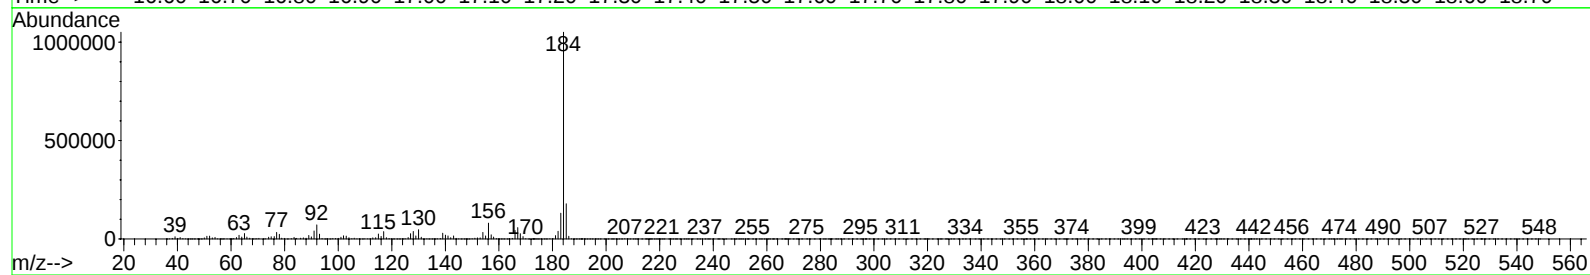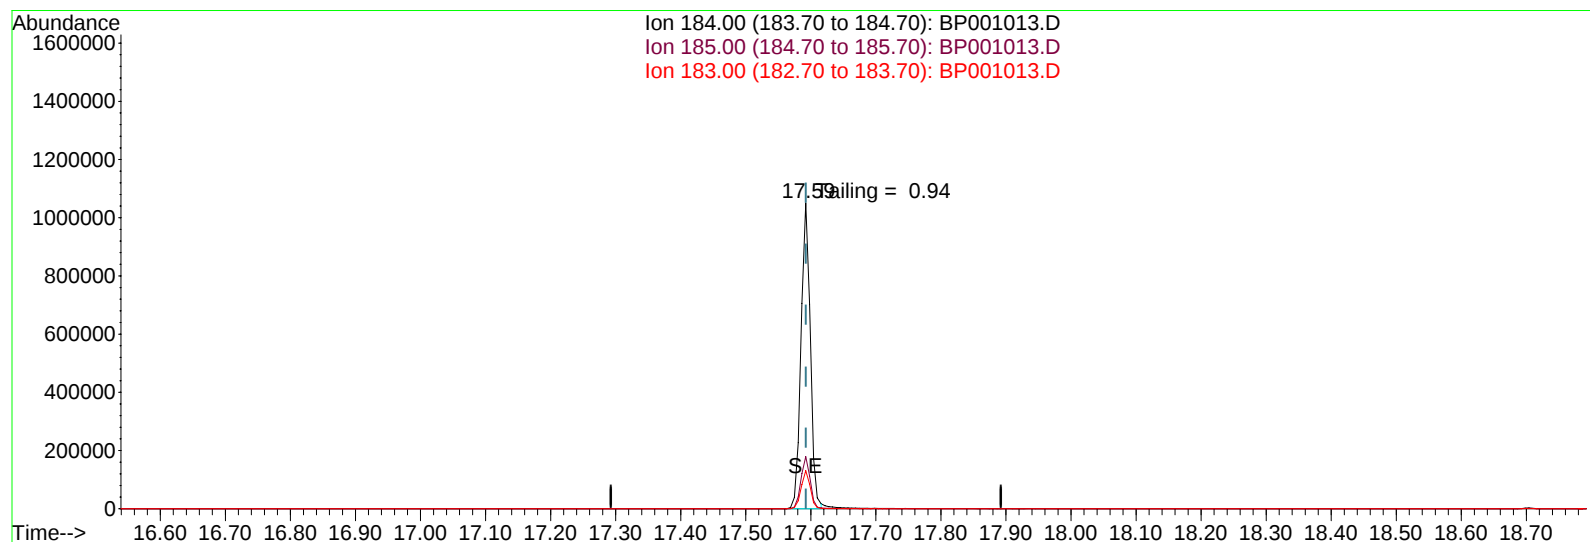

(77) Benzidine

17.592min (-0.000) 2894385.00ng

response 1065884

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	17.04
183.00	12.20	12.45
0.00	0.00	0.00