


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP110819\
 Data File : BP001006.D
 Acq On : 08 Nov 2019 08:17
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 06 17:07:13 2019

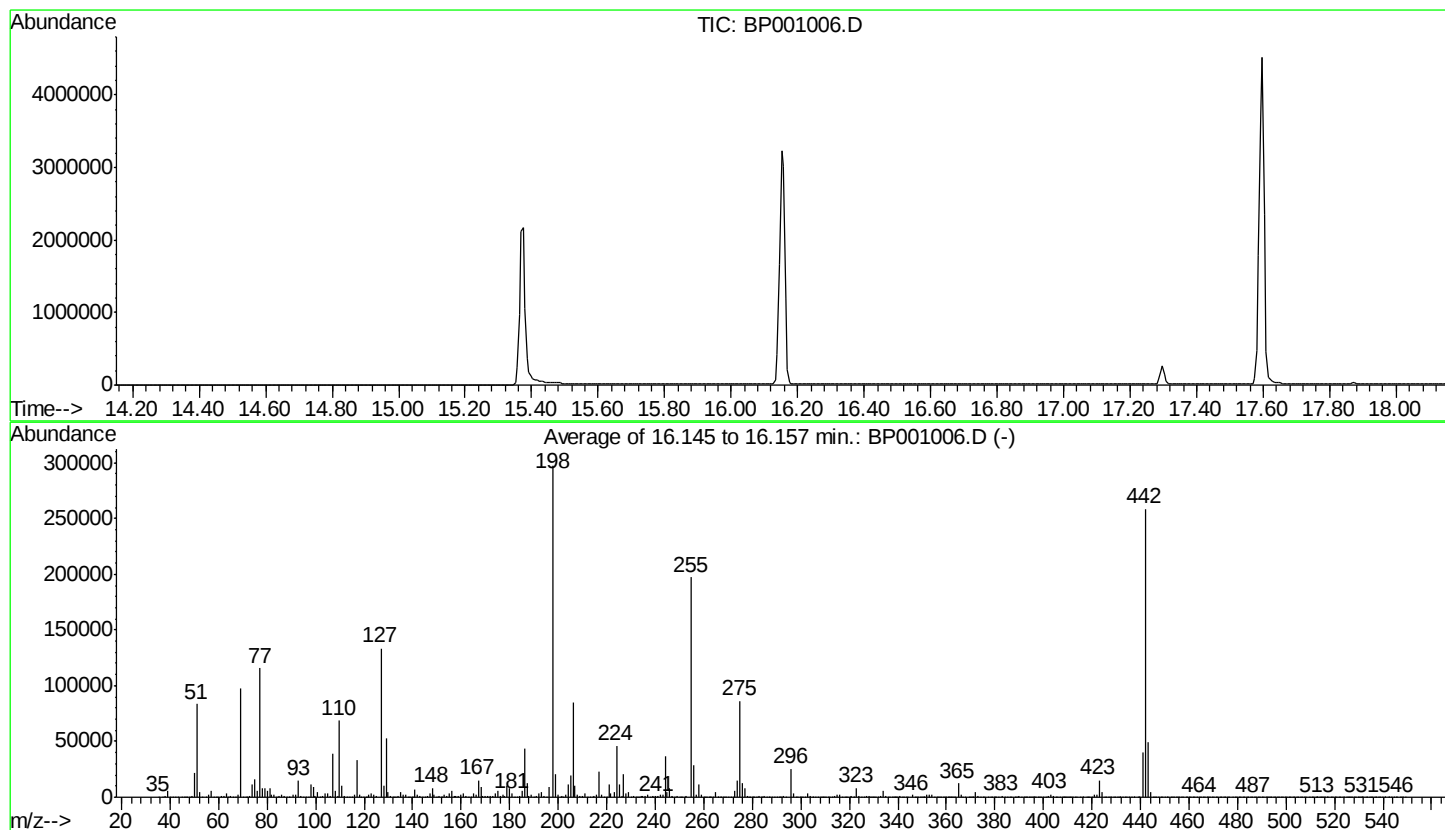

AutoFind: Scans 2390, 2391, 2392; Background Corrected with Scan 2381

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.0	83310	PASS
68	69	0.00	2	2.0	1948	PASS
69	198	0.00	100	32.7	97237	PASS
70	69	0.00	2	0.6	589	PASS
127	198	10	80	44.8	133298	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	297375	PASS
199	198	5	9	6.8	20282	PASS
275	198	10	60	29.2	86709	PASS
365	198	1	100	4.1	12242	PASS
441	198	0.01	100	13.6	40541	PASS
442	198	50	100	86.9	258400	PASS
443	442	15	24	19.0	49058	PASS