


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP110819\
Data File : BP001013.D
Acq On : 08 Nov 2019 13:34
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110619.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 06 17:07:13 2019

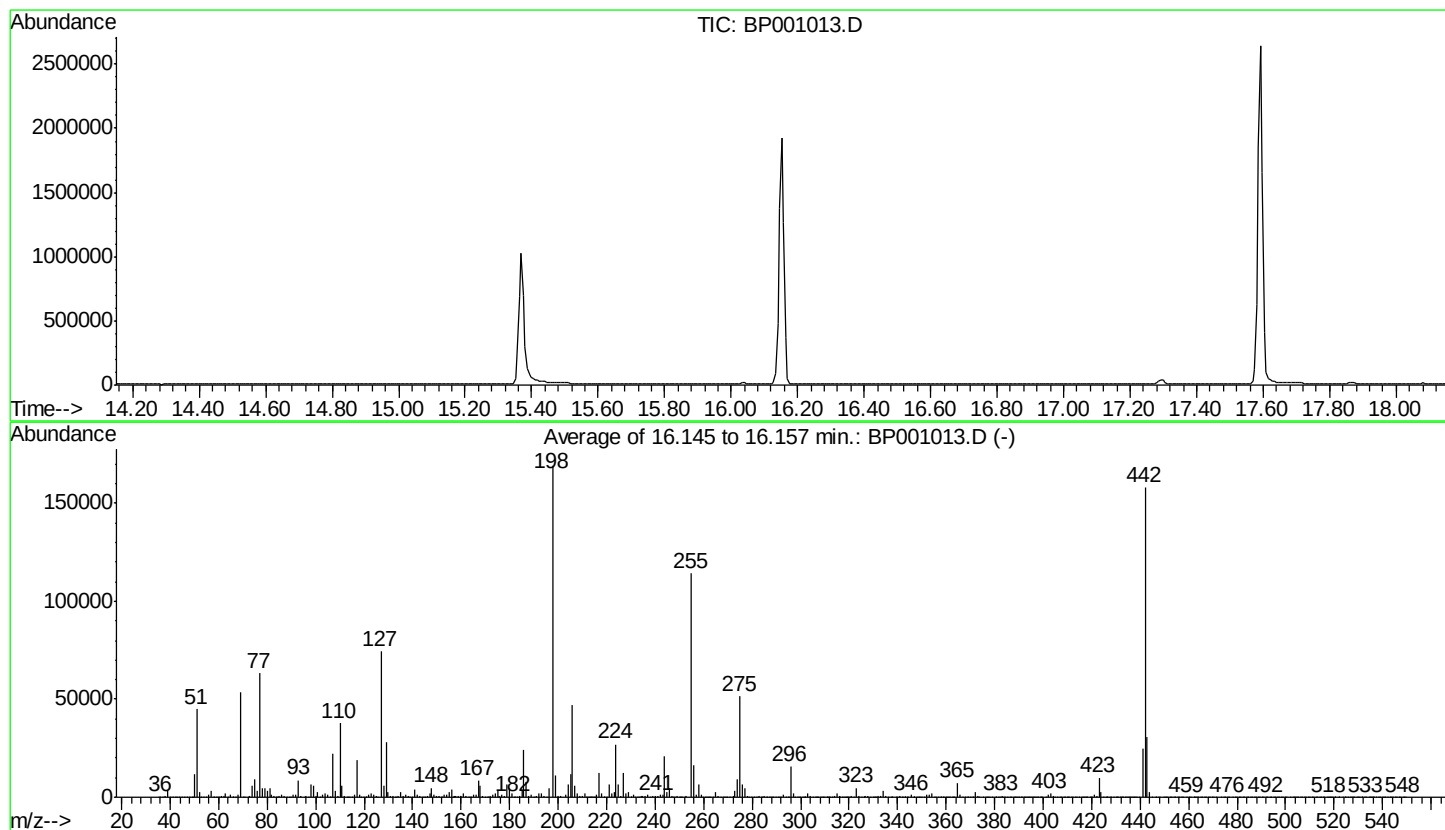

AutoFind: Scans 2390, 2391, 2392; Background Corrected with Scan 2382

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.6	44972	PASS
68	69	0.00	2	1.9	1036	PASS
69	198	0.00	100	31.5	53377	PASS
70	69	0.00	2	0.6	339	PASS
127	198	10	80	43.9	74344	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	169229	PASS
199	198	5	9	6.7	11357	PASS
275	198	10	60	30.4	51524	PASS
365	198	1	100	4.4	7494	PASS
441	198	0.01	100	14.8	25013	PASS
442	198	50	100	93.4	158042	PASS
443	442	15	24	19.3	30458	PASS