

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110821\
 Data File : BP007863.D
 Acq On : 08 Nov 2021 16:23
 Operator : CG/JU
 Sample : PB140492BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB140492BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007863.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.452	361	368	379	rBV	2820201	4189811	31.97%	8.384%
2	7.046	631	639	655	rBV	2736013	4366494	33.32%	8.738%
3	7.869	772	779	788	rBV	517534	819727	6.26%	1.640%
4	9.028	967	976	987	rBV	1563246	2596968	19.82%	5.197%
5	10.669	1247	1255	1265	rBV	688312	1174771	8.96%	2.351%
6	13.128	1664	1673	1689	rBV	4588074	6694290	51.08%	13.396%
7	14.504	1900	1907	1921	rBV	1229601	1785443	13.62%	3.573%
8	15.998	2153	2161	2174	rBV	4120981	5977243	45.61%	11.961%
9	17.257	2369	2375	2385	rBV	1753445	2409352	18.39%	4.821%
10	19.822	2805	2811	2816	rBV	10689684	13104450	100.00%	26.223%
11	21.345	3065	3070	3082	rBV	2452821	3265526	24.92%	6.535%
12	23.763	3474	3481	3490	rVB2	1770211	3589399	27.39%	7.183%




Sum of corrected areas: 49973474

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110821\
Data File : BP007863.D
Acq On : 08 Nov 2021 16:23
Operator : CG/JU
Sample : PB140492BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140492BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

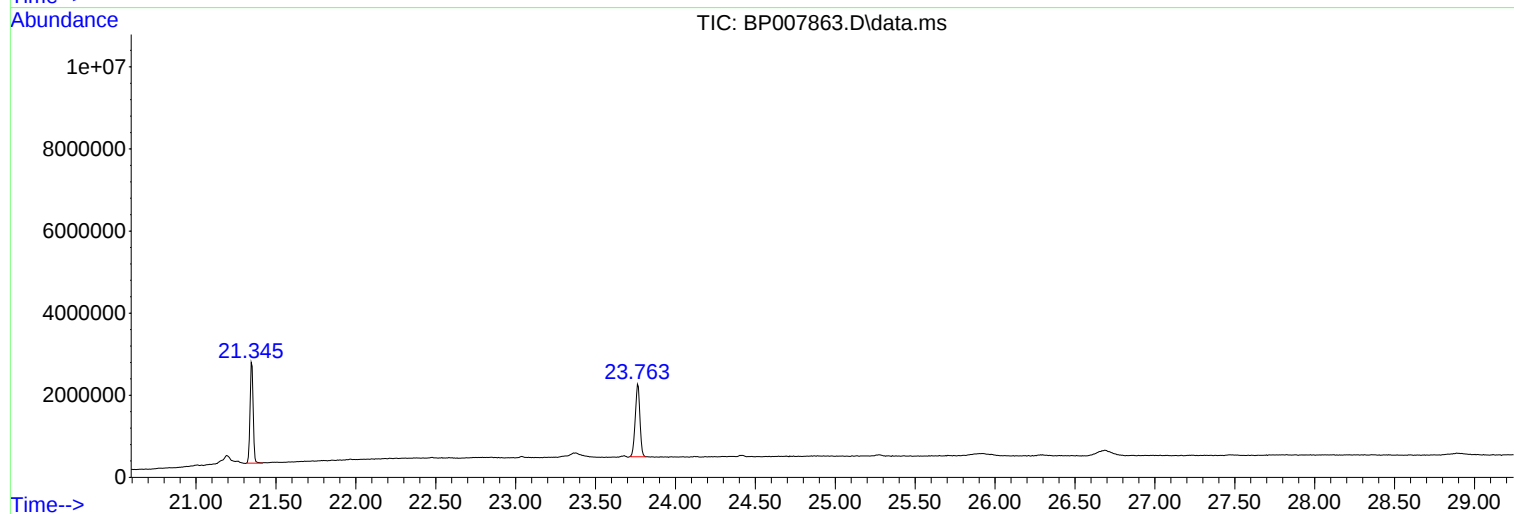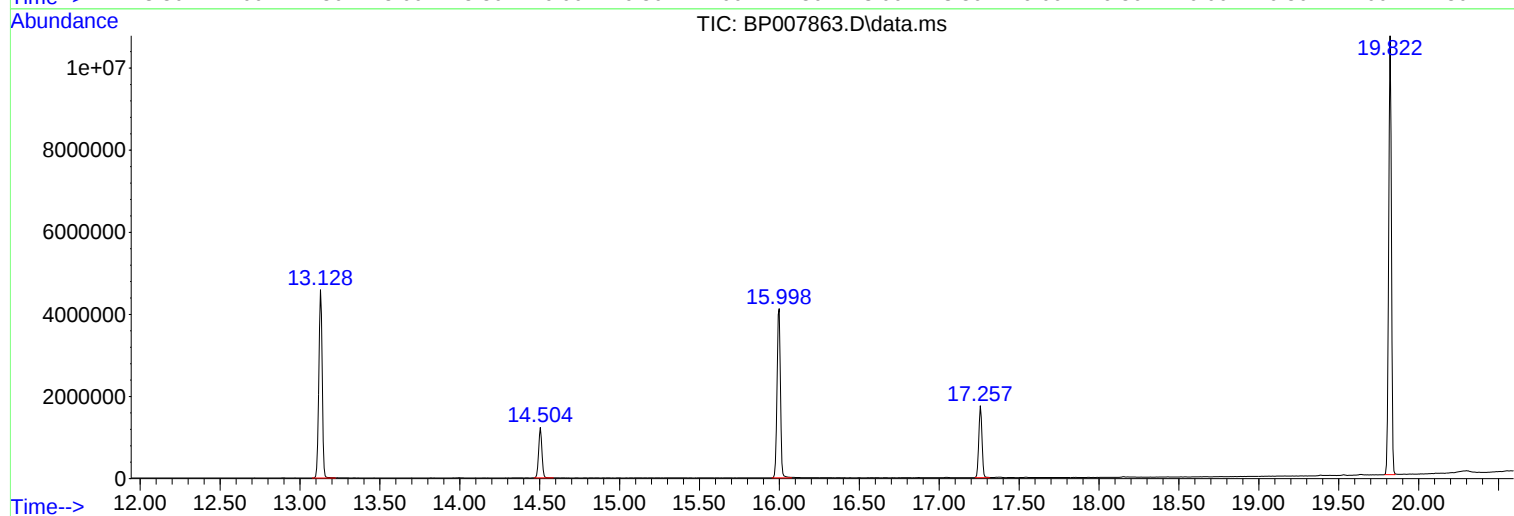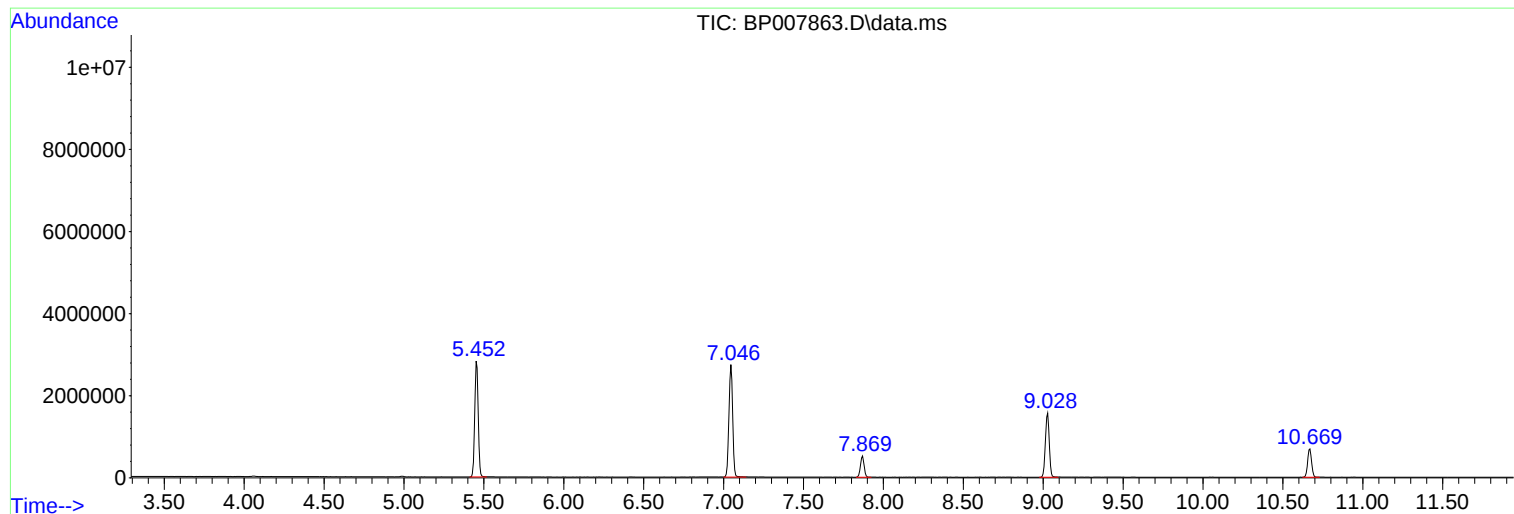

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110821\
Data File : BP007863.D
Acq On : 08 Nov 2021 16:23
Operator : CG/JU
Sample : PB140492BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140492BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110821\
Data File : BP007863.D
Acq On : 08 Nov 2021 16:23
Operator : CG/JU
Sample : PB140492BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140492BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------