

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110821\
 Data File : BP007881.D
 Acq On : 09 Nov 2021 02:36
 Operator : CG/JU
 Sample : M4556-01 2X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 OR-02-110521

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007881.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.446	360	367	380	rBV	866568	1230040	42.90%	5.090%
2	7.034	631	637	646	rBV	802711	1262453	44.03%	5.224%
3	7.858	771	777	786	rBV	484917	763208	26.62%	3.158%
4	9.016	967	974	985	rVB	432064	725855	25.32%	3.003%
5	10.446	1208	1217	1227	rBV	71005	128602	4.49%	0.532%
6	10.657	1242	1253	1260	rBV	640931	1085600	37.86%	4.492%
7	13.122	1664	1672	1682	rBV	1201557	1778914	62.05%	7.361%
8	14.216	1852	1858	1866	rBV	51959	88152	3.07%	0.365%
9	14.498	1898	1906	1912	rBV	1013489	1486487	51.85%	6.151%
10	14.557	1912	1916	1925	rVB	25991	46726	1.63%	0.193%
11	14.898	1967	1974	1982	rVB2	16730	34447	1.20%	0.143%
12	15.110	2004	2010	2017	rBV10	11177	33813	1.18%	0.140%
13	15.363	2049	2053	2058	rVB3	25255	34153	1.19%	0.141%
14	15.545	2080	2084	2096	rVB	36374	67114	2.34%	0.278%
15	15.987	2153	2159	2169	rBV	1042962	1513534	52.79%	6.263%
16	16.222	2195	2199	2208	rBV2	36091	68056	2.37%	0.282%
17	17.069	2340	2343	2352	rVB2	24127	43884	1.53%	0.182%
18	17.251	2368	2374	2378	rBV	1311276	1850033	64.53%	7.655%
19	17.292	2378	2381	2387	rVB	244189	330340	11.52%	1.367%
20	17.381	2392	2396	2402	rVV	108383	165437	5.77%	0.685%
21	17.445	2403	2407	2413	rVB4	17332	31862	1.11%	0.132%
22	18.122	2518	2522	2525	rBV	61542	90642	3.16%	0.375%
23	18.169	2526	2530	2535	rVB	78887	107468	3.75%	0.445%
24	18.245	2539	2543	2548	rBV2	39609	57268	2.00%	0.237%
25	18.310	2549	2554	2557	rBV2	111427	189216	6.60%	0.783%
26	18.604	2601	2604	2607	rVB	33731	37887	1.32%	0.157%
27	19.010	2669	2673	2676	rBV2	67770	112500	3.92%	0.465%
28	19.063	2680	2682	2686	rVB3	55833	70591	2.46%	0.292%
29	19.263	2711	2716	2721	rBV	676667	872660	30.44%	3.611%
30	19.616	2767	2776	2784	rBV	682317	1144253	39.91%	4.735%
31	19.810	2804	2809	2814	rBV	2228042	2867128	100.00%	11.863%
32	20.098	2855	2858	2862	rVB2	117677	139257	4.86%	0.576%
33	20.198	2872	2875	2878	rVB2	81771	95151	3.32%	0.394%
34	20.251	2882	2884	2888	rVB	80864	95891	3.34%	0.397%
35	21.339	3063	3069	3073	rBV2	1901907	2837838	98.98%	11.742%
36	21.380	3073	3076	3085	rVB	315468	416998	14.54%	1.725%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110821\
Data File : BP007881.D
Acq On : 09 Nov 2021 02:36
Operator : CG/JU
Sample : M4556-01 2X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OR-02-110521

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	23.757	3474	3480	3486	rBV2 1203504	2264282	78.97%	9.369%
----	--------	------	------	------	--------------	---------	--------	--------




Sum of corrected areas: 24167740

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110821\
Data File : BP007881.D
Acq On : 09 Nov 2021 02:36
Operator : CG/JU
Sample : M4556-01 2X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OR-02-110521

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

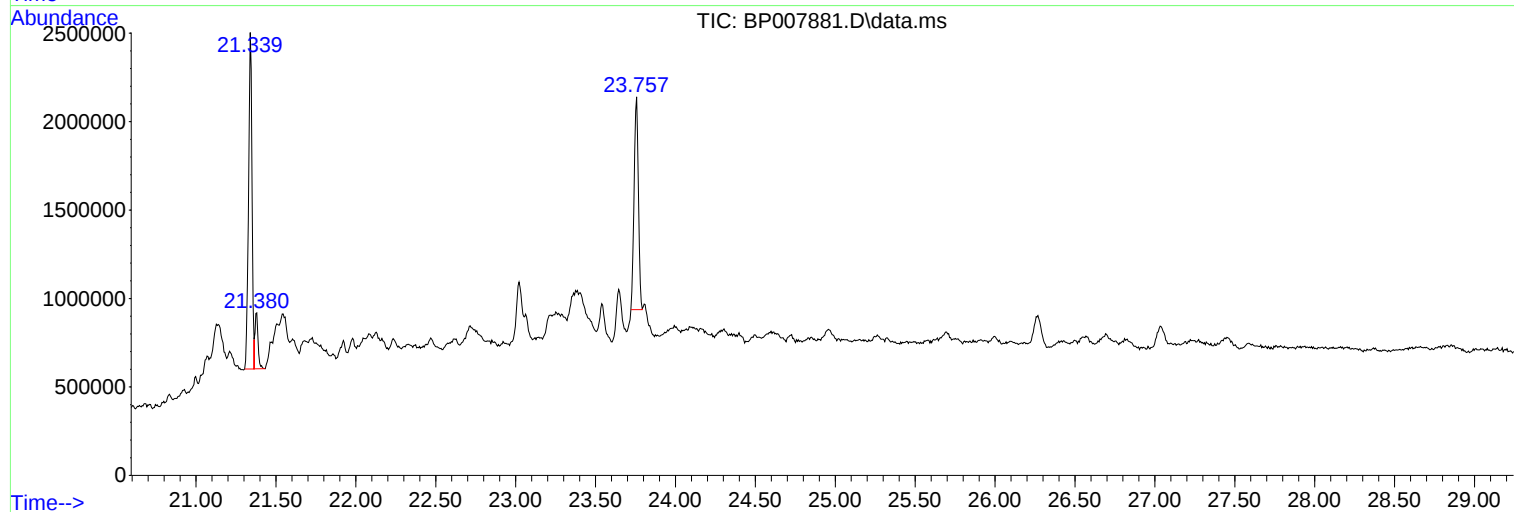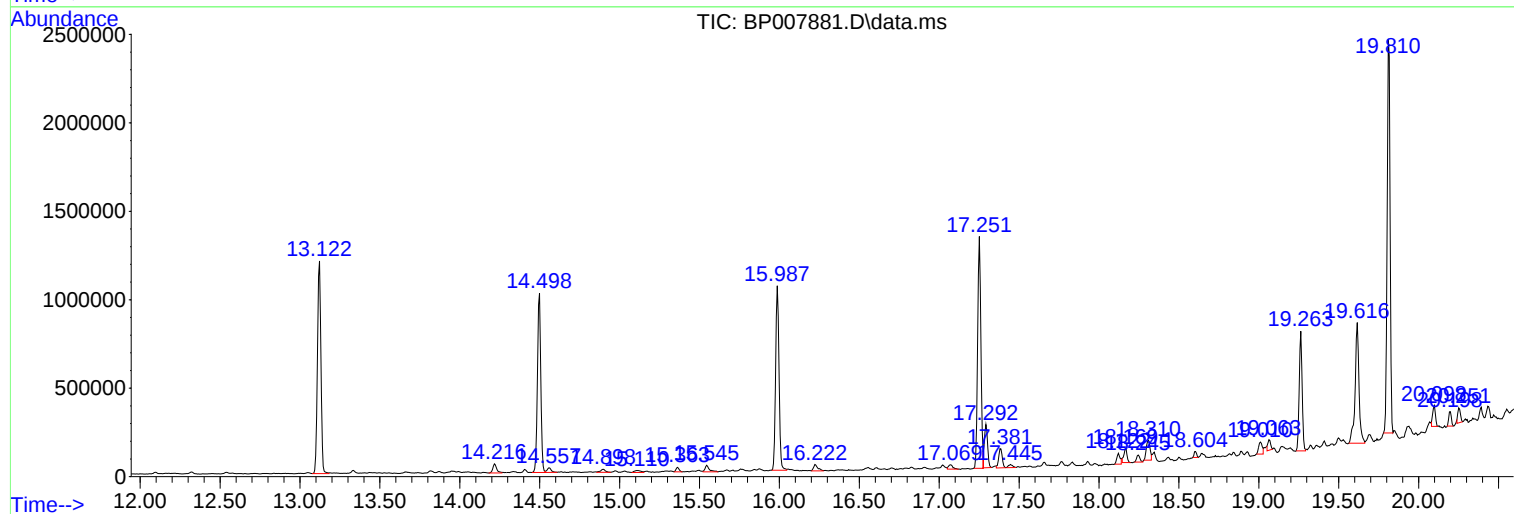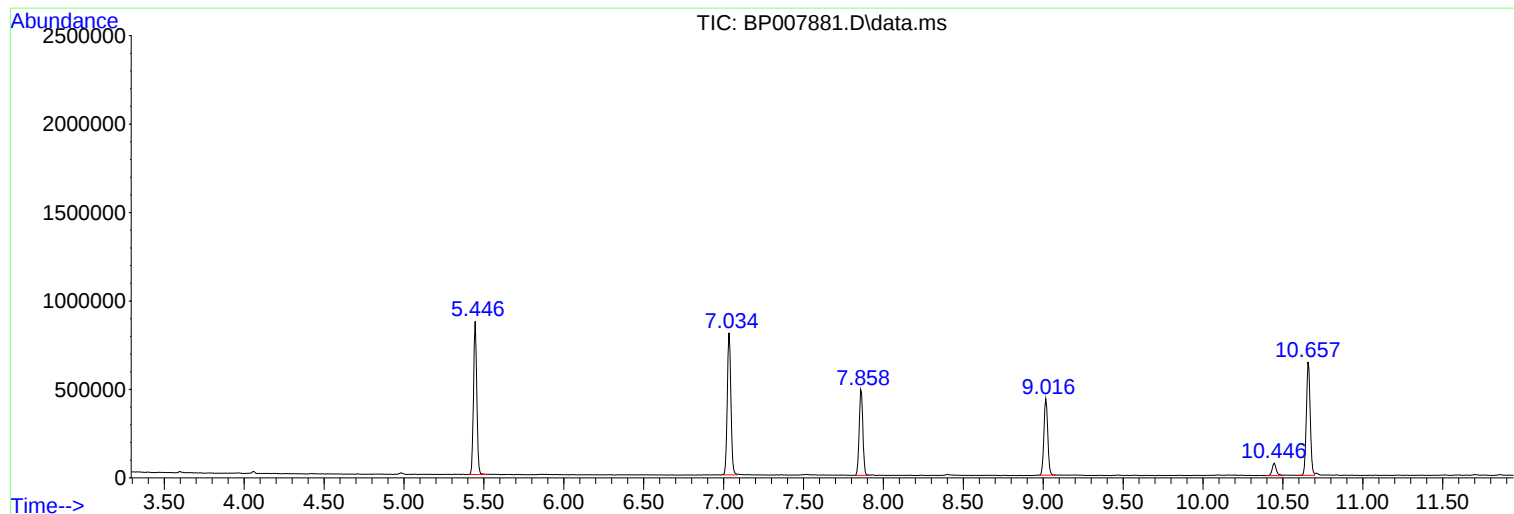

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110821\
Data File : BP007881.D
Acq On : 09 Nov 2021 02:36
Operator : CG/JU
Sample : M4556-01 2X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OR-02-110521

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110821\
Data File : BP007881.D
Acq On : 09 Nov 2021 02:36
Operator : CG/JU
Sample : M4556-01 2X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OR-02-110521

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------