
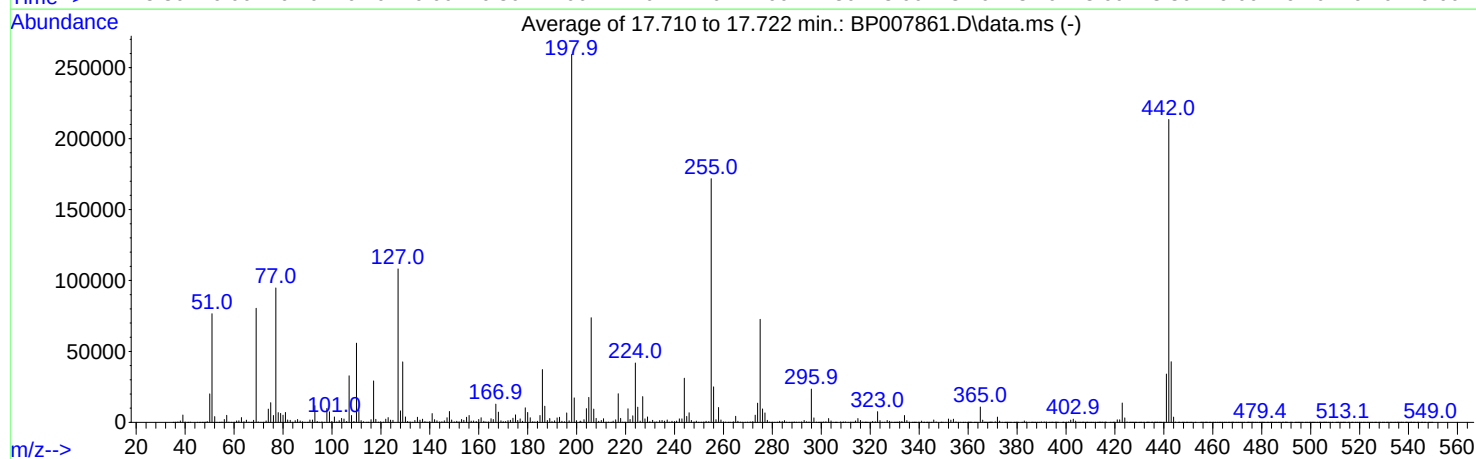


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110821\
 Data File : BP007861.D
 Acq On : 08 Nov 2021 15:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 09 10:45:24 2021

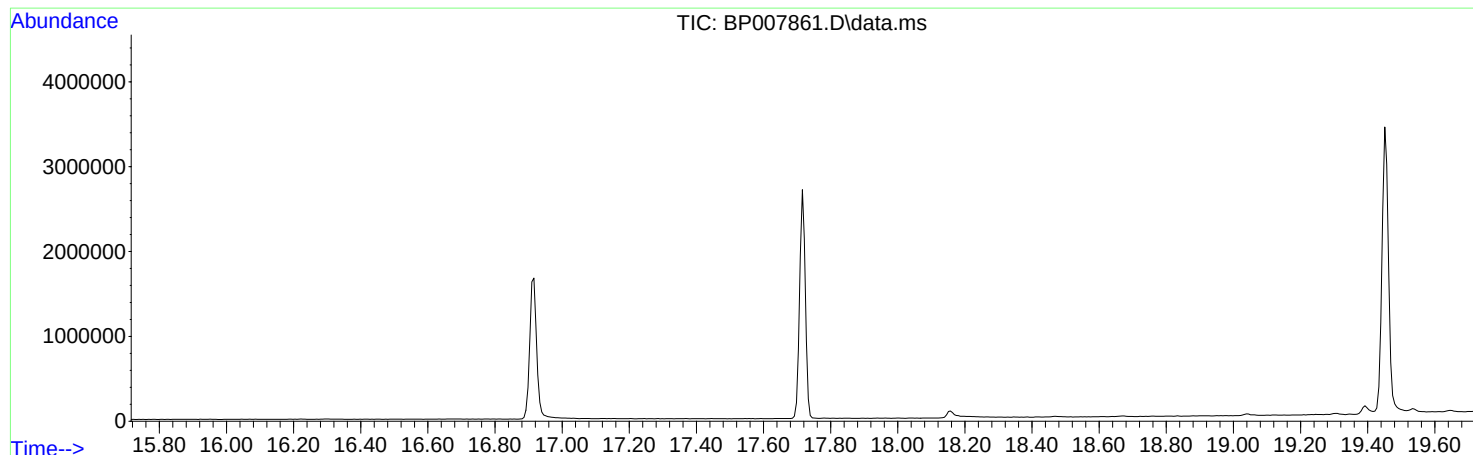




AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2443

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.5	76622	PASS
68	69	0.00	2	1.8	1473	PASS
69	198	0.00	100	31.0	80384	PASS
70	69	0.00	2	0.5	372	PASS
127	198	10	80	41.7	108135	PASS
197	198	0.00	2	0.5	1170	PASS
198	198	100	100	100.0	259313	PASS
199	198	5	9	6.7	17267	PASS
275	198	10	60	28.0	72643	PASS
365	198	1	100	4.2	10883	PASS
441	198	0.01	100	13.1	34096	PASS
442	442	100	100	100.0	213477	PASS
443	442	15	24	20.0	42754	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110821\
 Data File : BP007861.D
 Acq On : 08 Nov 2021 15:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Nov 08 16:32:16 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 08 16:32:09 2021
 Response via : Initial Calibration

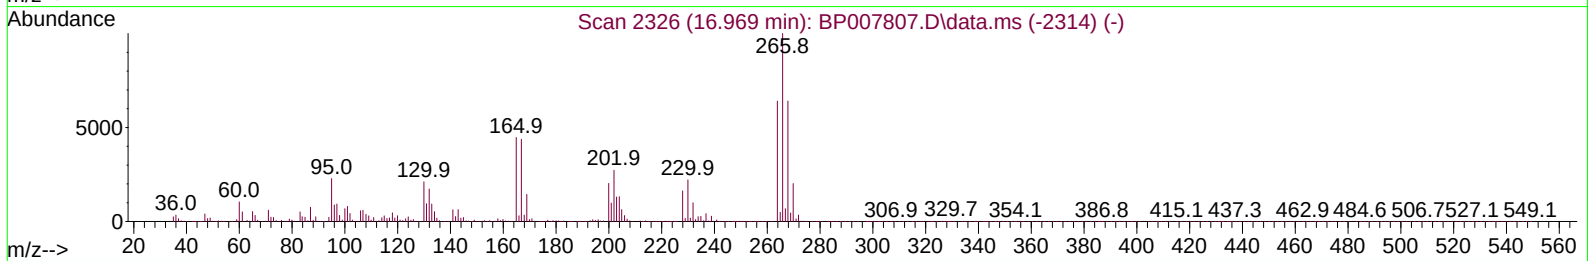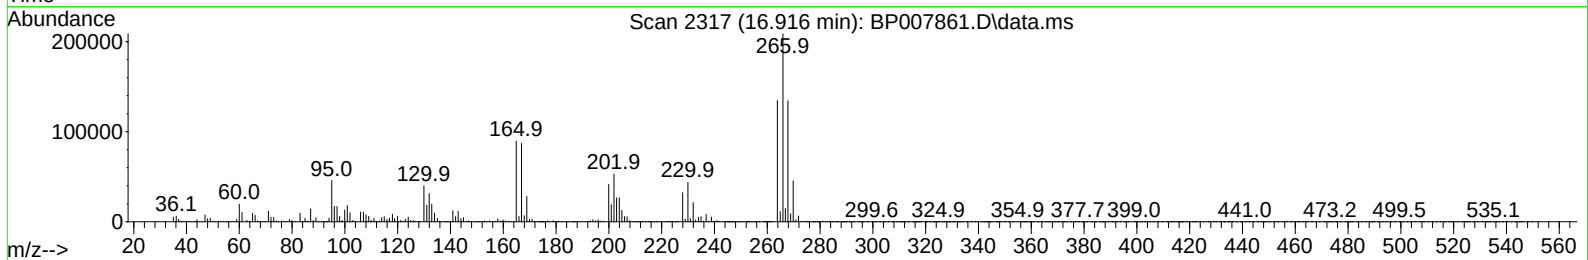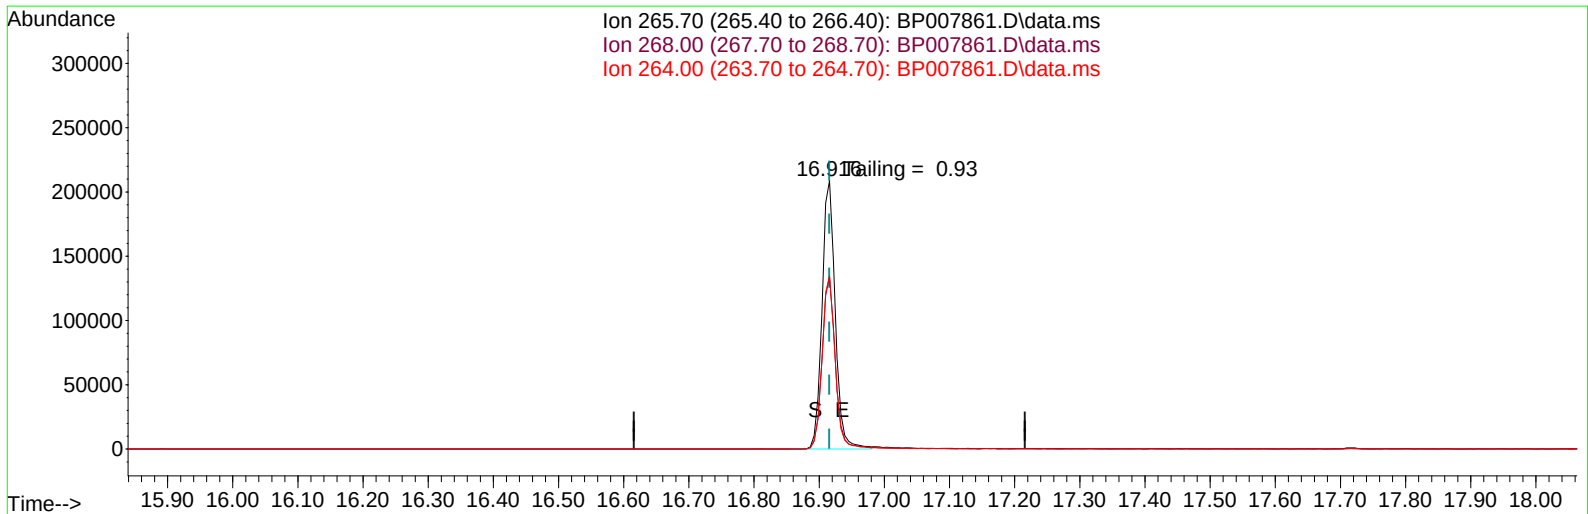

TIC: BP007861.D\data.ms

(70) Pentachlorophenol (C)

16.916min (0.000) 820221.20 ng




response 299773

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.60	64.33
264.00	60.90	64.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110821\
 Data File : BP007861.D
 Acq On : 08 Nov 2021 15:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Nov 08 16:32:16 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 08 16:32:09 2021
 Response via : Initial Calibration

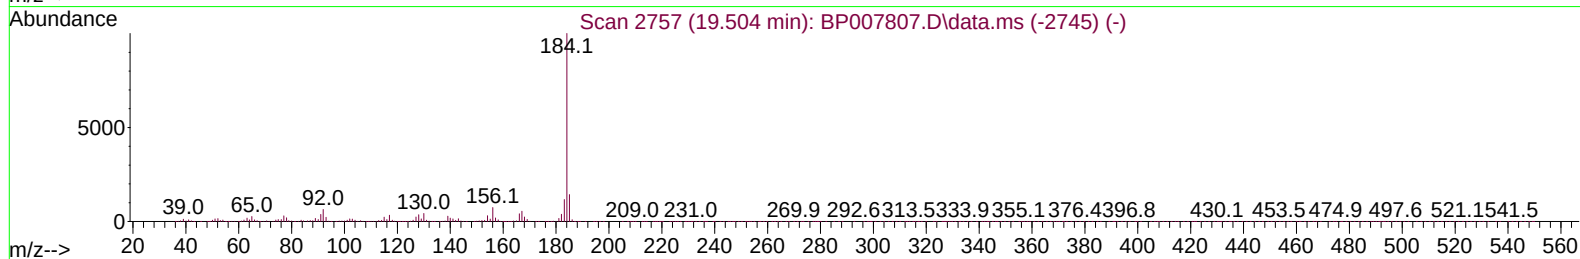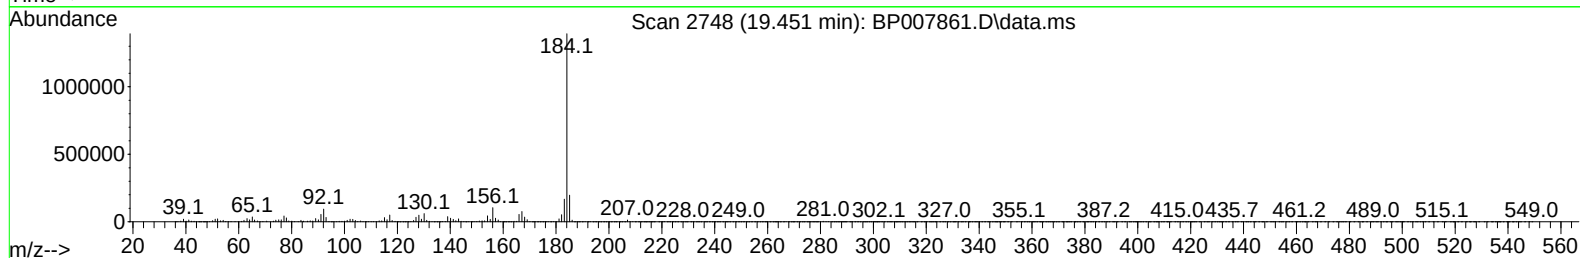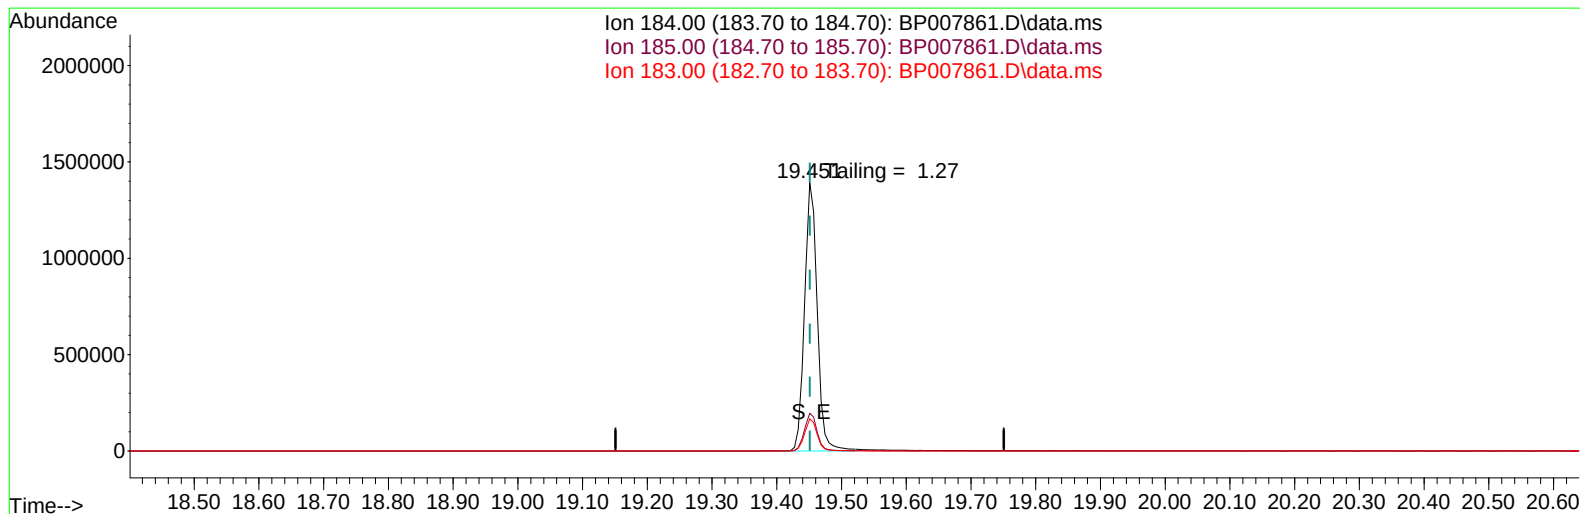

TIC: BP007861.D\data.ms

(77) Benzidine

19.451min (0.000) 231090.91 ng

response 1921974

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.09
183.00	11.40	12.02
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/4/2021	BNA_P	<u>BP007861.D</u>
Compound Name	Response	Retention Time
DDT	1034810	20.66
DDD	32192	20.22
DDE	2013	19.74
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
34205	1069015	3.20

Instrument :
BNA_P
ClientSampleId :
DFTPP