

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
 Data File : BP017994.D
 Acq On : 09 Nov 2023 18:24
 Operator : MA/JU
 Sample : PB156741BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK741

Quant Time: Nov 09 23:16:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 09 22:34:38 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.869	152	64065	20.000	ng/ul	0.00
20) Naphthalene-d8	10.687	136	256089	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.539	164	161280	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.322	188	371596	20.000	ng/ul	0.00
79) Chrysene-d12	21.451	240	364544	20.000	ng/ul	0.00
88) Perylene-d12	23.957	264	424040	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.246	96	10101	5.397	ng/uL	0.00
4) Pyridine-d5	3.681	84	126754	26.059	ng/ul	0.00
7) Phenol-d5	7.034	99	142211	23.621	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.216	67	93529	25.646	ng/ul	0.00
11) 2-Chlorophenol-d4	7.387	132	124009	25.743	ng/ul	0.00
15) 4-Methylphenol-d8	8.587	113	121162	25.091	ng/ul	0.00
21) Nitrobenzene-d5	9.075	128	59030	25.740	ng/ul	0.00
24) 2-Nitrophenol-d4	9.787	143	64275	25.183	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.316	165	100757	22.036	ng/ul	0.00
31) 4-Chloroaniline-d4	10.869	131	157447	25.128	ng/ul	0.00
46) Dimethylphthalate-d6	13.963	166	400303	27.000	ng/ul	0.00
49) Acenaphthylene-d8	14.239	160	421625	26.526	ng/ul	0.00
54) 4-Nitrophenol-d4	14.804	143	41742	19.223	ng/ul	0.00
60) Fluorene-d10	15.545	176	317223	25.814	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	57668	22.225	ng/ul	0.00
73) Anthracene-d10	17.422	188	523413	26.288	ng/ul	0.00
81) Pyrene-d10	19.674	212	651194	27.756	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.792	264	675923	27.424	ng/ul	0.00
Target Compounds						
59) Diethylphthalate	15.369	149	25239	1.049	ng/ul	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
Data File : BP017994.D
Acq On : 09 Nov 2023 18:24
Operator : MA/JU
Sample : PB156741BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK741

Quant Time: Nov 09 23:16:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 09 22:34:38 2023
Response via : Initial Calibration

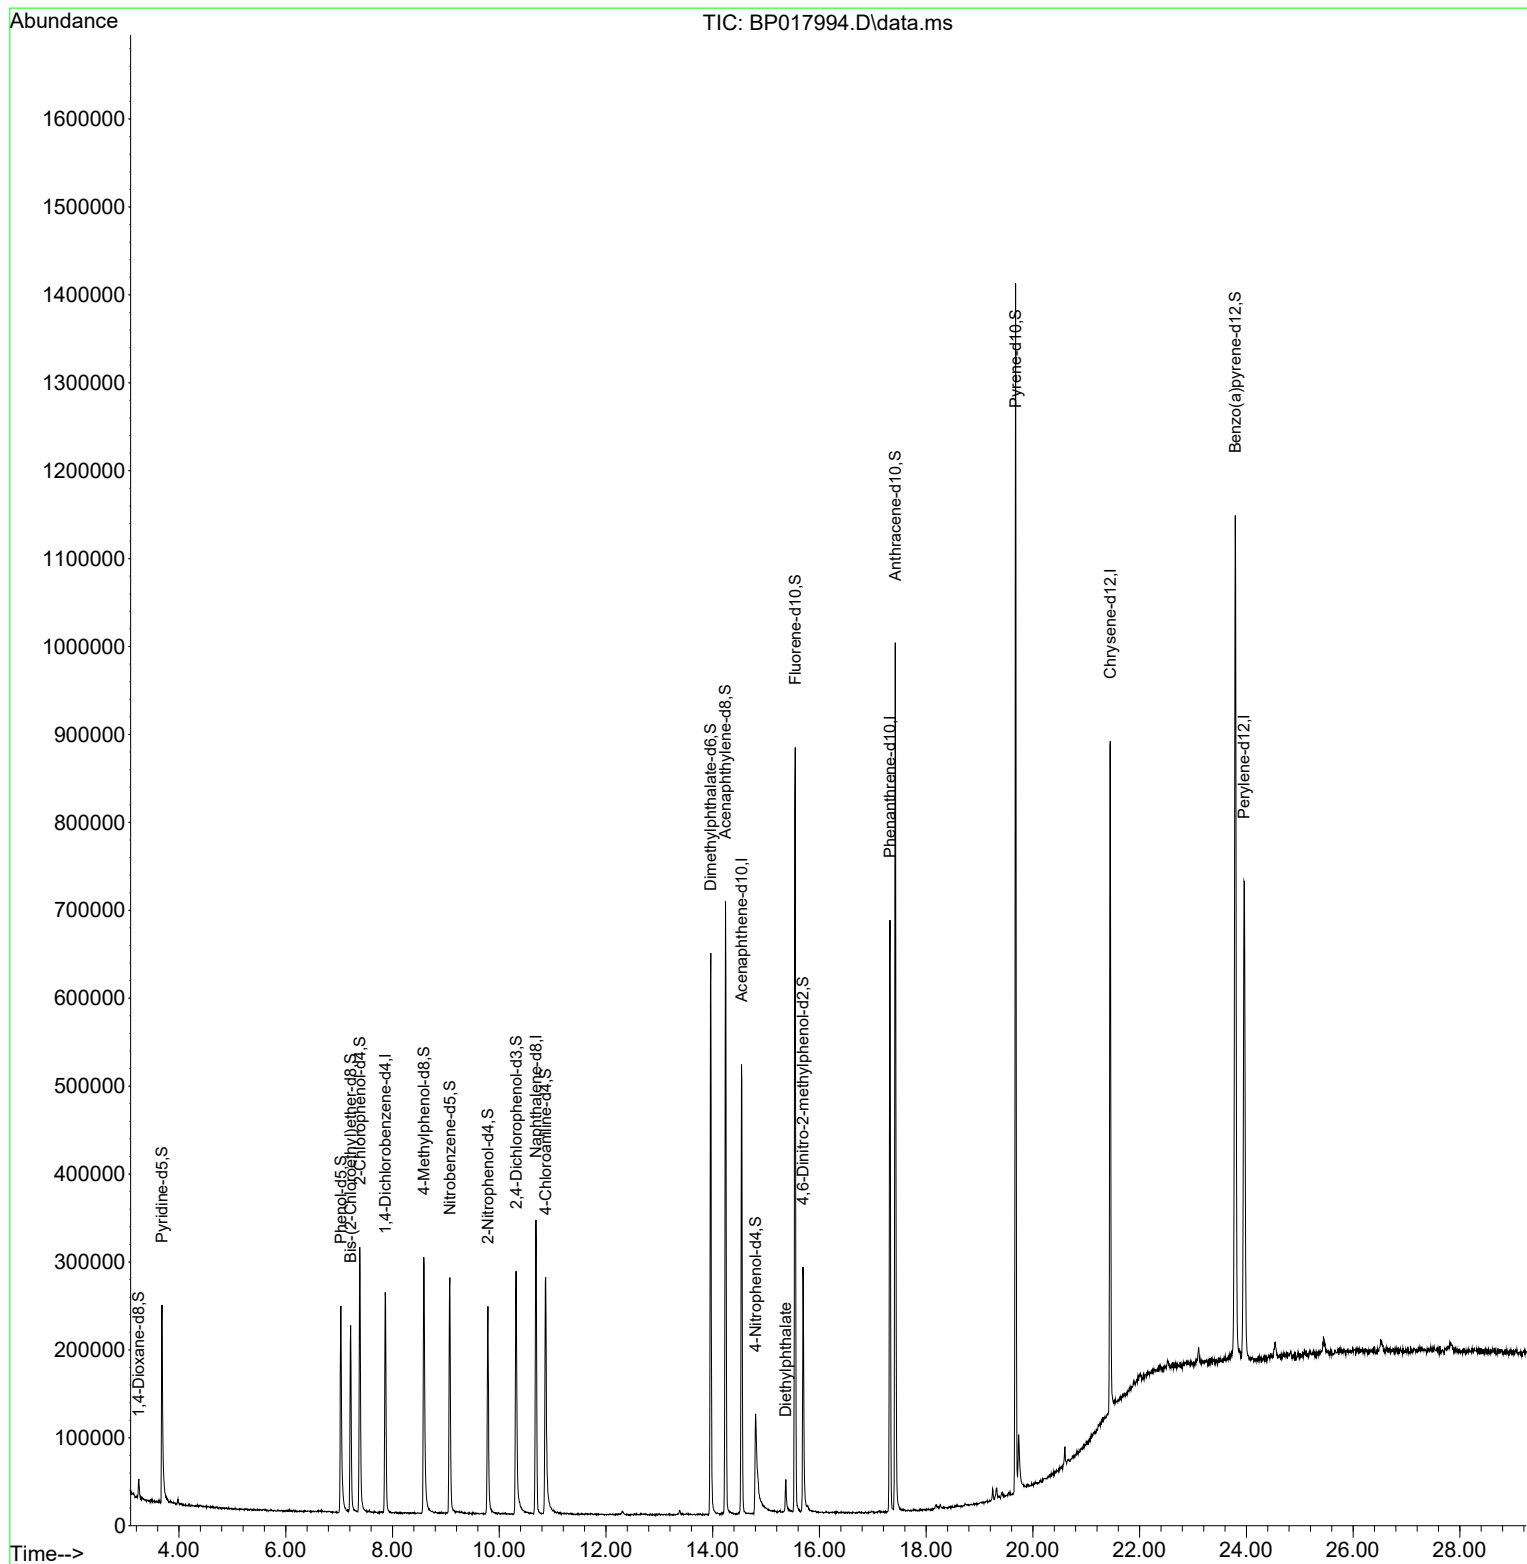

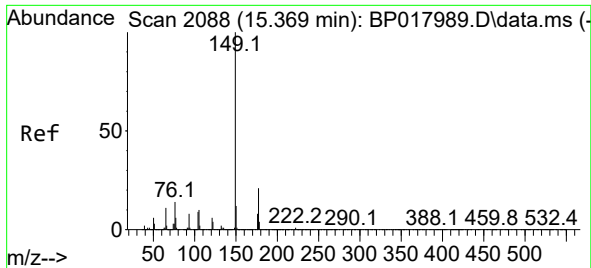

#59
Diethylphthalate
Concen: 1.049 ng/ul
RT: 15.369 min Scan# 2088
Delta R.T. -0.000 min
Lab File: BP017994.D
Acq: 09 Nov 2023 18:24

Instrument :
BNA_P
ClientSampleId :
SBLK741

Tgt Ion:149 Resp: 25239
Ion Ratio Lower Upper
149 100
177 17.1 16.7 25.1
150 11.6 9.9 14.9

