

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP110923\  
 Data File : BP018000.D  
 Acq On : 09 Nov 2023 21:49  
 Operator : MA/JU  
 Sample : 05082-08  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 BH329

Quant Time: Nov 09 23:18:38 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP110923.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Thu Nov 09 22:34:38 2023  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc   | Units | Dev(Min) |
|-------------------------------|--------|------|----------|--------|-------|----------|
| Internal Standards            |        |      |          |        |       |          |
| 1) 1,4-Dichlorobenzene-d4     | 7.869  | 152  | 50468    | 20.000 | ng/u1 | 0.00     |
| 20) Naphthalene-d8            | 10.687 | 136  | 207584   | 20.000 | ng/u1 | 0.00     |
| 38) Acenaphthene-d10          | 14.540 | 164  | 133614   | 20.000 | ng/u1 | 0.00     |
| 64) Phenanthrene-d10          | 17.316 | 188  | 312080   | 20.000 | ng/u1 | 0.00     |
| 79) Chrysene-d12              | 21.445 | 240  | 315384   | 20.000 | ng/u1 | 0.00     |
| 88) Perylene-d12              | 23.957 | 264  | 368513   | 20.000 | ng/u1 | -0.01    |
| System Monitoring Compounds   |        |      |          |        |       |          |
| 3) 1,4-Dioxane-d8             | 3.246  | 96   | 5589     | 3.791  | ng/uL | 0.00     |
| 4) Pyridine-d5                | 3.687  | 84   | 45065    | 11.761 | ng/u1 | 0.00     |
| 7) Phenol-d5                  | 7.040  | 99   | 33281    | 7.017  | ng/u1 | 0.00     |
| 9) Bis-(2-Chloroethyl)eth...  | 7.216  | 67   | 96038    | 33.428 | ng/u1 | 0.00     |
| 11) 2-Chlorophenol-d4         | 7.387  | 132  | 95287    | 25.110 | ng/u1 | 0.00     |
| 15) 4-Methylphenol-d8         | 8.593  | 113  | 63073    | 16.581 | ng/u1 | 0.00     |
| 21) Nitrobenzene-d5           | 9.069  | 128  | 60483    | 32.536 | ng/u1 | 0.00     |
| 24) 2-Nitrophenol-d4          | 9.787  | 143  | 66430    | 32.109 | ng/u1 | 0.00     |
| 28) 2,4-Dichlorophenol-d3     | 10.310 | 165  | 109450   | 29.531 | ng/u1 | 0.00     |
| 31) 4-Chloroaniline-d4        | 10.863 | 131  | 154888   | 30.496 | ng/u1 | 0.00     |
| 46) Dimethylphthalate-d6      | 13.963 | 166  | 173132   | 14.096 | ng/u1 | 0.00     |
| 49) Acenaphthylene-d8         | 14.240 | 160  | 440869   | 33.480 | ng/u1 | 0.00     |
| 54) 4-Nitrophenol-d4          | 14.781 | 143  | 44       | 0.024  | ng/u1 | -0.02    |
| 60) Fluorene-d10              | 15.540 | 176  | 358440   | 35.208 | ng/u1 | 0.00     |
| 65) 4,6-Dinitro-2-methylph... | 15.692 | 200  | 66720    | 30.618 | ng/u1 | 0.00     |
| 73) Anthracene-d10            | 17.422 | 188  | 621990   | 37.196 | ng/u1 | 0.00     |
| 81) Pyrene-d10                | 19.669 | 212  | 790114   | 38.926 | ng/u1 | 0.00     |
| 92) Benzo(a)pyrene-d12        | 23.792 | 264  | 815457   | 38.070 | ng/u1 | 0.00     |
| Target Compounds              |        |      |          |        |       |          |
| 2) 1,4-Dioxane                | 3.275  | 88   | 32989    | 19.859 | ng/uL | 99       |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP110923\  
Data File : BP018000.D  
Acq On : 09 Nov 2023 21:49  
Operator : MA/JU  
Sample : 05082-08  
Misc :  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
BH329

Quant Time: Nov 09 23:18:38 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP110923.MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Thu Nov 09 22:34:38 2023  
Response via : Initial Calibration

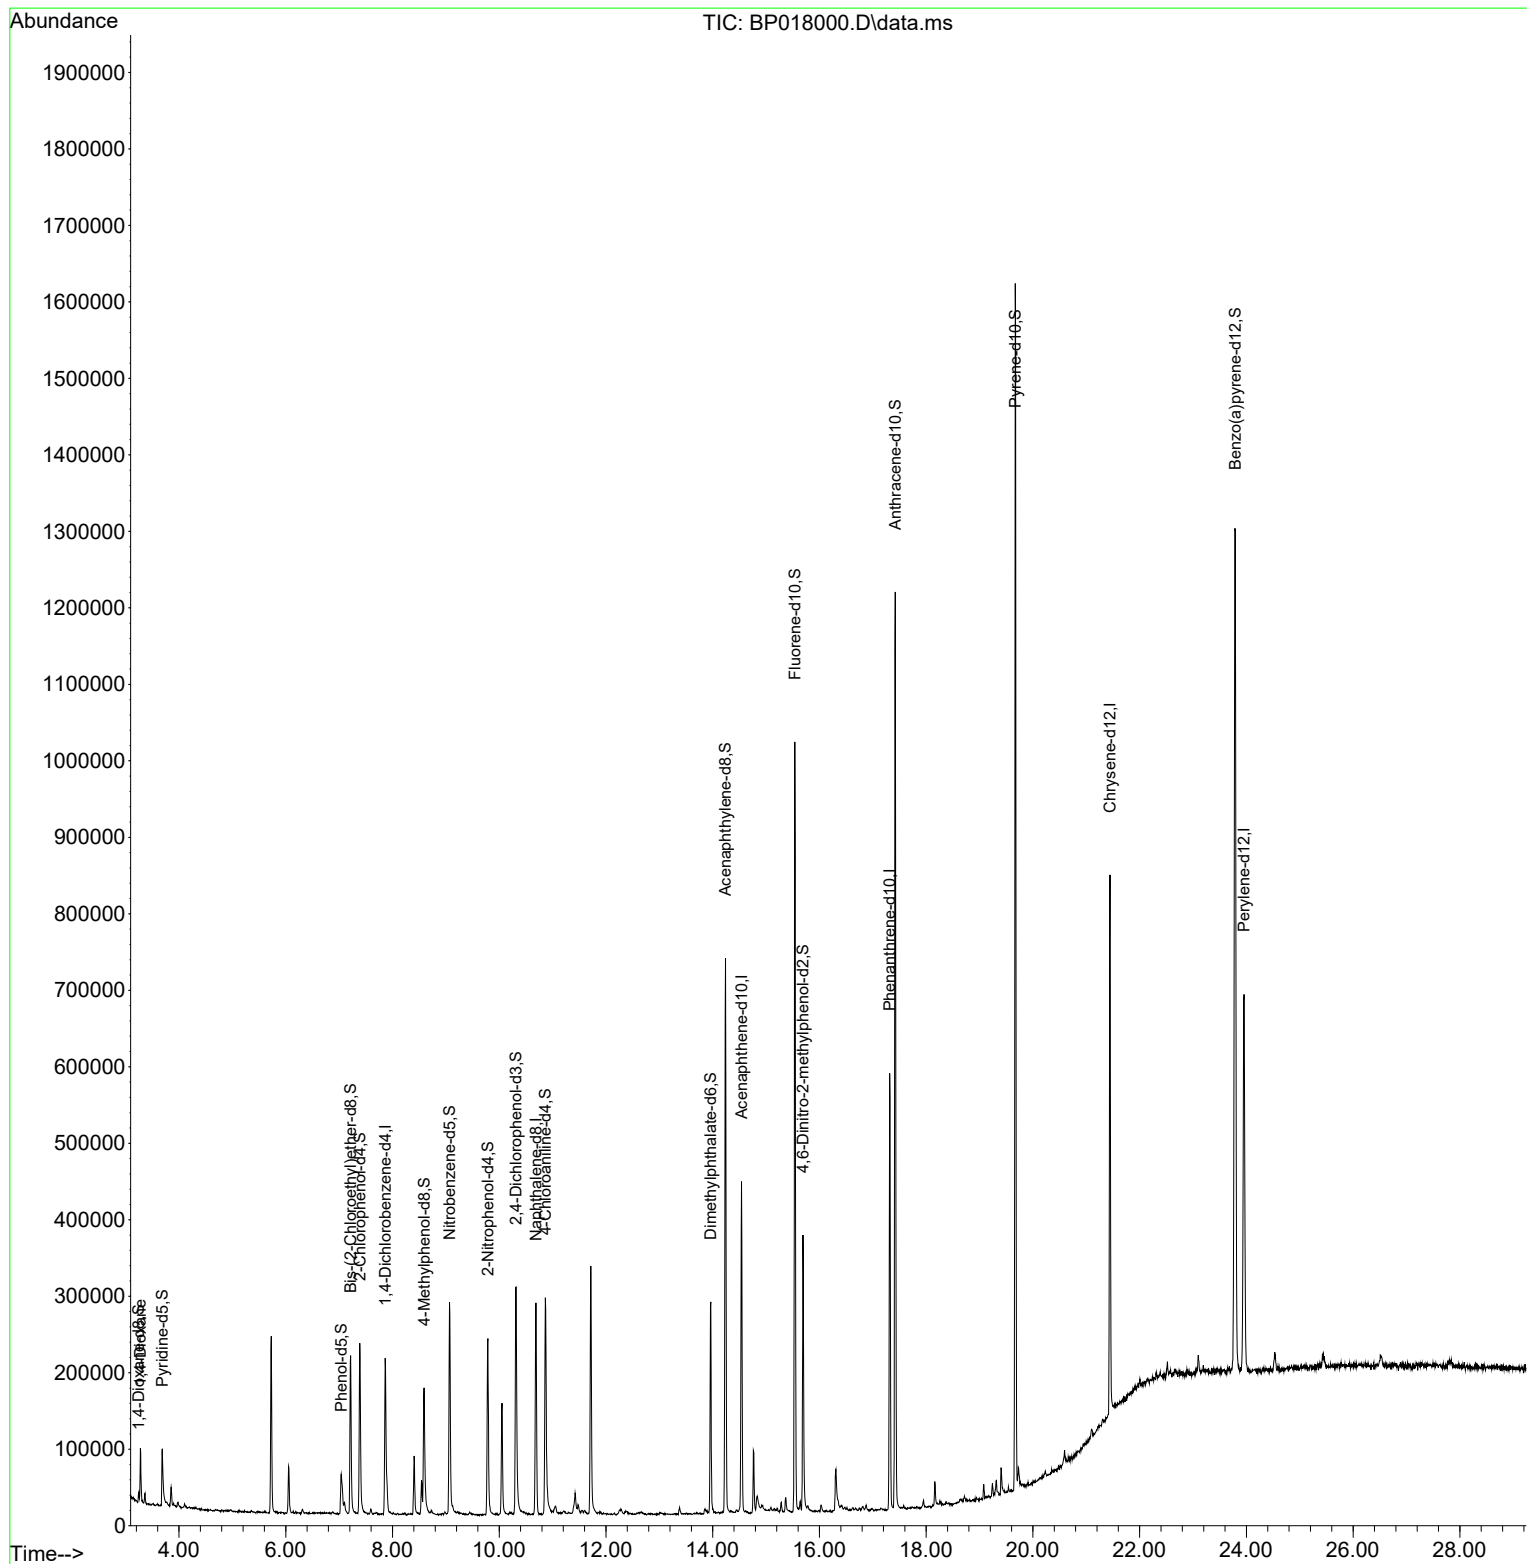

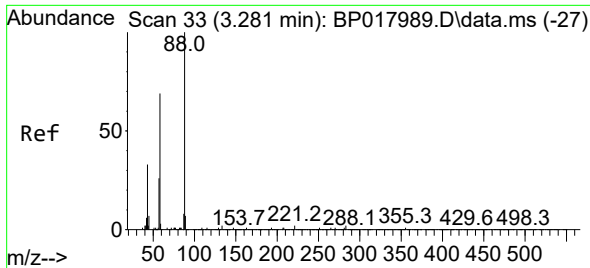

#2  
 1,4-Dioxane  
 Concen: 19.859 ng/uL  
 RT: 3.275 min Scan# 31  
 Delta R.T. -0.006 min  
 Lab File: BP018000.D  
 Acq: 09 Nov 2023 21:49

Instrument :  
 BNA\_P  
 ClientSampleId :  
 BH329

Tgt Ion: 88 Resp: 32989  
 Ion Ratio Lower Upper  
 88 100  
 43 33.3 26.3 39.5  
 58 68.5 54.0 81.0

